

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020171.D
 Acq On : 15 Jun 2022 12:51
 Operator : CG/JU
 Sample : N3317-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.005	152	156	163	rVB5	6278	11479	0.52%	0.120%
2	7.799	794	801	816	rBV	354977	628069	28.28%	6.558%
3	10.587	1267	1275	1288	rBV	572225	1005582	45.28%	10.500%
4	12.910	1667	1670	1680	rVB5	999	2354	0.11%	0.025%
5	14.428	1921	1928	1946	rBV	1015092	1559691	70.24%	16.287%
6	15.445	2096	2101	2109	rBV5	2691	6664	0.30%	0.070%
7	16.151	2215	2221	2224	rBV5	4538	8679	0.39%	0.091%
8	16.181	2224	2226	2233	rVB7	2775	4887	0.22%	0.051%
9	16.498	2275	2280	2282	rBV5	4099	6663	0.30%	0.070%
10	16.557	2287	2290	2297	rBV7	3105	5112	0.23%	0.053%
11	16.616	2297	2300	2303	rVB2	2117	2751	0.12%	0.029%
12	16.663	2304	2308	2310	rBV4	2589	3511	0.16%	0.037%
13	16.692	2310	2313	2315	rVB2	2657	2748	0.12%	0.029%
14	16.722	2315	2318	2321	rBV4	2378	3045	0.14%	0.032%
15	16.863	2340	2342	2347	rVB3	1662	2580	0.12%	0.027%
16	16.951	2352	2357	2363	rBV6	7086	16215	0.73%	0.169%
17	17.075	2376	2378	2382	rBV5	1823	2368	0.11%	0.025%
18	17.163	2387	2393	2404	rBV	1299788	1987817	89.52%	20.757%
19	17.369	2425	2428	2431	rBV5	2331	2972	0.13%	0.031%
20	17.686	2478	2482	2485	rBV6	2698	3940	0.18%	0.041%
21	18.081	2546	2549	2550	rBV3	2407	2559	0.12%	0.027%
22	18.375	2597	2599	2602	rBV4	2114	2345	0.11%	0.024%
23	19.504	2789	2791	2799	rBV8	5303	9062	0.41%	0.095%
24	21.357	3101	3106	3116	rBV	1681726	2220576	100.00%	23.188%
25	23.668	3493	3499	3511	rVB2	1052139	2074904	93.44%	21.666%




Sum of corrected areas: 9576573

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020171.D
Acq On : 15 Jun 2022 12:51
Operator : CG/JU
Sample : N3317-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

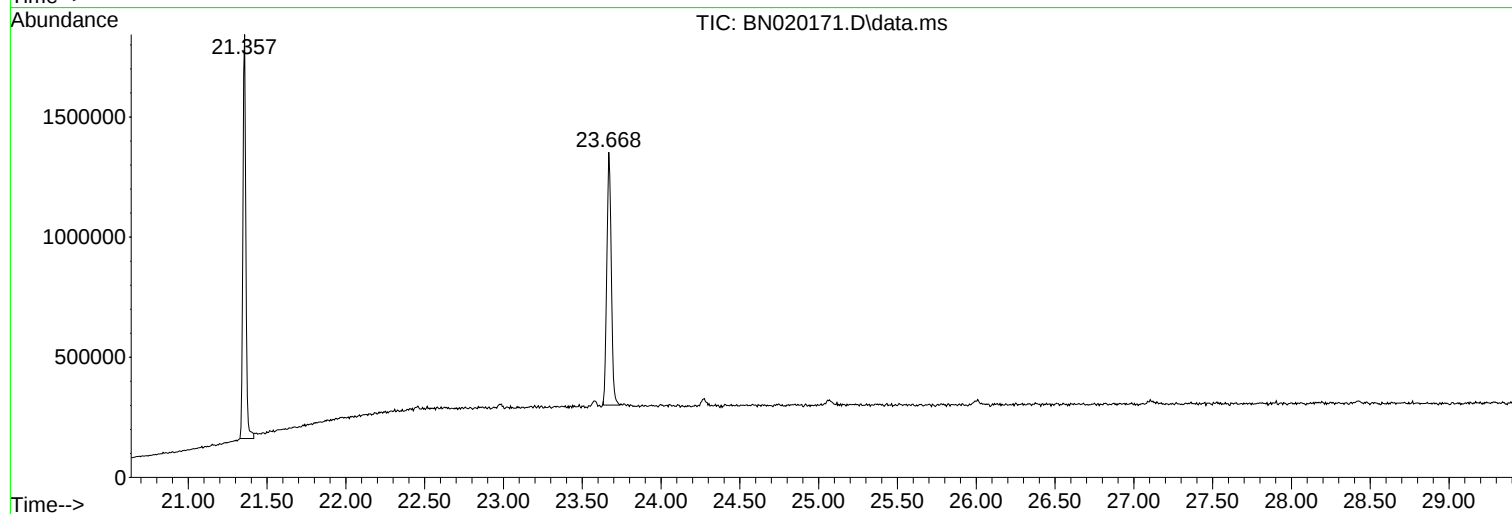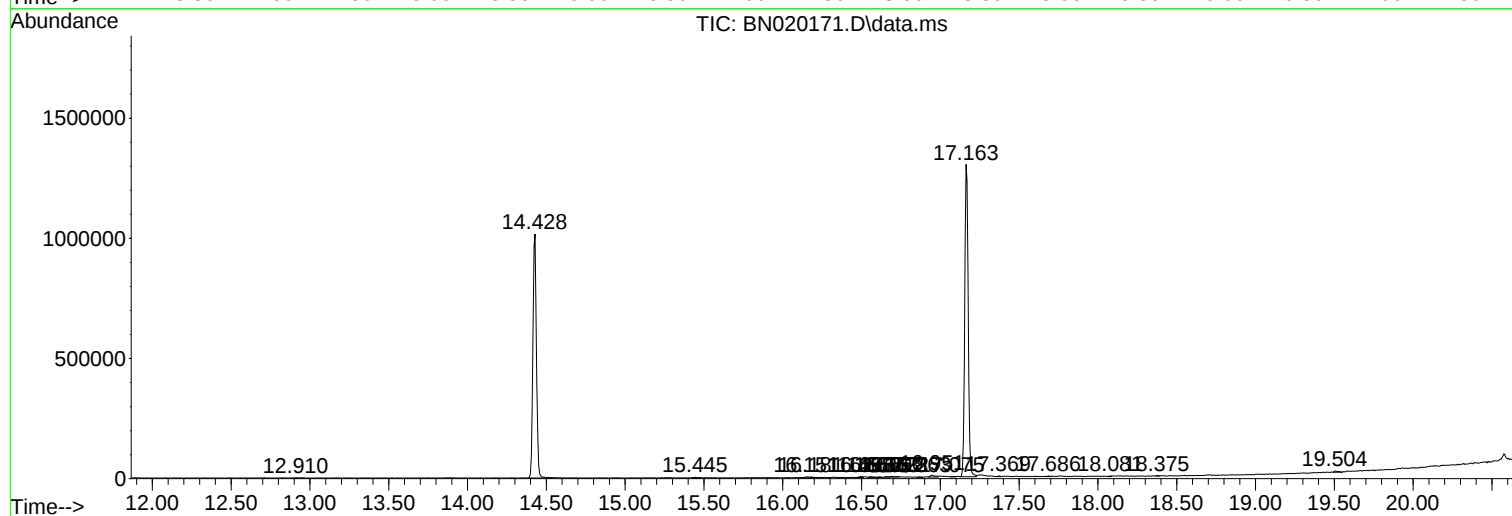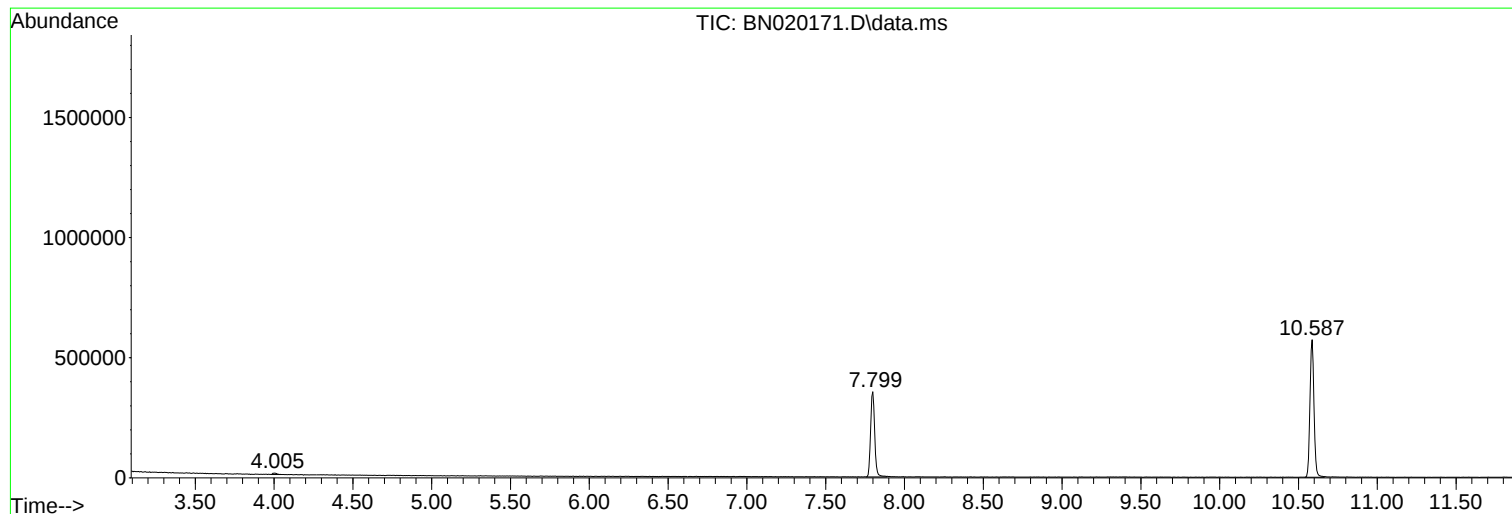

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020171.D
Acq On : 15 Jun 2022 12:51
Operator : CG/JU
Sample : N3317-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020171.D
Acq On : 15 Jun 2022 12:51
Operator : CG/JU
Sample : N3317-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc