

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020175.D
 Acq On : 15 Jun 2022 15:17
 Operator : CG/JU
 Sample : N3285-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	40	rVB	29267	45806	0.92%	0.101%
2	3.681	98	101	118	rBV	106680	203227	4.06%	0.447%
3	3.911	135	140	147	rBV2	13726	24295	0.49%	0.053%
4	3.999	152	155	162	rVB	10462	15952	0.32%	0.035%
5	4.799	287	291	295	rVB6	3799	6259	0.13%	0.014%
6	4.916	307	311	318	rBV3	8883	15624	0.31%	0.034%
7	6.981	655	662	672	rBV	185455	316958	6.34%	0.697%
8	7.128	681	687	702	rBV	516870	870577	17.40%	1.916%
9	7.334	715	722	735	rBV	571929	955498	19.10%	2.102%
10	7.434	735	739	745	rVB7	3814	6794	0.14%	0.015%
11	7.799	794	801	809	rBV	481371	795381	15.90%	1.750%
12	8.510	915	922	938	rBV	533813	920378	18.40%	2.025%
13	8.952	990	997	1011	rBV	685343	1187477	23.74%	2.613%
14	9.669	1111	1119	1133	rBV	583315	1002402	20.04%	2.206%
15	10.216	1204	1212	1223	rBV	841589	1467644	29.34%	3.229%
16	10.587	1267	1275	1283	rBV	780718	1353799	27.06%	2.979%
17	10.722	1291	1298	1314	rBV	777556	1413873	28.26%	3.111%
18	12.175	1538	1545	1552	rBV2	14355	27313	0.55%	0.060%
19	13.839	1821	1828	1843	rBV	1807958	2564005	51.25%	5.642%
20	14.116	1868	1875	1891	rBV	1911455	2937812	58.73%	6.464%
21	14.428	1921	1928	1937	rBV	1288838	1964962	39.28%	4.324%
22	14.645	1959	1965	1983	rBV	157746	330575	6.61%	0.727%
23	14.851	1996	2000	2005	rBV4	12460	17196	0.34%	0.038%
24	15.169	2051	2054	2061	rBV7	2615	5548	0.11%	0.012%
25	15.239	2061	2066	2069	rBV2	4549	7519	0.15%	0.017%
26	15.416	2089	2096	2109	rBV	2499815	3802914	76.02%	8.368%
27	15.539	2110	2117	2132	rVV	1097740	1559317	31.17%	3.431%
28	15.657	2132	2137	2145	rVB2	32801	53210	1.06%	0.117%
29	16.145	2218	2220	2226	rVV6	4826	9235	0.18%	0.020%
30	16.204	2226	2230	2234	rVB5	10783	15945	0.32%	0.035%
31	16.504	2274	2281	2283	rBV7	5101	9717	0.19%	0.021%
32	16.686	2304	2312	2316	rVV5	5943	16759	0.34%	0.037%
33	16.851	2337	2340	2344	rVB5	5848	7585	0.15%	0.017%
34	16.945	2351	2356	2362	rBV6	10931	21536	0.43%	0.047%
35	17.169	2387	2394	2403	rBV	1584495	2360996	47.20%	5.195%
36	17.263	2404	2410	2423	rVV2	2815181	4424156	88.44%	9.735%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020175.D
 Acq On : 15 Jun 2022 15:17
 Operator : CG/JU
 Sample : N3285-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	17.757	2491	2494	2498	rBV4	4573	5517	0.11%	0.012%
38	17.845	2504	2509	2514	rVB8	7880	13154	0.26%	0.029%
39	18.069	2543	2547	2556	rBV	68021	115246	2.30%	0.254%
40	18.545	2625	2628	2630	rBV3	3461	5077	0.10%	0.011%
41	19.127	2722	2727	2732	rVB	39962	56637	1.13%	0.125%
42	19.198	2735	2739	2743	rBV	39926	57237	1.14%	0.126%
43	19.357	2761	2766	2775	rBV2	53611	98818	1.98%	0.217%
44	19.504	2788	2791	2794	rBV3	18796	20730	0.41%	0.046%
45	19.563	2794	2801	2811	rBV2	3487734	5002634	100.00%	11.008%
46	20.574	2971	2973	2977	rVB	43383	45041	0.90%	0.099%
47	21.357	3101	3106	3118	rBV	1928030	2569864	51.37%	5.655%
48	23.527	3467	3475	3482	rBV	2226234	4494844	89.85%	9.890%
49	23.674	3493	3500	3511	rVB2	1096624	2224287	44.46%	4.894%




Sum of corrected areas: 45447330

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020175.D
Acq On : 15 Jun 2022 15:17
Operator : CG/JU
Sample : N3285-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

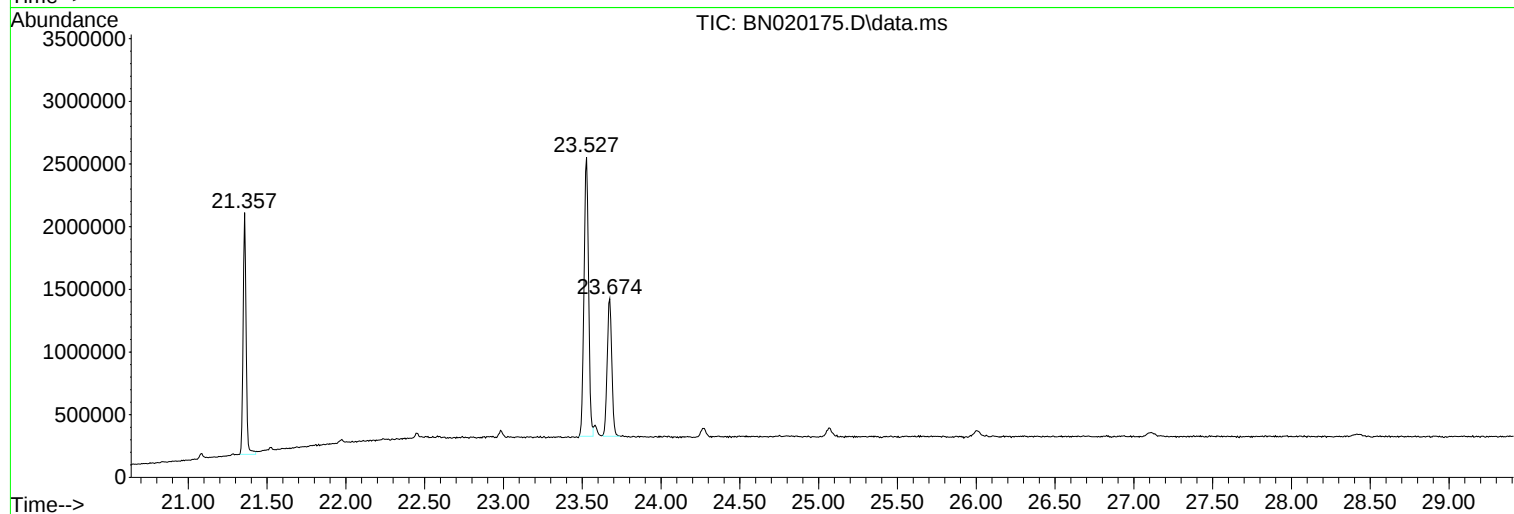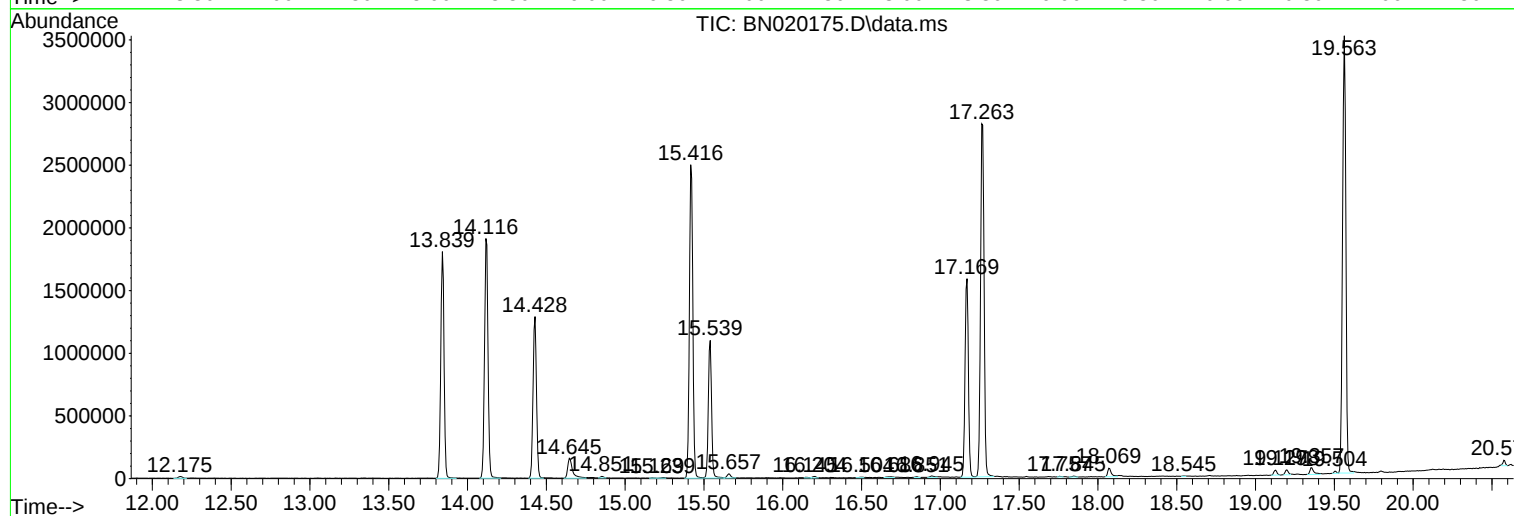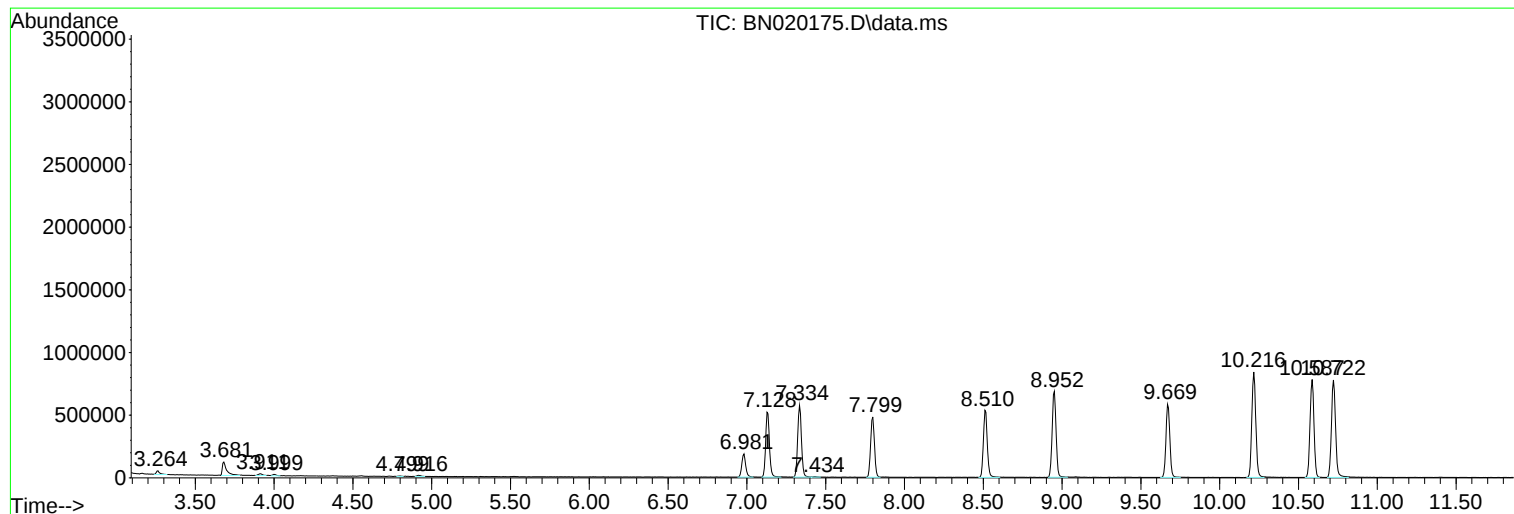

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020175.D
Acq On : 15 Jun 2022 15:17
Operator : CG/JU
Sample : N3285-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020175.D
Acq On : 15 Jun 2022 15:17
Operator : CG/JU
Sample : N3285-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------