

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020180.D
 Acq On : 15 Jun 2022 18:19
 Operator : CG/JU
 Sample : N3285-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	25	30	37	rBV	24365	38502	0.83%	0.094%
2	3.352	43	45	53	rVB4	9730	15029	0.33%	0.037%
3	3.675	98	100	115	rBV	110691	208641	4.51%	0.509%
4	3.905	135	139	146	rVB	12243	22771	0.49%	0.056%
5	3.999	152	155	163	rVB	13487	23331	0.50%	0.057%
6	4.364	213	217	225	rVB2	15466	26996	0.58%	0.066%
7	4.464	231	234	239	rVB5	4232	6856	0.15%	0.017%
8	4.922	307	312	319	rVB4	8712	14469	0.31%	0.035%
9	6.940	650	655	657	rBV2	12240	17361	0.38%	0.042%
10	6.981	657	662	672	rVB	130506	225074	4.87%	0.549%
11	7.128	680	687	701	rBV	422957	711125	15.38%	1.733%
12	7.334	715	722	735	rBV	448205	752760	16.28%	1.835%
13	7.434	735	739	747	rVV7	3572	6442	0.14%	0.016%
14	7.499	747	750	754	rVB4	3825	4889	0.11%	0.012%
15	7.799	794	801	811	rBV	439228	736924	15.94%	1.796%
16	8.058	839	845	850	rVB6	2495	5381	0.12%	0.013%
17	8.516	916	923	936	rBV	394553	681431	14.74%	1.661%
18	8.710	951	956	963	rVB2	4371	8571	0.19%	0.021%
19	8.893	982	987	990	rBV5	2987	5843	0.13%	0.014%
20	8.952	990	997	1006	rVV	558124	961432	20.79%	2.344%
21	9.087	1017	1020	1022	rBV3	4159	5703	0.12%	0.014%
22	9.122	1022	1026	1033	rVB3	12178	20133	0.44%	0.049%
23	9.669	1111	1119	1134	rBV	474943	812727	17.58%	1.981%
24	9.928	1157	1163	1165	rBV5	2958	4864	0.11%	0.012%
25	10.216	1205	1212	1228	rBV	686989	1210154	26.17%	2.950%
26	10.587	1267	1275	1286	rBV	714083	1246080	26.95%	3.037%
27	10.722	1290	1298	1311	rBV	673208	1203172	26.02%	2.933%
28	11.399	1405	1413	1424	rBV4	10443	24240	0.52%	0.059%
29	12.181	1539	1546	1553	rVB	12998	23182	0.50%	0.057%
30	12.887	1663	1666	1672	rVB6	2836	5130	0.11%	0.013%
31	13.340	1736	1743	1748	rBV4	3098	5346	0.12%	0.013%
32	13.840	1821	1828	1839	rBV	1538715	2224079	48.10%	5.421%
33	14.116	1868	1875	1891	rBV	1616499	2561147	55.39%	6.243%
34	14.428	1921	1928	1941	rBV	1211509	1832603	39.63%	4.467%
35	14.651	1960	1966	1981	rBV	109531	219582	4.75%	0.535%
36	14.787	1984	1989	1993	rVV7	5193	11654	0.25%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020180.D
 Acq On : 15 Jun 2022 18:19
 Operator : CG/JU
 Sample : N3285-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	14.857	1996	2001	2006	rVB6	8253	13038	0.28%	0.032%
38	15.116	2037	2045	2051	rBV4	6357	10783	0.23%	0.026%
39	15.240	2061	2066	2071	rBV6	5180	9718	0.21%	0.024%
40	15.287	2071	2074	2080	rVB4	6199	8900	0.19%	0.022%
41	15.416	2089	2096	2110	rBV	2233678	3409695	73.74%	8.311%
42	15.534	2110	2116	2129	rVV	879854	1247332	26.98%	3.040%
43	15.657	2132	2137	2144	rVB	28251	43063	0.93%	0.105%
44	16.151	2217	2221	2225	rBV	12980	19738	0.43%	0.048%
45	16.198	2226	2229	2235	rVB5	9842	15368	0.33%	0.037%
46	16.304	2246	2247	2255	rVB6	3459	6345	0.14%	0.015%
47	16.492	2274	2279	2282	rBV5	5779	8670	0.19%	0.021%
48	16.657	2301	2307	2309	rBV5	4046	6637	0.14%	0.016%
49	16.722	2315	2318	2321	rVB5	4043	4995	0.11%	0.012%
50	16.851	2336	2340	2345	rVB6	3769	5911	0.13%	0.014%
51	16.945	2351	2356	2362	rBV3	17900	32145	0.70%	0.078%
52	16.992	2362	2364	2369	rVB5	4024	6099	0.13%	0.015%
53	17.169	2387	2394	2402	rBV	1512013	2287369	49.47%	5.576%
54	17.269	2403	2411	2423	rVV	2657871	3973003	85.92%	9.684%
55	17.363	2423	2427	2432	rVB3	22771	34053	0.74%	0.083%
56	17.681	2477	2481	2486	rBV3	11374	14623	0.32%	0.036%
57	17.757	2491	2494	2497	rVB4	4511	6464	0.14%	0.016%
58	17.845	2507	2509	2513	rVB5	5842	6684	0.14%	0.016%
59	18.016	2534	2538	2540	rBV4	6211	7412	0.16%	0.018%
60	18.075	2543	2548	2554	rVV4	20459	33137	0.72%	0.081%
61	18.139	2554	2559	2563	rVB5	5265	10549	0.23%	0.026%
62	18.322	2585	2590	2595	rBV6	6893	10562	0.23%	0.026%
63	18.375	2595	2599	2601	rBV2	8978	9903	0.21%	0.024%
64	18.704	2652	2655	2659	rBV5	4283	6112	0.13%	0.015%
65	19.004	2703	2706	2712	rBV7	6175	9716	0.21%	0.024%
66	19.128	2722	2727	2732	rBV	37256	52119	1.13%	0.127%
67	19.198	2734	2739	2743	rBV	33410	51851	1.12%	0.126%
68	19.357	2762	2766	2770	rBV4	16823	27587	0.60%	0.067%
69	19.504	2788	2791	2794	rBV3	17121	20111	0.43%	0.049%
70	19.563	2794	2801	2813	rVV	3206103	4623981	100.00%	11.271%
71	19.792	2838	2840	2844	rVB3	10048	11113	0.24%	0.027%
72	20.575	2970	2973	2978	rVB	42136	44435	0.96%	0.108%
73	21.357	3100	3106	3116	rBV	1906224	2548866	55.12%	6.213%
74	23.527	3467	3475	3481	rBV	2029310	4204772	90.93%	10.249%
75	23.669	3492	3499	3510	rBV2	1155916	2298115	49.70%	5.602%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020180.D
Acq On : 15 Jun 2022 18:19
Operator : CG/JU
Sample : N3285-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION




Sum of corrected areas: 41024598

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020180.D
Acq On : 15 Jun 2022 18:19
Operator : CG/JU
Sample : N3285-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

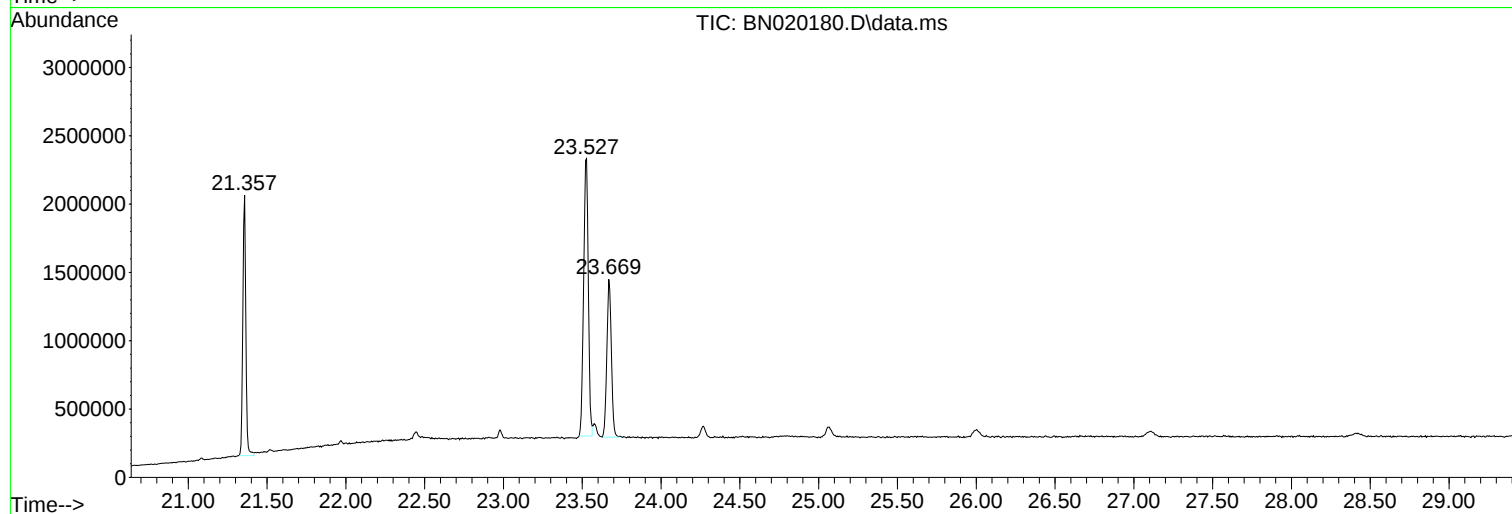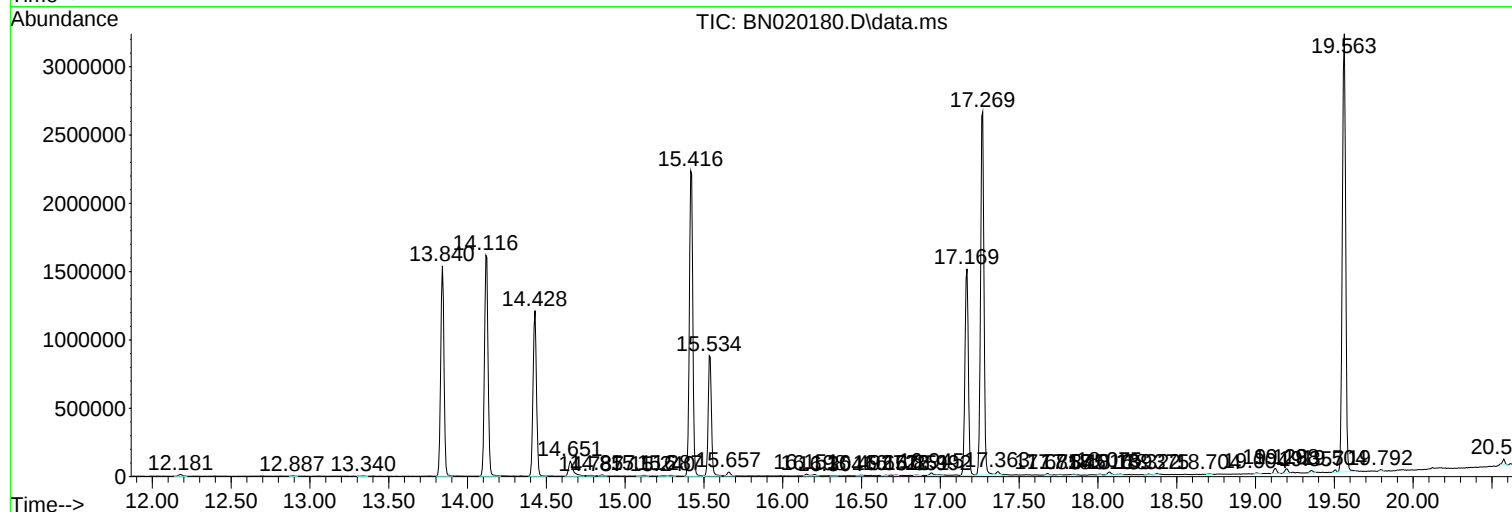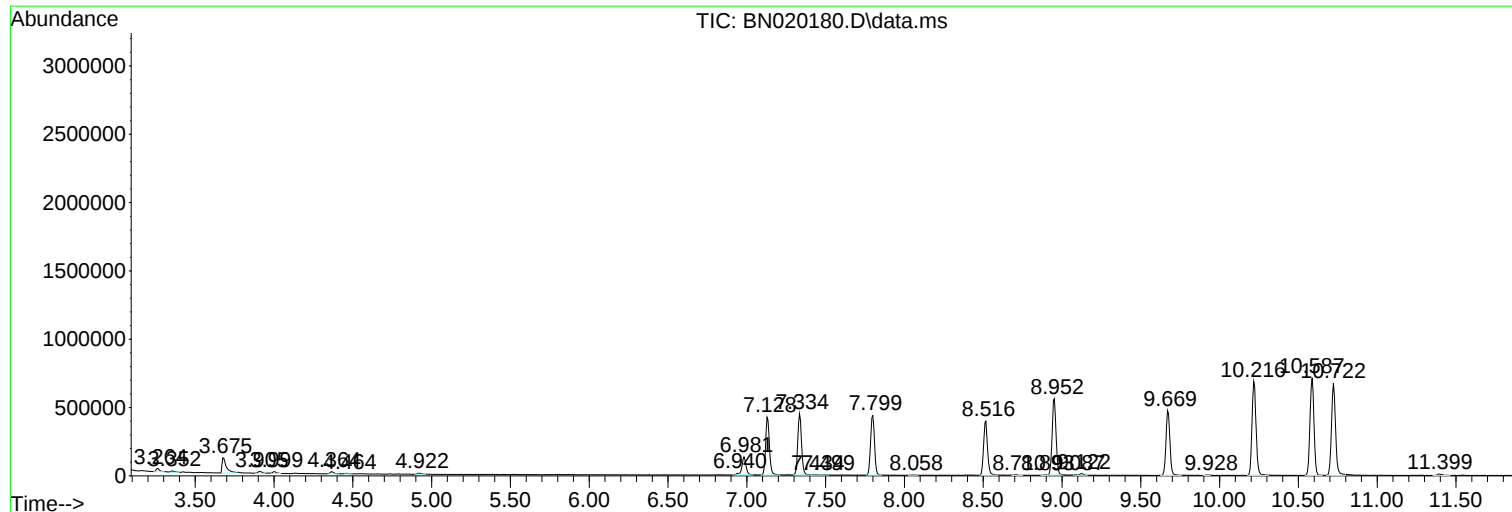

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020180.D
Acq On : 15 Jun 2022 18:19
Operator : CG/JU
Sample : N3285-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020180.D
Acq On : 15 Jun 2022 18:19
Operator : CG/JU
Sample : N3285-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------