

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020184.D
 Acq On : 15 Jun 2022 21:21
 Operator : CG/JU
 Sample : PB145543BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK543

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	36	rBV	28899	41566	1.06%	0.103%
2	3.669	95	99	121	rBV	380832	652052	16.70%	1.611%
3	3.999	152	155	160	rVB3	7167	11404	0.29%	0.028%
4	6.975	653	661	678	rBV	527673	918024	23.52%	2.269%
5	7.128	681	687	699	rBV	426976	698477	17.89%	1.726%
6	7.334	715	722	737	rBV	551981	925443	23.71%	2.287%
7	7.798	793	801	812	rBV	428064	730796	18.72%	1.806%
8	8.510	915	922	937	rBV	748017	1262847	32.35%	3.121%
9	8.945	988	996	1008	rBV	540302	934568	23.94%	2.310%
10	9.669	1112	1119	1134	rBV	483518	810477	20.76%	2.003%
11	10.216	1205	1212	1224	rBV	723314	1266754	32.45%	3.130%
12	10.587	1267	1275	1286	rBV	715861	1242316	31.83%	3.070%
13	10.722	1290	1298	1317	rBV	762708	1391694	35.65%	3.439%
14	12.181	1540	1546	1552	rBV2	11403	20000	0.51%	0.049%
15	13.339	1738	1743	1748	rBV3	9159	13097	0.34%	0.032%
16	13.839	1821	1828	1841	rBV	1467624	2081042	53.31%	5.143%
17	14.116	1867	1875	1889	rBV	1597298	2428668	62.22%	6.002%
18	14.428	1920	1928	1942	rBV	1234036	1869389	47.89%	4.620%
19	14.639	1957	1964	1982	rBV	563599	1027826	26.33%	2.540%
20	14.786	1987	1989	1994	rVB6	3137	5110	0.13%	0.013%
21	15.416	2089	2096	2110	rBV	2069875	3074834	78.77%	7.599%
22	15.533	2110	2116	2132	rVV	817464	1157602	29.66%	2.861%
23	15.657	2132	2137	2142	rVB	22768	36185	0.93%	0.089%
24	16.145	2216	2220	2224	rBV4	4012	5788	0.15%	0.014%
25	16.198	2225	2229	2235	rVB5	7175	11919	0.31%	0.029%
26	16.498	2272	2280	2283	rBV7	3720	7978	0.20%	0.020%
27	16.945	2351	2356	2361	rBV5	8644	17491	0.45%	0.043%
28	17.163	2387	2393	2403	rBV	1546187	2262490	57.96%	5.591%
29	17.263	2403	2410	2423	rVV2	2295934	3436501	88.04%	8.493%
30	17.410	2433	2435	2442	rVB7	2907	4466	0.11%	0.011%
31	18.074	2543	2548	2553	rBV6	6934	12044	0.31%	0.030%
32	18.139	2556	2559	2562	rBV4	2890	4083	0.10%	0.010%
33	19.121	2721	2726	2733	rBV3	28091	45624	1.17%	0.113%
34	19.198	2733	2739	2746	rBV	30486	48470	1.24%	0.120%
35	19.351	2761	2765	2768	rBV5	7125	12453	0.32%	0.031%
36	19.504	2788	2791	2794	rBV4	8200	8571	0.22%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020184.D
Acq On : 15 Jun 2022 21:21
Operator : CG/JU
Sample : PB145543BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK543

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	19.557	2794	2800	2813	rBV	2721817	3903432	100.00%	9.646%
38	19.921	2857	2862	2868	rBV7	13520	36006	0.92%	0.089%
39	20.568	2969	2972	2976	rBV	30513	35031	0.90%	0.087%
40	21.351	3099	3105	3117	rBV	1771869	2457618	62.96%	6.073%
41	23.515	3466	3473	3480	rBV2	1735840	3406156	87.26%	8.418%
42	23.662	3491	3498	3507	rVB2	1052483	2148717	55.05%	5.310%




Sum of corrected areas: 40465009

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020184.D
Acq On : 15 Jun 2022 21:21
Operator : CG/JU
Sample : PB145543BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

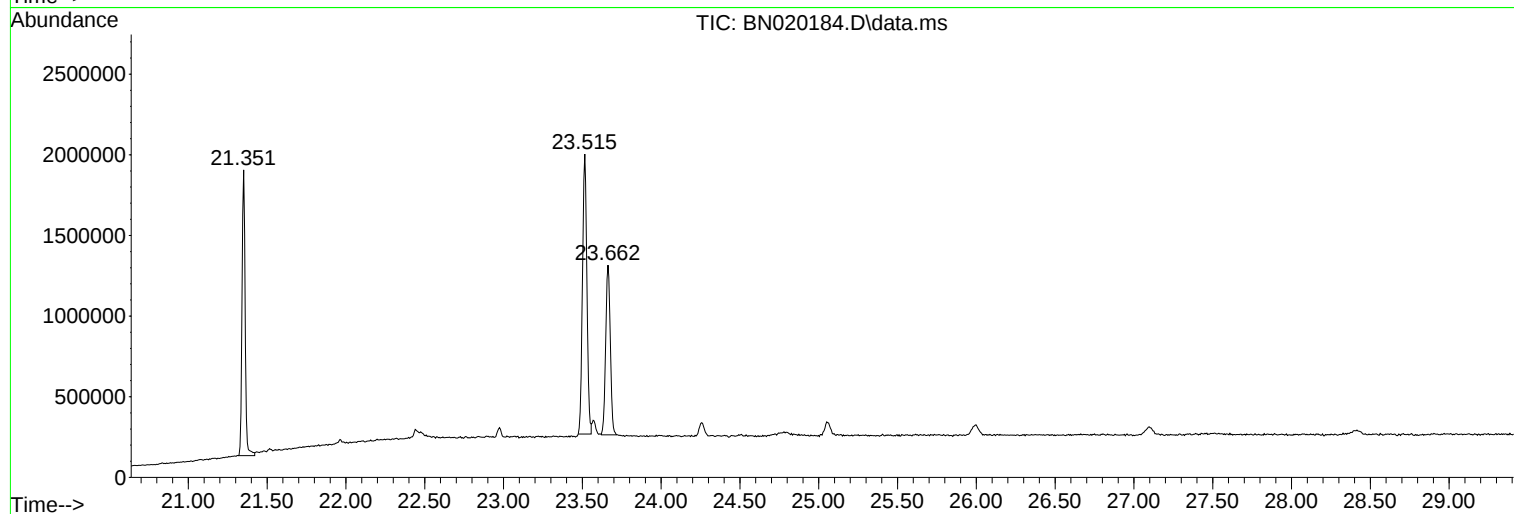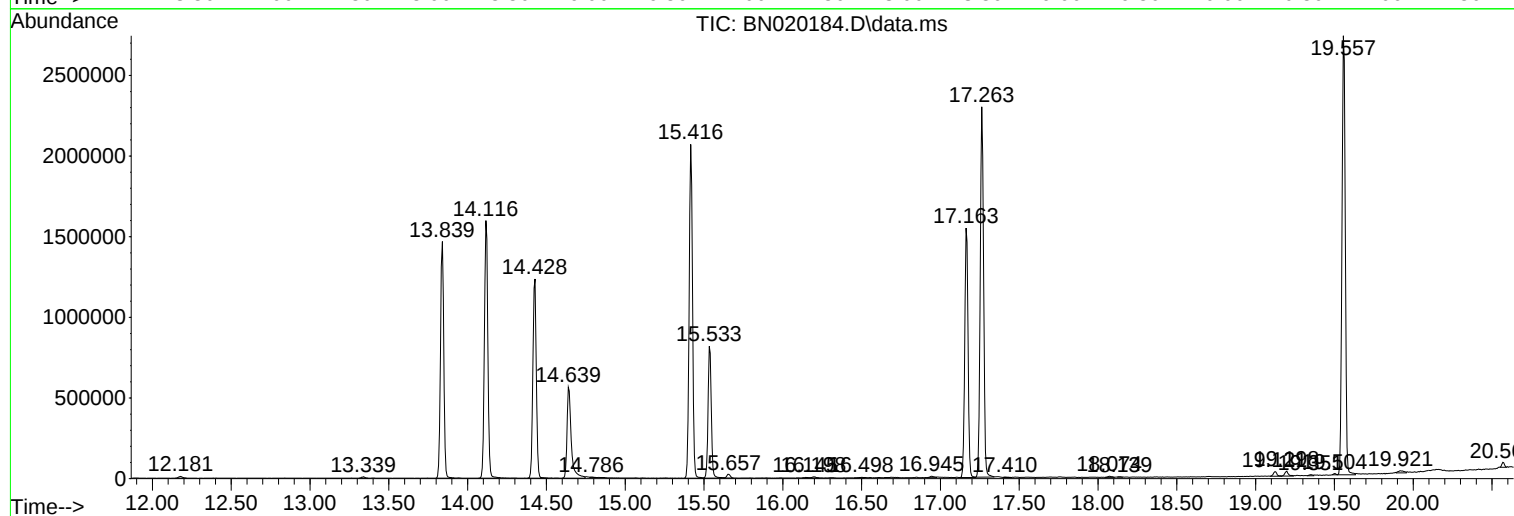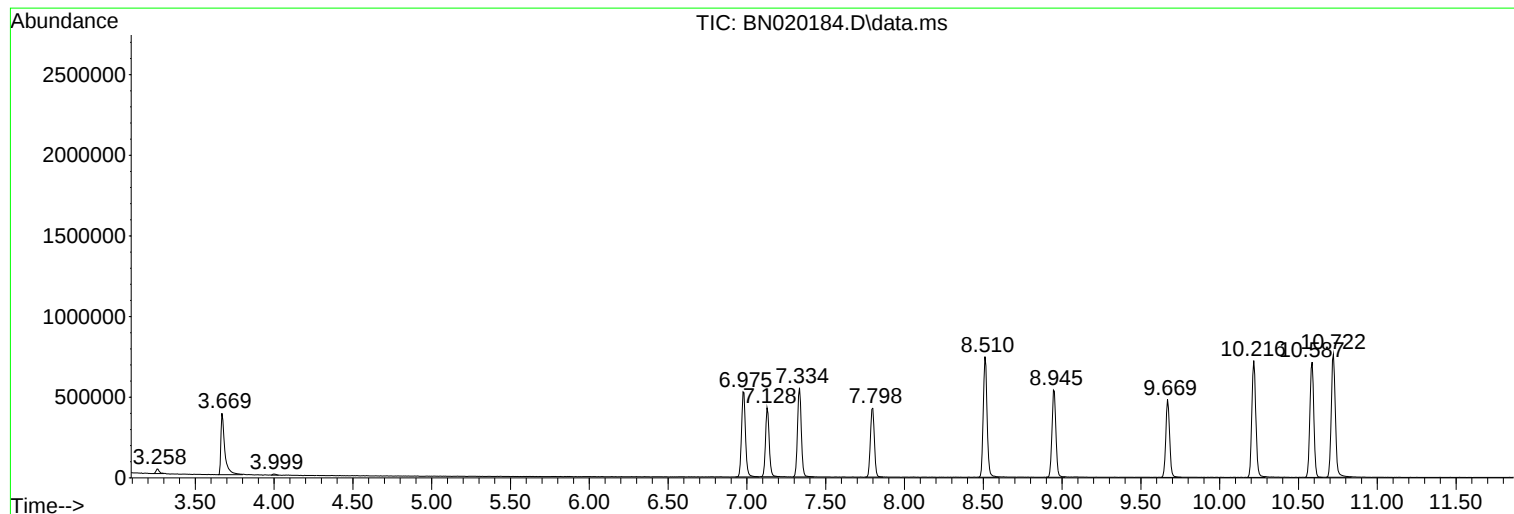

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020184.D
Acq On : 15 Jun 2022 21:21
Operator : CG/JU
Sample : PB145543BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020184.D
Acq On : 15 Jun 2022 21:21
Operator : CG/JU
Sample : PB145543BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------