

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020191.D
 Acq On : 16 Jun 2022 01:34
 Operator : CG/JU
 Sample : N3294-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	38	rVB	32824	51917	0.92%	0.109%
2	3.675	97	100	116	rBV	144936	246997	4.36%	0.520%
3	3.911	136	140	146	rVB	18743	31798	0.56%	0.067%
4	4.005	152	156	161	rVB2	9927	16120	0.28%	0.034%
5	4.558	246	250	255	rVB6	5240	7050	0.12%	0.015%
6	4.917	306	311	319	rVB3	10633	19822	0.35%	0.042%
7	5.511	410	412	422	rVB4	3831	7894	0.14%	0.017%
8	6.993	657	664	675	rBV	232635	404948	7.14%	0.852%
9	7.128	680	687	699	rBV	643872	1051214	18.54%	2.212%
10	7.334	716	722	734	rBV	693988	1179824	20.81%	2.482%
11	7.793	793	800	809	rBV	379304	624163	11.01%	1.313%
12	8.522	916	924	939	rBV	661133	1140814	20.12%	2.400%
13	8.946	988	996	1009	rBV	839336	1447748	25.54%	3.046%
14	9.087	1017	1020	1029	rVB7	4383	8606	0.15%	0.018%
15	9.669	1111	1119	1129	rBV	726826	1223223	21.58%	2.574%
16	10.222	1206	1213	1232	rBV	1007948	1826853	32.23%	3.843%
17	10.581	1267	1274	1283	rBV	600635	1059871	18.70%	2.230%
18	10.722	1290	1298	1315	rBV	949221	1730417	30.52%	3.641%
19	12.175	1540	1545	1550	rBV2	18588	30243	0.53%	0.064%
20	13.340	1737	1743	1749	rBV2	11833	19596	0.35%	0.041%
21	13.840	1821	1828	1840	rBV	2151539	3055450	53.90%	6.428%
22	14.116	1866	1875	1892	rBV	2346918	3547240	62.57%	7.463%
23	14.422	1920	1927	1935	rBV	1021971	1527744	26.95%	3.214%
24	14.675	1962	1970	1984	rBV	190931	377883	6.67%	0.795%
25	14.851	1997	2000	2009	rVB4	14512	24415	0.43%	0.051%
26	15.240	2060	2066	2070	rBV3	4608	10122	0.18%	0.021%
27	15.416	2089	2096	2110	rBV	3084923	4518694	79.71%	9.507%
28	15.534	2110	2116	2132	rVV	1313976	1857763	32.77%	3.909%
29	15.657	2132	2137	2143	rVB	39682	62084	1.10%	0.131%
30	16.198	2225	2229	2235	rVB2	13389	19185	0.34%	0.040%
31	16.504	2275	2281	2288	rBV10	4851	13174	0.23%	0.028%
32	16.681	2303	2311	2315	rBV7	7455	16500	0.29%	0.035%
33	16.722	2316	2318	2325	rVB7	4452	5855	0.10%	0.012%
34	16.845	2336	2339	2344	rVB5	7103	9129	0.16%	0.019%
35	16.939	2351	2355	2359	rBV5	8953	14833	0.26%	0.031%
36	17.163	2386	2393	2403	rBV	1281147	1846992	32.58%	3.886%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020191.D
 Acq On : 16 Jun 2022 01:34
 Operator : CG/JU
 Sample : N3294-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	17.263	2403	2410	2424	rBV2	3497482	5189395	91.54%	10.918%
38	17.551	2454	2459	2462	rBV6	4748	8799	0.16%	0.019%
39	17.845	2506	2509	2514	rVB5	7371	8441	0.15%	0.018%
40	18.069	2543	2547	2555	rBV	57650	93529	1.65%	0.197%
41	18.139	2557	2559	2563	rVB2	8758	9909	0.17%	0.021%
42	18.551	2625	2629	2633	rBV7	4881	8604	0.15%	0.018%
43	19.122	2721	2726	2732	rBV	51792	71920	1.27%	0.151%
44	19.192	2734	2738	2743	rBV	48331	70535	1.24%	0.148%
45	19.351	2761	2765	2774	rBV3	42949	78675	1.39%	0.166%
46	19.504	2788	2791	2794	rBV3	14589	15067	0.27%	0.032%
47	19.563	2794	2801	2808	rBV	3893149	5668931	100.00%	11.927%
48	19.792	2837	2840	2846	rBV	16721	20588	0.36%	0.043%
49	20.569	2969	2972	2977	rVB	40159	45768	0.81%	0.096%
50	21.351	3100	3105	3114	rBV	1272495	1694467	29.89%	3.565%
51	23.521	3466	3474	3480	rBV	2068818	4153155	73.26%	8.738%
52	23.663	3492	3498	3508	rVB2	683737	1357330	23.94%	2.856%




Sum of corrected areas: 47531294

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020191.D
Acq On : 16 Jun 2022 01:34
Operator : CG/JU
Sample : N3294-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

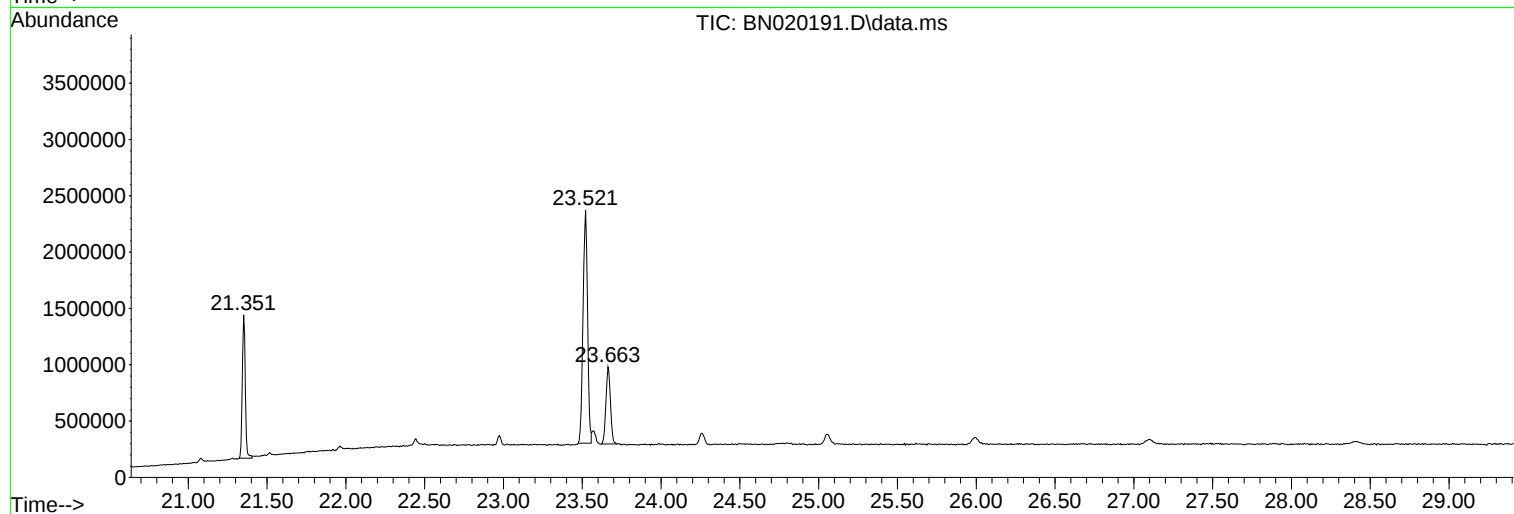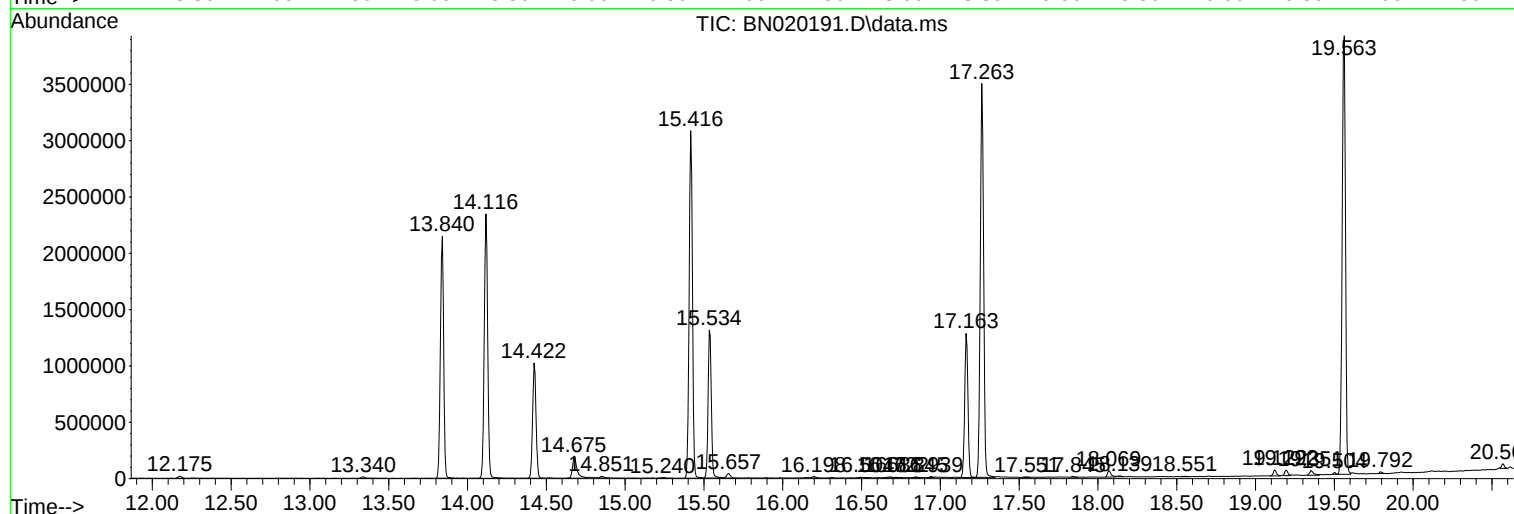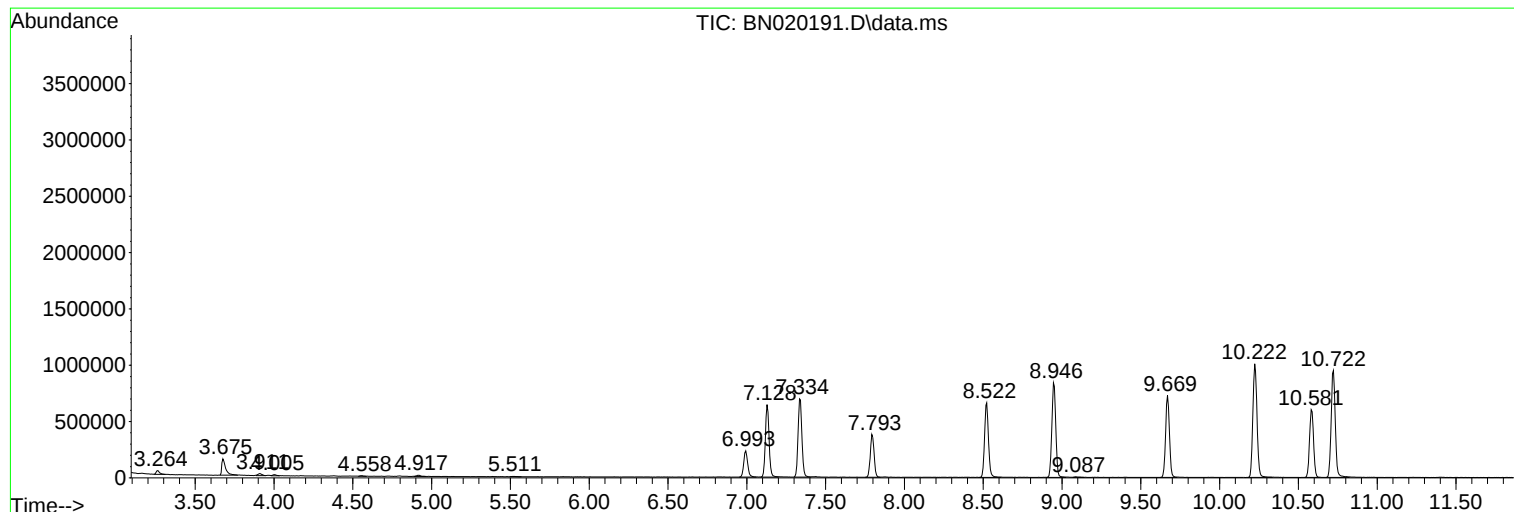

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020191.D
Acq On : 16 Jun 2022 01:34
Operator : CG/JU
Sample : N3294-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020191.D
Acq On : 16 Jun 2022 01:34
Operator : CG/JU
Sample : N3294-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc