

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020193.D
 Acq On : 16 Jun 2022 02:46
 Operator : CG/JU
 Sample : N3294-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	26	29	38	rVB	29715	47340	0.90%	0.102%
2	3.358	42	46	51	rVB3	9841	15431	0.29%	0.033%
3	3.675	97	100	118	rBV	133109	250014	4.75%	0.537%
4	3.905	135	139	146	rVB	14148	26146	0.50%	0.056%
5	3.999	152	155	164	rVB	18115	30957	0.59%	0.066%
6	4.364	213	217	224	rVB3	18111	29880	0.57%	0.064%
7	4.458	230	233	239	rBV6	6215	11578	0.22%	0.025%
8	4.917	307	311	319	rVB3	9916	17914	0.34%	0.038%
9	5.516	411	413	419	rVB4	3368	5689	0.11%	0.012%
10	6.940	650	655	658	rBV2	13538	21362	0.41%	0.046%
11	6.993	658	664	676	rVB	146247	259081	4.92%	0.556%
12	7.128	680	687	701	rBV	492353	814833	15.49%	1.749%
13	7.334	715	722	733	rBV	510383	859927	16.34%	1.846%
14	7.793	794	800	809	rBV	545497	881923	16.76%	1.893%
15	8.046	837	843	850	rBV7	3598	8220	0.16%	0.018%
16	8.522	917	924	937	rBV	446323	779437	14.81%	1.673%
17	8.710	950	956	959	rBV3	3656	7338	0.14%	0.016%
18	8.887	980	986	989	rBV5	3614	6157	0.12%	0.013%
19	8.946	989	996	1008	rVV	664903	1124054	21.36%	2.413%
20	9.122	1016	1026	1030	rBV4	11798	23704	0.45%	0.051%
21	9.669	1111	1119	1135	rBV	572427	955976	18.17%	2.052%
22	10.222	1206	1213	1227	rBV	794850	1391307	26.44%	2.987%
23	10.581	1265	1274	1282	rBV	852506	1481850	28.16%	3.181%
24	10.722	1289	1298	1309	rBV	764809	1372906	26.09%	2.947%
25	11.399	1407	1413	1424	rVB2	13212	25030	0.48%	0.054%
26	12.175	1540	1545	1553	rBV	15154	27000	0.51%	0.058%
27	13.840	1821	1828	1840	rBV	1722206	2532225	48.13%	5.436%
28	14.116	1868	1875	1895	rBV	1975947	2954796	56.16%	6.343%
29	14.422	1920	1927	1939	rBV	1432489	2187005	41.57%	4.695%
30	14.681	1963	1971	1986	rBV	129771	273590	5.20%	0.587%
31	14.792	1986	1990	1994	rVV6	6824	13332	0.25%	0.029%
32	14.851	1994	2000	2007	rVB7	10547	18907	0.36%	0.041%
33	15.116	2041	2045	2051	rVB3	7398	11633	0.22%	0.025%
34	15.234	2061	2065	2071	rBV3	5476	9221	0.18%	0.020%
35	15.287	2071	2074	2079	rVB2	5960	8274	0.16%	0.018%
36	15.416	2089	2096	2106	rBV	2586747	3871385	73.58%	8.311%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020193.D
 Acq On : 16 Jun 2022 02:46
 Operator : CG/JU
 Sample : N3294-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	15.534	2110	2116	2132	rVV	1061683	1480234	28.13%	3.178%
38	15.657	2132	2137	2148	rVB	34091	61155	1.16%	0.131%
39	16.145	2217	2220	2224	rBV	13852	18732	0.36%	0.040%
40	16.198	2224	2229	2233	rVB3	11431	18930	0.36%	0.041%
41	16.310	2243	2248	2257	rVB8	2663	6551	0.12%	0.014%
42	16.498	2271	2280	2283	rBV8	4792	10877	0.21%	0.023%
43	16.686	2309	2312	2315	rVV3	3661	6622	0.13%	0.014%
44	16.716	2315	2317	2321	rVB4	4498	5656	0.11%	0.012%
45	16.845	2335	2339	2344	rVB6	5341	7458	0.14%	0.016%
46	16.939	2351	2355	2362	rBV4	19883	31661	0.60%	0.068%
47	16.992	2362	2364	2368	rVB4	5651	6569	0.12%	0.014%
48	17.163	2386	2393	2403	rBV	1841844	2722371	51.74%	5.844%
49	17.263	2403	2410	2422	rVV2	3076538	4568740	86.83%	9.808%
50	17.363	2423	2427	2432	rVV2	32319	50003	0.95%	0.107%
51	17.404	2432	2434	2441	rVB7	4423	8577	0.16%	0.018%
52	17.545	2454	2458	2463	rVB6	4299	7521	0.14%	0.016%
53	17.675	2477	2480	2485	rVB3	11578	15528	0.30%	0.033%
54	17.845	2506	2509	2514	rVB5	6283	7665	0.15%	0.016%
55	18.010	2533	2537	2541	rVB7	8495	12494	0.24%	0.027%
56	18.069	2543	2547	2554	rVV2	21701	34974	0.66%	0.075%
57	18.139	2555	2559	2565	rVB7	6222	10680	0.20%	0.023%
58	18.322	2587	2590	2593	rBV5	7824	9440	0.18%	0.020%
59	18.375	2595	2599	2604	rVV3	8311	13458	0.26%	0.029%
60	18.698	2652	2654	2658	rVB5	5506	6604	0.13%	0.014%
61	19.004	2703	2706	2709	rBV4	8633	11672	0.22%	0.025%
62	19.122	2722	2726	2731	rBV2	45597	60382	1.15%	0.130%
63	19.192	2734	2738	2742	rBV	43140	57653	1.10%	0.124%
64	19.351	2761	2765	2769	rBV4	20143	28132	0.53%	0.060%
65	19.504	2787	2791	2794	rBV3	18868	24752	0.47%	0.053%
66	19.557	2794	2800	2808	rBV	3647831	5261640	100.00%	11.296%
67	19.792	2837	2840	2846	rVB3	15508	20936	0.40%	0.045%
68	20.569	2970	2972	2977	rVB	34932	35541	0.68%	0.076%
69	21.351	3099	3105	3116	rBV	2182669	2905105	55.21%	6.237%
70	23.516	3465	3473	3480	rBV2	2155901	4338511	82.46%	9.314%
71	23.663	3491	3498	3507	rVB	1238167	2358340	44.82%	5.063%




Sum of corrected areas: 46580586

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020193.D
Acq On : 16 Jun 2022 02:46
Operator : CG/JU
Sample : N3294-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

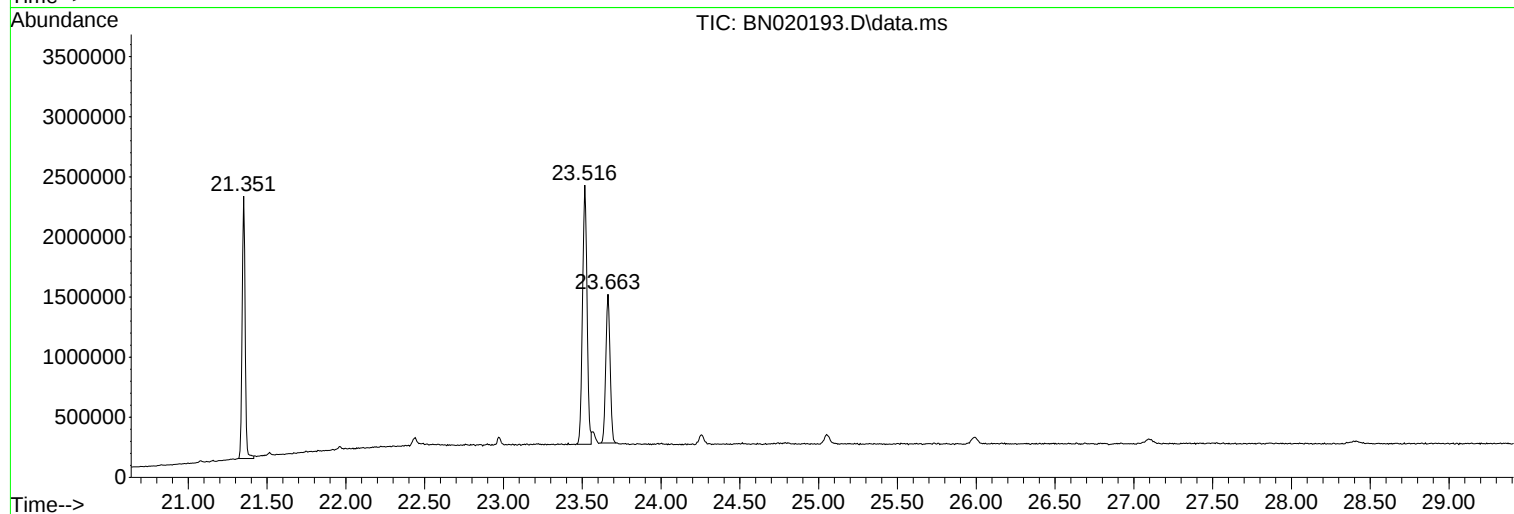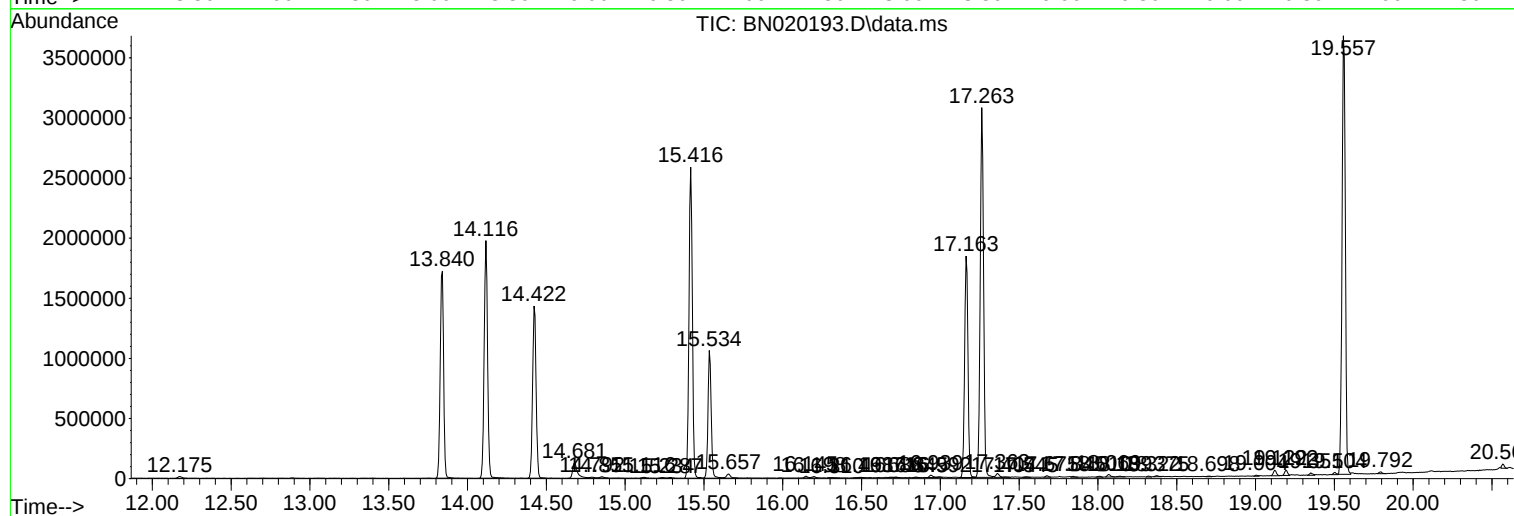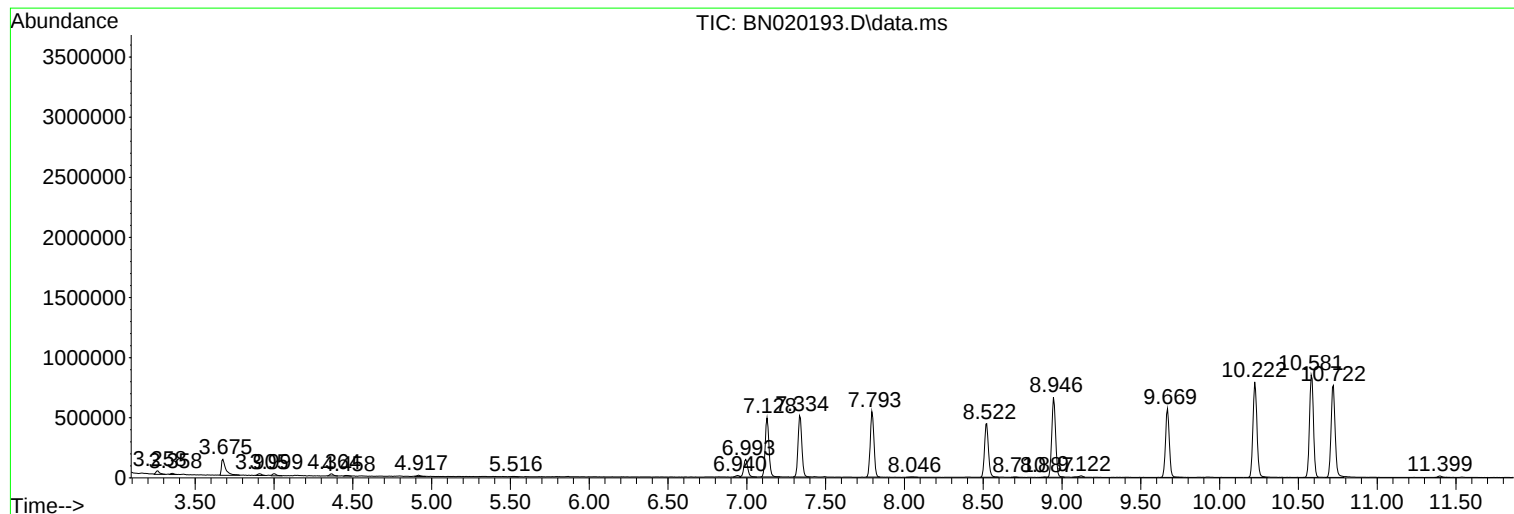

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020193.D
Acq On : 16 Jun 2022 02:46
Operator : CG/JU
Sample : N3294-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020193.D
Acq On : 16 Jun 2022 02:46
Operator : CG/JU
Sample : N3294-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc