

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020207.D
 Acq On : 16 Jun 2022 16:42
 Operator : CG/JU
 Sample : PB145551BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK551

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	36	rVB	37027	50048	1.20%	0.118%
2	3.664	95	98	116	rBV	462407	787995	18.90%	1.857%
3	3.999	152	155	159	rVB2	7700	11699	0.28%	0.028%
4	6.987	656	663	678	rBV	571340	981505	23.54%	2.313%
5	7.128	680	687	701	rVB	476423	784425	18.81%	1.849%
6	7.334	715	722	734	rBV	617595	1023468	24.54%	2.412%
7	7.793	793	800	813	rBV	494102	817233	19.60%	1.926%
8	8.516	916	923	941	rBV	793006	1343988	32.23%	3.168%
9	8.946	988	996	1011	rBV	614395	1040078	24.94%	2.451%
10	9.669	1110	1119	1131	rBV	515706	895943	21.49%	2.112%
11	10.222	1206	1213	1223	rBV	776961	1325808	31.79%	3.125%
12	10.581	1264	1274	1283	rBV	765555	1334545	32.00%	3.145%
13	10.716	1289	1297	1313	rBV	837107	1479925	35.49%	3.488%
14	12.175	1540	1545	1554	rVB2	12866	22264	0.53%	0.052%
15	13.834	1820	1827	1841	rBV	1610540	2238508	53.68%	5.276%
16	14.116	1867	1875	1895	rBV	1681548	2561569	61.43%	6.037%
17	14.422	1920	1927	1938	rBV	1285886	1926231	46.19%	4.540%
18	14.669	1962	1969	1987	rBV	528224	1061463	25.45%	2.502%
19	14.845	1996	1999	2005	rVB6	2993	4828	0.12%	0.011%
20	15.416	2089	2096	2110	rBV	2189653	3258610	78.14%	7.680%
21	15.534	2110	2116	2129	rVV	926313	1250712	29.99%	2.948%
22	15.651	2132	2136	2145	rVB2	27826	42525	1.02%	0.100%
23	16.198	2225	2229	2233	rVB3	8739	12654	0.30%	0.030%
24	16.492	2273	2279	2282	rBV4	3022	6320	0.15%	0.015%
25	16.845	2336	2339	2342	rVB2	3423	4367	0.10%	0.010%
26	16.945	2351	2356	2359	rBV3	6405	12426	0.30%	0.029%
27	17.163	2386	2393	2400	rBV	1602117	2327118	55.81%	5.485%
28	17.263	2403	2410	2423	rVV2	2451125	3677300	88.18%	8.667%
29	17.757	2490	2494	2501	rBV10	2804	5423	0.13%	0.013%
30	18.075	2543	2548	2551	rBV5	4928	8484	0.20%	0.020%
31	19.122	2721	2726	2732	rBV2	31088	44456	1.07%	0.105%
32	19.192	2734	2738	2743	rVV	27495	39648	0.95%	0.093%
33	19.351	2763	2765	2772	rBV5	3396	4888	0.12%	0.012%
34	19.504	2787	2791	2793	rBV5	9441	11851	0.28%	0.028%
35	19.557	2794	2800	2814	rVV	2959212	4170030	100.00%	9.828%
36	20.545	2966	2968	2969	rBV	9832	7686	0.18%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020207.D
Acq On : 16 Jun 2022 16:42
Operator : CG/JU
Sample : PB145551BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK551

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	20.574	2969	2973	2977	rVB2	30037	38390	0.92%	0.090%
38	21.351	3100	3105	3115	rBV	1784472	2389443	57.30%	5.632%
39	23.515	3466	3473	3480	rBV2	1778530	3406545	81.69%	8.029%
40	23.663	3492	3498	3509	rVB2	999134	2018335	48.40%	4.757%




Sum of corrected areas: 42428734

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020207.D
Acq On : 16 Jun 2022 16:42
Operator : CG/JU
Sample : PB145551BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

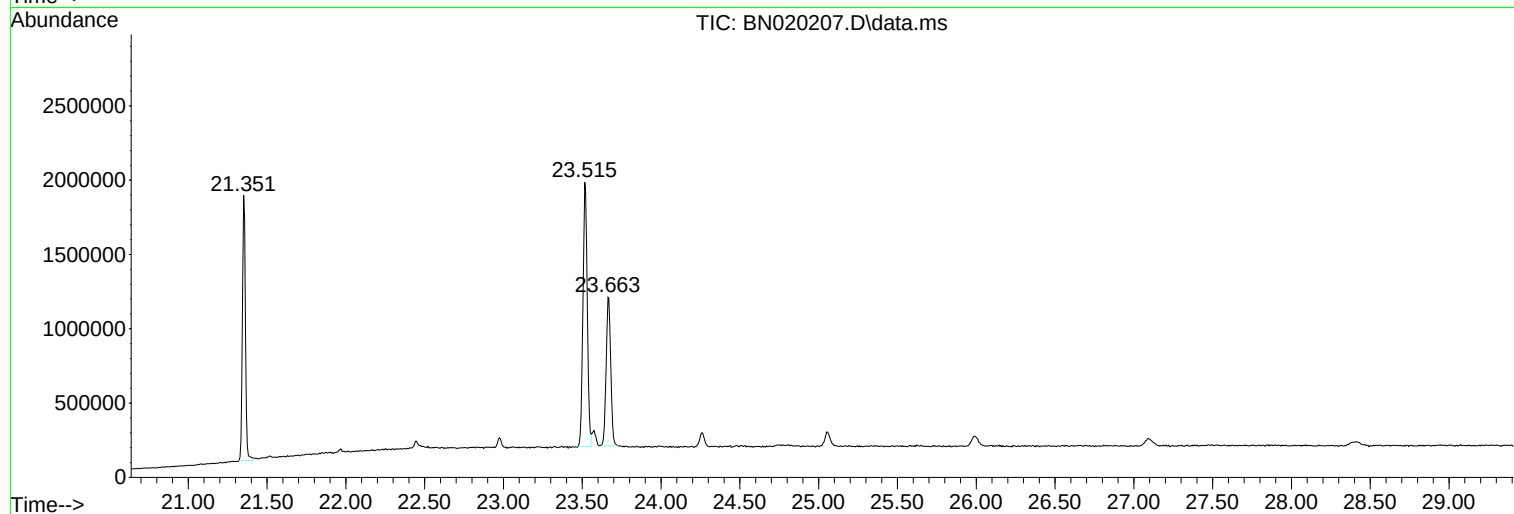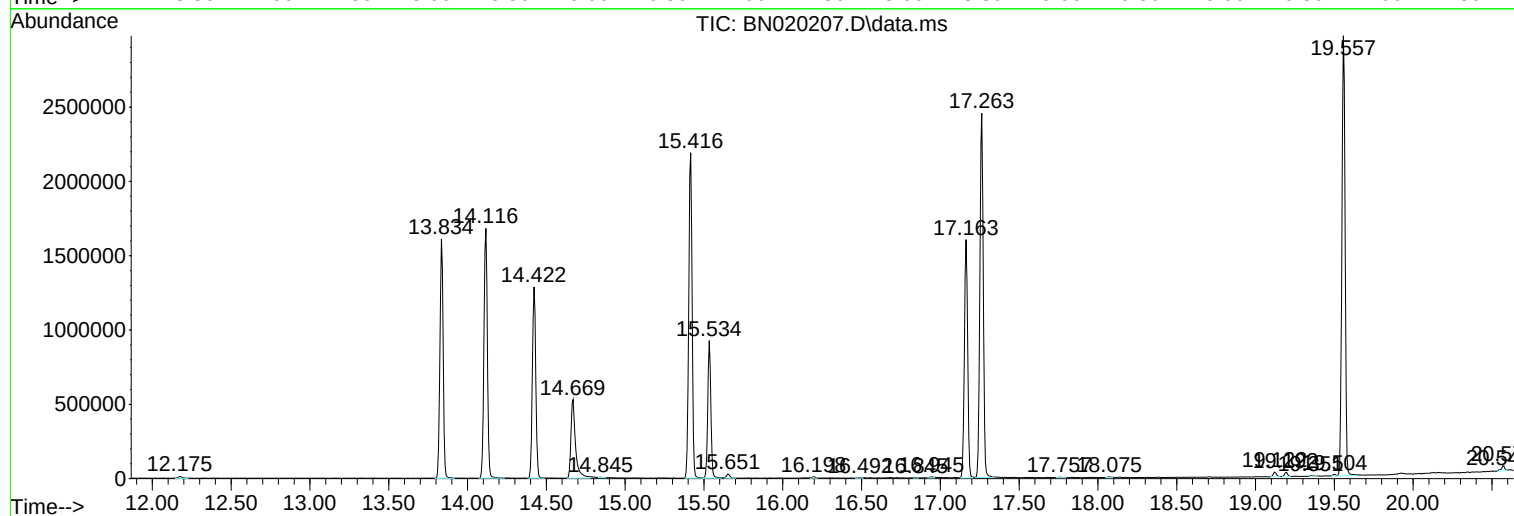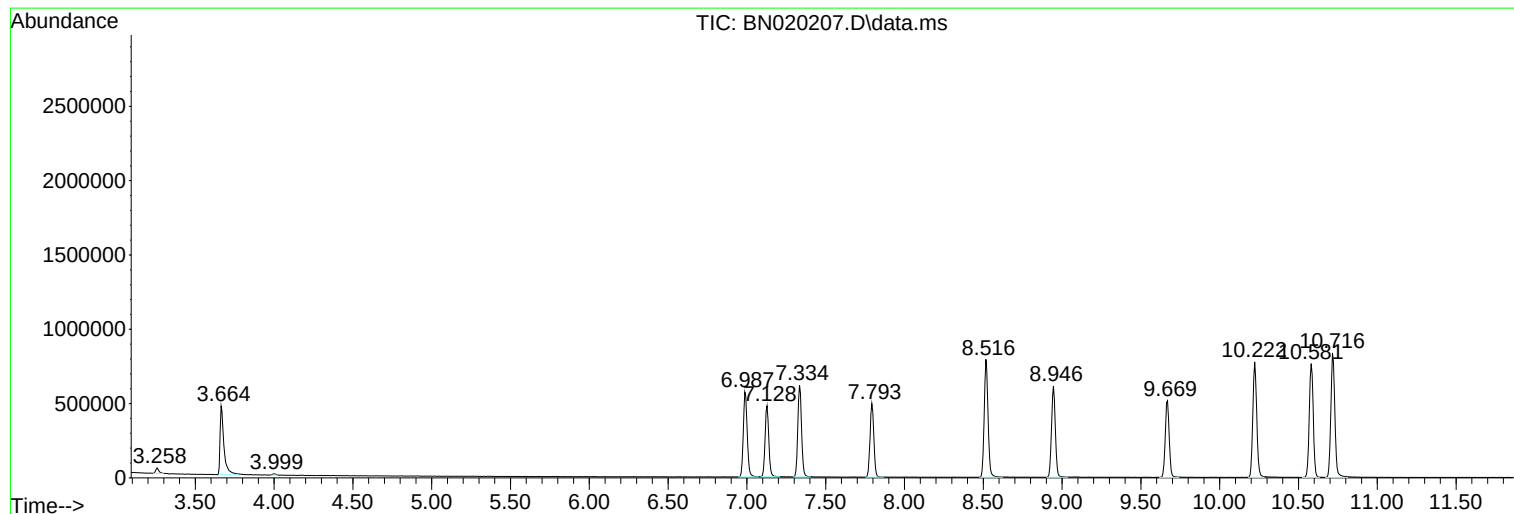

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020207.D
Acq On : 16 Jun 2022 16:42
Operator : CG/JU
Sample : PB145551BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020207.D
Acq On : 16 Jun 2022 16:42
Operator : CG/JU
Sample : PB145551BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc