

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020216.D
 Acq On : 16 Jun 2022 22:08
 Operator : CG/JU
 Sample : N3294-12
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	38	rVB	30667	46611	0.88%	0.099%
2	3.669	95	99	113	rBV	163783	286578	5.40%	0.607%
3	3.905	135	139	146	rVB	16247	27939	0.53%	0.059%
4	4.005	152	156	160	rVB4	9493	13802	0.26%	0.029%
5	4.905	305	309	315	rBV	7860	12785	0.24%	0.027%
6	5.846	465	469	475	rVB4	3535	6034	0.11%	0.013%
7	6.987	657	663	674	rBV	136633	245100	4.62%	0.519%
8	7.128	680	687	698	rBV	570567	958546	18.07%	2.030%
9	7.334	714	722	735	rBV	573577	953932	17.98%	2.020%
10	7.428	735	738	743	rVB5	3992	6016	0.11%	0.013%
11	7.793	793	800	812	rBV	546927	897638	16.92%	1.901%
12	8.516	916	923	939	rBV	473717	805788	15.19%	1.706%
13	8.946	988	996	1009	rBV	757725	1285931	24.24%	2.723%
14	9.663	1110	1118	1132	rBV	621250	1065962	20.10%	2.257%
15	10.222	1204	1213	1224	rBV	859298	1498971	28.26%	3.174%
16	10.581	1265	1274	1282	rBV	870571	1498738	28.25%	3.173%
17	10.716	1289	1297	1313	rBV	879027	1568732	29.57%	3.321%
18	12.175	1539	1545	1556	rVB3	15418	27607	0.52%	0.058%
19	13.834	1820	1827	1841	rBV	1988539	2833563	53.42%	5.999%
20	14.116	1866	1875	1894	rBV	2054424	3184300	60.03%	6.742%
21	14.422	1920	1927	1936	rBV	1429719	2119014	39.95%	4.487%
22	14.675	1964	1970	1986	rBV	110343	232064	4.37%	0.491%
23	14.969	2012	2020	2023	rBV2	10772	22837	0.43%	0.048%
24	15.234	2061	2065	2071	rVB5	4504	7446	0.14%	0.016%
25	15.416	2088	2096	2110	rBV	2700596	4160460	78.43%	8.809%
26	15.534	2110	2116	2128	rVV	1188395	1605871	30.27%	3.400%
27	15.651	2131	2136	2143	rVB	34764	53182	1.00%	0.113%
28	16.198	2224	2229	2233	rVB5	12366	18652	0.35%	0.039%
29	16.839	2335	2338	2343	rVB4	5820	7069	0.13%	0.015%
30	16.933	2348	2354	2361	rBV8	7894	21780	0.41%	0.046%
31	17.092	2379	2381	2386	rVB5	4836	6223	0.12%	0.013%
32	17.163	2386	2393	2400	rBV	1712965	2526873	47.64%	5.350%
33	17.263	2403	2410	2426	rVV	3146210	4712321	88.84%	9.977%
34	17.463	2440	2444	2451	rBV9	3551	7734	0.15%	0.016%
35	18.063	2543	2546	2551	rBV4	20890	32830	0.62%	0.070%
36	19.122	2722	2726	2731	rVB2	50445	66794	1.26%	0.141%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020216.D
 Acq On : 16 Jun 2022 22:08
 Operator : CG/JU
 Sample : N3294-12
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	19.192	2734	2738	2742	rVB	40768	55888	1.05%	0.118%
38	19.345	2762	2764	2768	rVB3	15552	18086	0.34%	0.038%
39	19.498	2787	2790	2793	rBV3	16299	17476	0.33%	0.037%
40	19.557	2793	2800	2808	rBV2	3785451	5304544	100.00%	11.231%
41	20.569	2969	2972	2975	rVB2	33306	37365	0.70%	0.079%
42	21.351	3099	3105	3112	rBV	1860314	2464397	46.46%	5.218%
43	22.968	3377	3380	3386	rVB	79172	116238	2.19%	0.246%
44	23.515	3465	3473	3480	rBV2	1986045	4159584	78.42%	8.807%
45	23.663	3491	3498	3508	rVB2	999897	2053265	38.71%	4.347%
46	24.251	3595	3598	3604	rVB	109554	177806	3.35%	0.376%




Sum of corrected areas: 47230372

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020216.D
Acq On : 16 Jun 2022 22:08
Operator : CG/JU
Sample : N3294-12
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

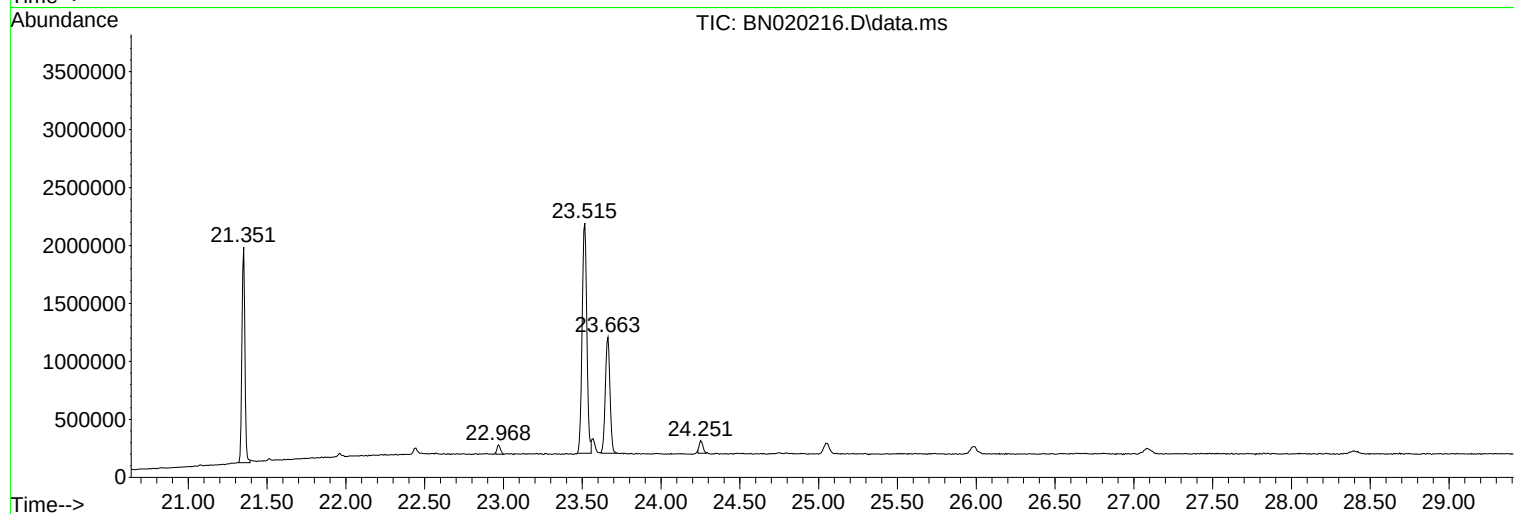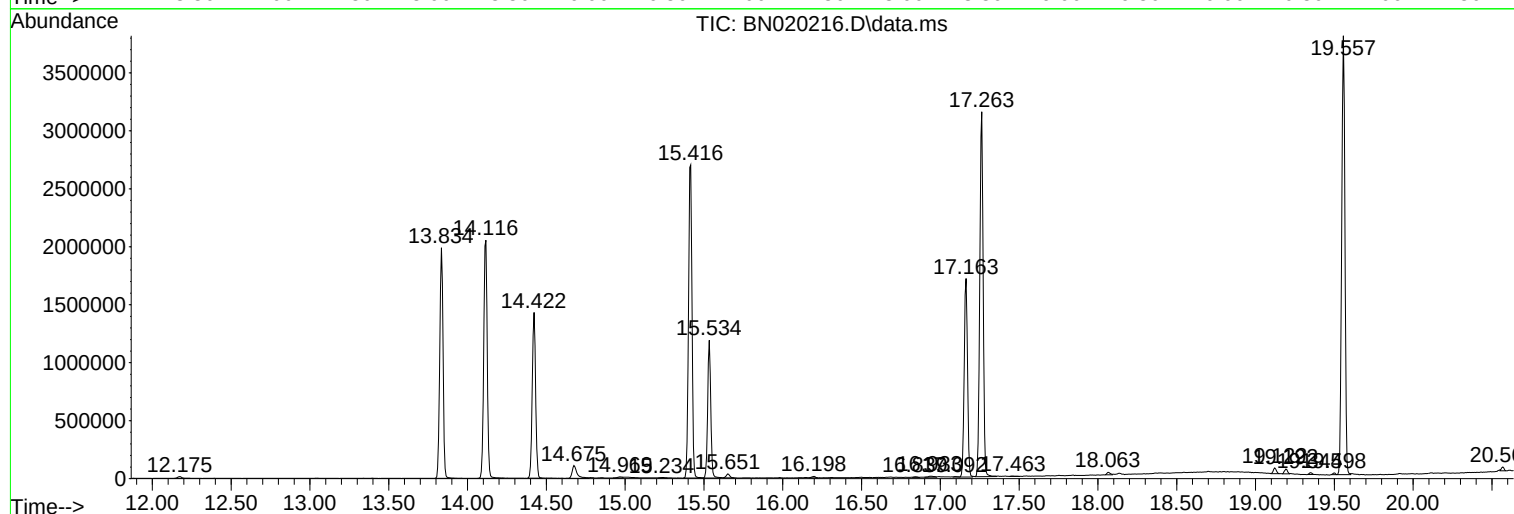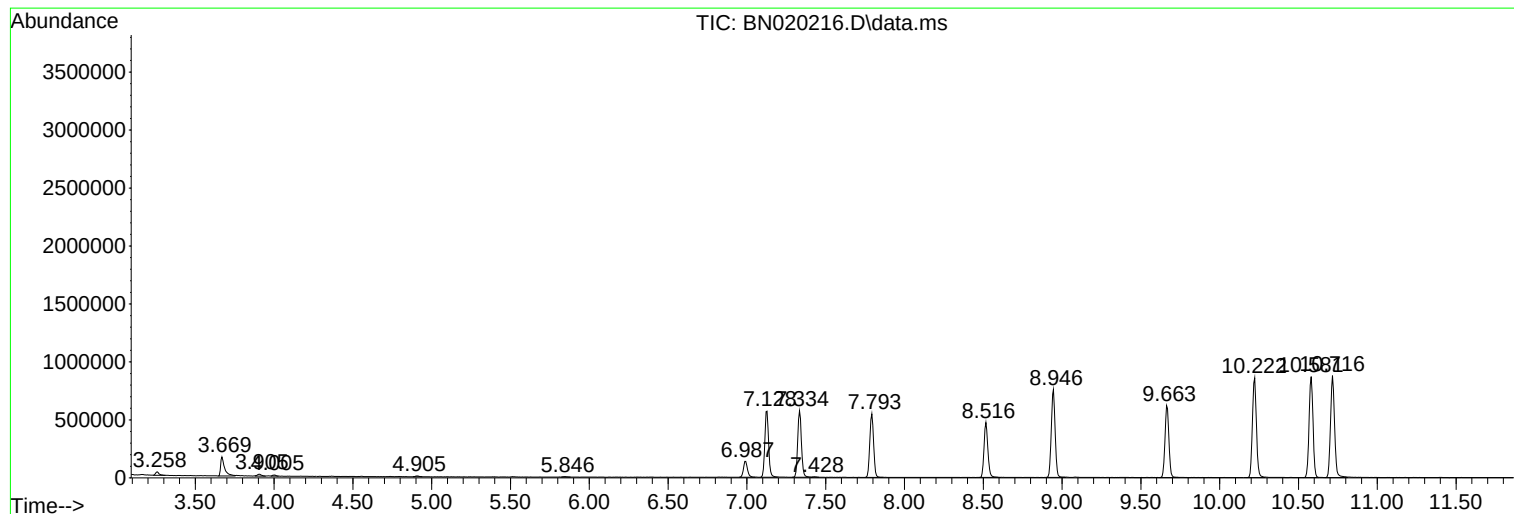

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020216.D
Acq On : 16 Jun 2022 22:08
Operator : CG/JU
Sample : N3294-12
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020216.D
Acq On : 16 Jun 2022 22:08
Operator : CG/JU
Sample : N3294-12
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------