

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020219.D
 Acq On : 16 Jun 2022 23:57
 Operator : CG/JU
 Sample : N3294-17
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4R0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	38	rVB	28459	46097	1.00%	0.108%
2	3.670	96	99	115	rBV	133197	234297	5.08%	0.550%
3	3.828	124	126	131	rVV4	3742	5987	0.13%	0.014%
4	3.905	134	139	146	rVB	13221	23337	0.51%	0.055%
5	3.999	151	155	162	rVB	11082	19627	0.43%	0.046%
6	4.546	245	248	254	rBV6	3083	5212	0.11%	0.012%
7	4.911	305	310	312	rBV2	6662	8115	0.18%	0.019%
8	5.511	411	412	420	rVB8	3517	6295	0.14%	0.015%
9	6.987	657	663	675	rBV	128918	227893	4.94%	0.535%
10	7.122	679	686	697	rBV	508593	861969	18.70%	2.023%
11	7.210	697	701	706	rVB4	3818	7023	0.15%	0.016%
12	7.334	715	722	736	rBV	515267	869872	18.87%	2.042%
13	7.793	792	800	808	rBV	493454	825636	17.91%	1.938%
14	7.869	808	813	817	rVB3	4537	6486	0.14%	0.015%
15	8.516	916	923	937	rBV	443232	753689	16.35%	1.769%
16	8.946	987	996	1007	rBV	677308	1156470	25.09%	2.715%
17	9.087	1016	1020	1025	rBV4	6823	11894	0.26%	0.028%
18	9.663	1110	1118	1134	rBV	566517	956226	20.74%	2.245%
19	9.922	1157	1162	1172	rVV2	8824	18498	0.40%	0.043%
20	10.222	1205	1213	1226	rBV	777770	1385525	30.06%	3.252%
21	10.581	1266	1274	1283	rVB	813863	1379507	29.93%	3.238%
22	10.716	1289	1297	1310	rBV	702740	1255207	27.23%	2.946%
23	11.393	1408	1412	1417	rBV6	4708	9144	0.20%	0.021%
24	12.169	1537	1544	1553	rVB	16645	28123	0.61%	0.066%
25	12.710	1630	1636	1643	rBV5	7670	15886	0.34%	0.037%
26	13.040	1689	1692	1699	rVB5	3679	4964	0.11%	0.012%
27	13.263	1723	1730	1734	rVB4	3603	5310	0.12%	0.012%
28	13.834	1820	1827	1839	rBV	1797749	2483842	53.88%	5.830%
29	14.110	1866	1874	1891	rBV	1804502	2851473	61.86%	6.693%
30	14.222	1891	1893	1899	rVB5	4445	7035	0.15%	0.017%
31	14.422	1920	1927	1936	rBV	1245467	1946508	42.23%	4.569%
32	14.675	1960	1970	1978	rBV	105061	205730	4.46%	0.483%
33	14.787	1986	1989	1993	rVB5	5134	7137	0.15%	0.017%
34	14.845	1993	1999	2006	rVB9	7418	13786	0.30%	0.032%
35	14.957	2012	2018	2026	rBV2	14300	39987	0.87%	0.094%
36	15.234	2060	2065	2071	rVB2	13402	19253	0.42%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020219.D
 Acq On : 16 Jun 2022 23:57
 Operator : CG/JU
 Sample : N3294-17
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4R0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	15.410	2088	2095	2106	rBV	2382805	3645262	79.08%	8.556%
38	15.534	2109	2116	2126	rBV	1009061	1389461	30.14%	3.261%
39	15.651	2131	2136	2142	rVB	30925	48914	1.06%	0.115%
40	15.981	2188	2192	2193	rBV3	3410	4991	0.11%	0.012%
41	16.116	2208	2215	2217	rBV8	3809	8325	0.18%	0.020%
42	16.198	2225	2229	2232	rVB3	8458	12444	0.27%	0.029%
43	16.316	2244	2249	2256	rBV8	3743	7365	0.16%	0.017%
44	16.492	2274	2279	2282	rBV7	3829	8374	0.18%	0.020%
45	16.681	2309	2311	2314	rVV4	5137	5475	0.12%	0.013%
46	16.769	2323	2326	2330	rVB6	3708	5001	0.11%	0.012%
47	16.845	2335	2339	2342	rBV5	7230	10968	0.24%	0.026%
48	16.939	2348	2355	2360	rBV9	9277	24005	0.52%	0.056%
49	17.163	2386	2393	2402	rBV	1517771	2328460	50.51%	5.466%
50	17.263	2403	2410	2423	rVV2	2684953	4080538	88.52%	9.578%
51	17.845	2505	2509	2514	rVB	99919	123686	2.68%	0.290%
52	18.069	2542	2547	2554	rBV	97169	161708	3.51%	0.380%
53	19.022	2706	2709	2721	rVB2	49940	82763	1.80%	0.194%
54	19.122	2723	2726	2734	rVB2	45487	64142	1.39%	0.151%
55	19.192	2734	2738	2743	rBV	40372	54846	1.19%	0.129%
56	19.351	2761	2765	2777	rVB2	67642	105223	2.28%	0.247%
57	19.498	2787	2790	2793	rBV4	16121	19416	0.42%	0.046%
58	19.557	2794	2800	2807	rBV2	3331541	4609732	100.00%	10.820%
59	20.569	2966	2972	2977	rBV3	42314	68891	1.49%	0.162%
60	21.039	3049	3052	3055	rBV2	41913	45680	0.99%	0.107%
61	21.086	3057	3060	3068	rVB5	48222	86787	1.88%	0.204%
62	21.351	3100	3105	3115	rBV	1763852	2319631	50.32%	5.445%
63	23.515	3466	3473	3480	rBV2	1864017	3651734	79.22%	8.572%
64	23.663	3491	3498	3510	rVB2	960256	1925707	41.77%	4.520%




Sum of corrected areas: 42602569

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020219.D
Acq On : 16 Jun 2022 23:57
Operator : CG/JU
Sample : N3294-17
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4R0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

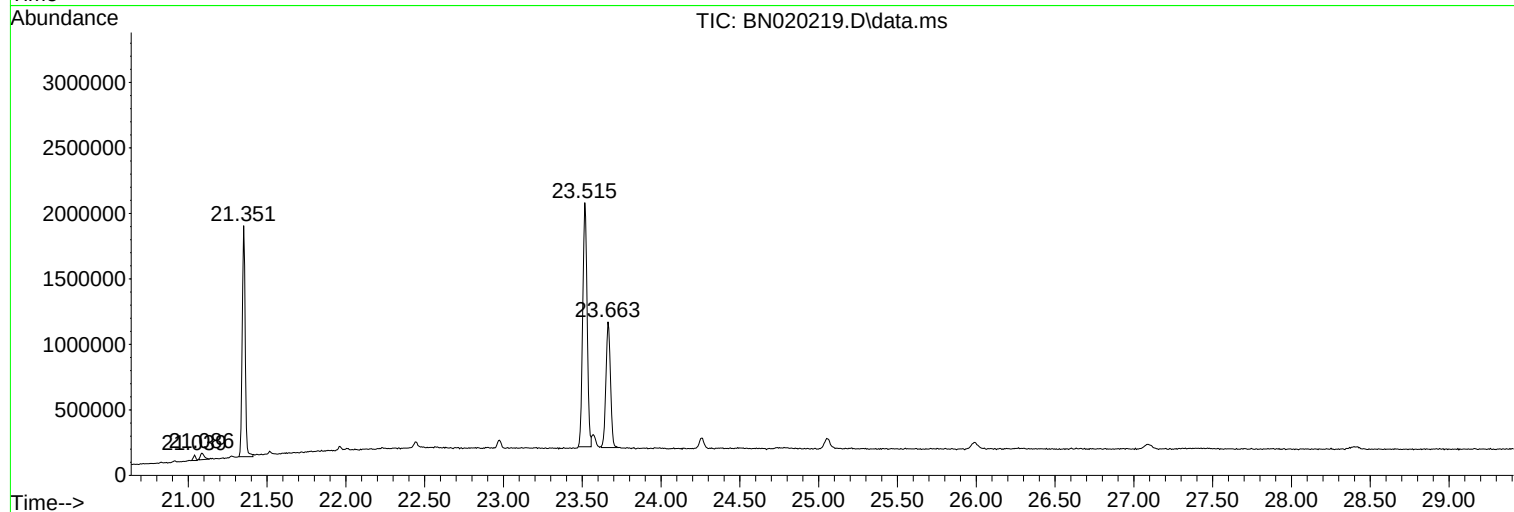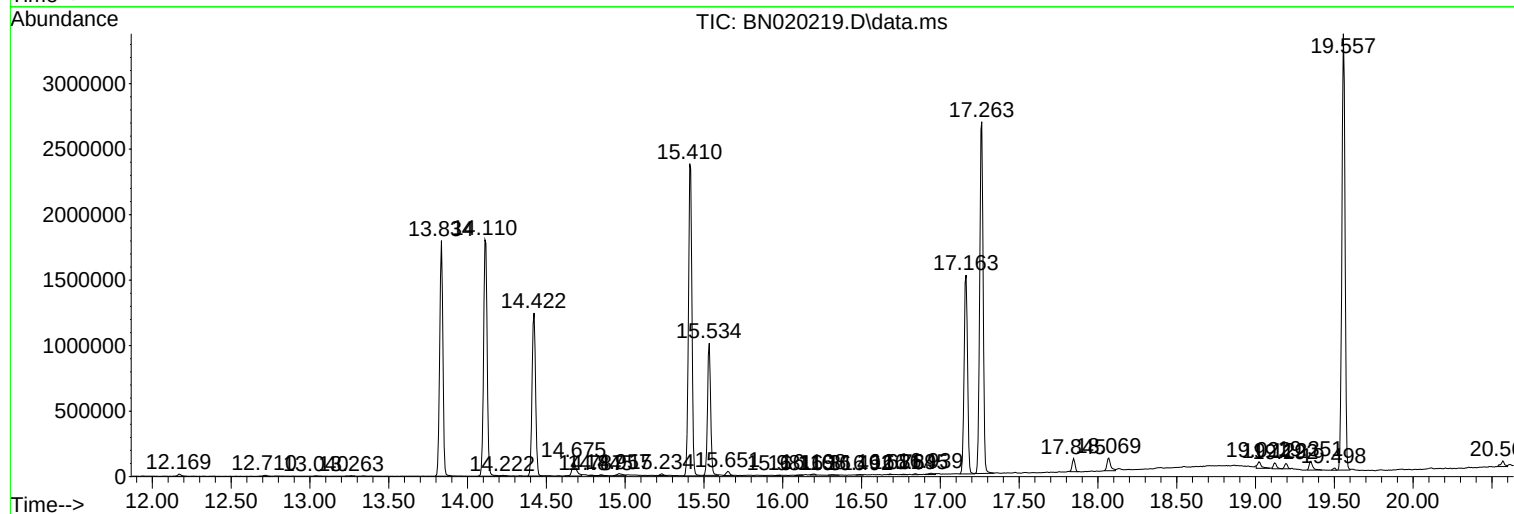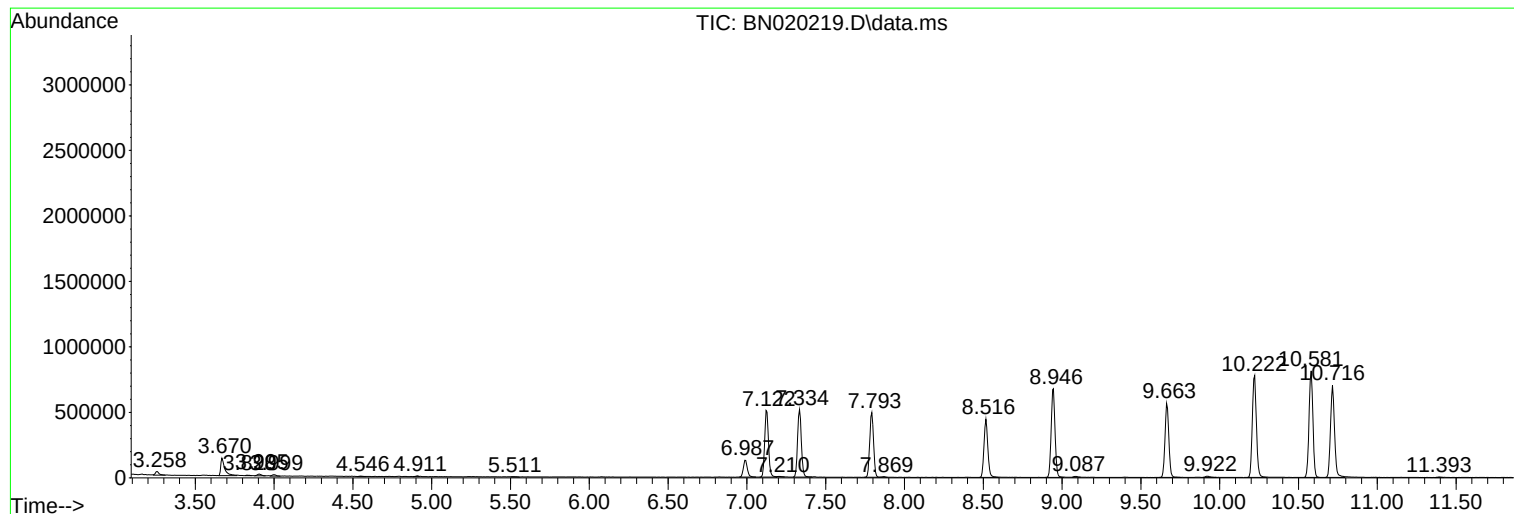

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020219.D
Acq On : 16 Jun 2022 23:57
Operator : CG/JU
Sample : N3294-17
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4R0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020219.D
Acq On : 16 Jun 2022 23:57
Operator : CG/JU
Sample : N3294-17
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4R0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc