

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020220.D
 Acq On : 17 Jun 2022 00:33
 Operator : CG/JU
 Sample : N3294-10
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	39	rVB	32879	51872	0.98%	0.111%
2	3.670	95	99	115	rBV	165710	298702	5.63%	0.638%
3	3.905	134	139	146	rBV	18744	33588	0.63%	0.072%
4	3.999	152	155	160	rVB2	11733	16462	0.31%	0.035%
5	4.905	305	309	315	rVB2	7734	13238	0.25%	0.028%
6	5.517	410	413	420	rVB3	4215	7581	0.14%	0.016%
7	5.846	465	469	477	rVB6	5236	9241	0.17%	0.020%
8	6.987	657	663	679	rVB	173214	298247	5.62%	0.637%
9	7.122	680	686	699	rBV	554268	923380	17.41%	1.973%
10	7.334	715	722	733	rBV	591940	978843	18.45%	2.091%
11	7.422	736	737	745	rVB5	4137	6014	0.11%	0.013%
12	7.793	793	800	808	rBV	507596	835900	15.76%	1.786%
13	8.516	916	923	936	rBV	542060	901655	17.00%	1.926%
14	8.946	988	996	1009	rBV	725897	1231164	23.21%	2.631%
15	9.087	1015	1020	1033	rVB4	5966	13324	0.25%	0.028%
16	9.663	1111	1118	1138	rBV	609635	1024943	19.32%	2.190%
17	10.222	1205	1213	1228	rBV	827894	1492505	28.13%	3.189%
18	10.581	1266	1274	1286	rVB	799860	1381151	26.04%	2.951%
19	10.716	1289	1297	1311	rBV	815483	1462760	27.57%	3.125%
20	11.940	1500	1505	1510	rBV2	7550	12061	0.23%	0.026%
21	12.175	1535	1545	1553	rBV	15143	27144	0.51%	0.058%
22	13.834	1820	1827	1840	rBV	1883156	2657469	50.09%	5.678%
23	14.110	1867	1874	1887	rBV	1895088	2993951	56.44%	6.397%
24	14.422	1920	1927	1935	rBV	1272611	1954357	36.84%	4.176%
25	14.504	1938	1941	1950	rVB6	3963	8085	0.15%	0.017%
26	14.669	1963	1969	1986	rBV	143949	306210	5.77%	0.654%
27	14.787	1986	1989	1994	rVV5	5889	10904	0.21%	0.023%
28	14.851	1994	2000	2004	rVB4	10142	16312	0.31%	0.035%
29	15.234	2060	2065	2070	rVV3	7807	12662	0.24%	0.027%
30	15.410	2086	2095	2106	rBV	2638588	3933805	74.15%	8.405%
31	15.534	2109	2116	2131	rVV	1177225	1614262	30.43%	3.449%
32	15.651	2131	2136	2142	rVB2	32040	49942	0.94%	0.107%
33	16.145	2217	2220	2224	rBV4	3623	5946	0.11%	0.013%
34	16.198	2224	2229	2236	rVB4	10183	17435	0.33%	0.037%
35	16.839	2336	2338	2343	rVB6	4302	5751	0.11%	0.012%
36	16.939	2350	2355	2361	rBV4	8389	16328	0.31%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020220.D
 Acq On : 17 Jun 2022 00:33
 Operator : CG/JU
 Sample : N3294-10
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	17.163	2386	2393	2402	rBV	1540008	2345068	44.21%	5.011%
38	17.263	2402	2410	2424	rBV	3077317	4678098	88.18%	9.995%
39	17.763	2489	2495	2497	rBV4	3723	6887	0.13%	0.015%
40	17.845	2504	2509	2513	rBV6	12085	18635	0.35%	0.040%
41	18.063	2541	2546	2554	rBV	96304	147407	2.78%	0.315%
42	18.134	2554	2558	2566	rVB	36151	52882	1.00%	0.113%
43	18.545	2625	2628	2635	rVB6	4491	7086	0.13%	0.015%
44	18.998	2702	2705	2710	rBV7	3707	5796	0.11%	0.012%
45	19.122	2721	2726	2732	rBV	43270	62924	1.19%	0.134%
46	19.192	2733	2738	2744	rBV	41434	66385	1.25%	0.142%
47	19.351	2759	2765	2772	rBV	70045	112520	2.12%	0.240%
48	19.504	2787	2791	2793	rBV4	15800	18713	0.35%	0.040%
49	19.557	2794	2800	2808	rBV	3769783	5304918	100.00%	11.335%
50	20.569	2966	2972	2976	rBV2	36244	56599	1.07%	0.121%
51	21.086	3056	3060	3068	rBV5	49092	106139	2.00%	0.227%
52	21.351	3099	3105	3112	rBV	1909523	2442859	46.05%	5.219%
53	23.516	3465	3473	3480	rBV2	2178135	4475772	84.37%	9.563%
54	23.663	3491	3498	3511	rVB	1067599	2083238	39.27%	4.451%
55	24.257	3595	3599	3606	rVB	95350	187679	3.54%	0.401%




Sum of corrected areas: 46802799

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020220.D
Acq On : 17 Jun 2022 00:33
Operator : CG/JU
Sample : N3294-10
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

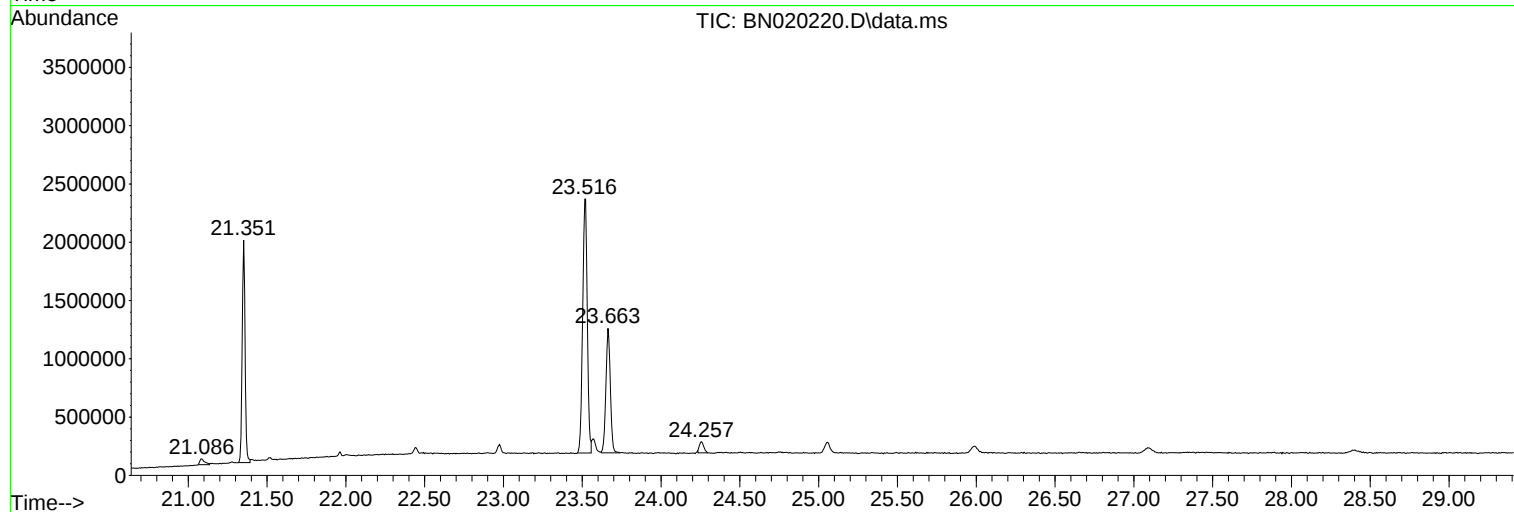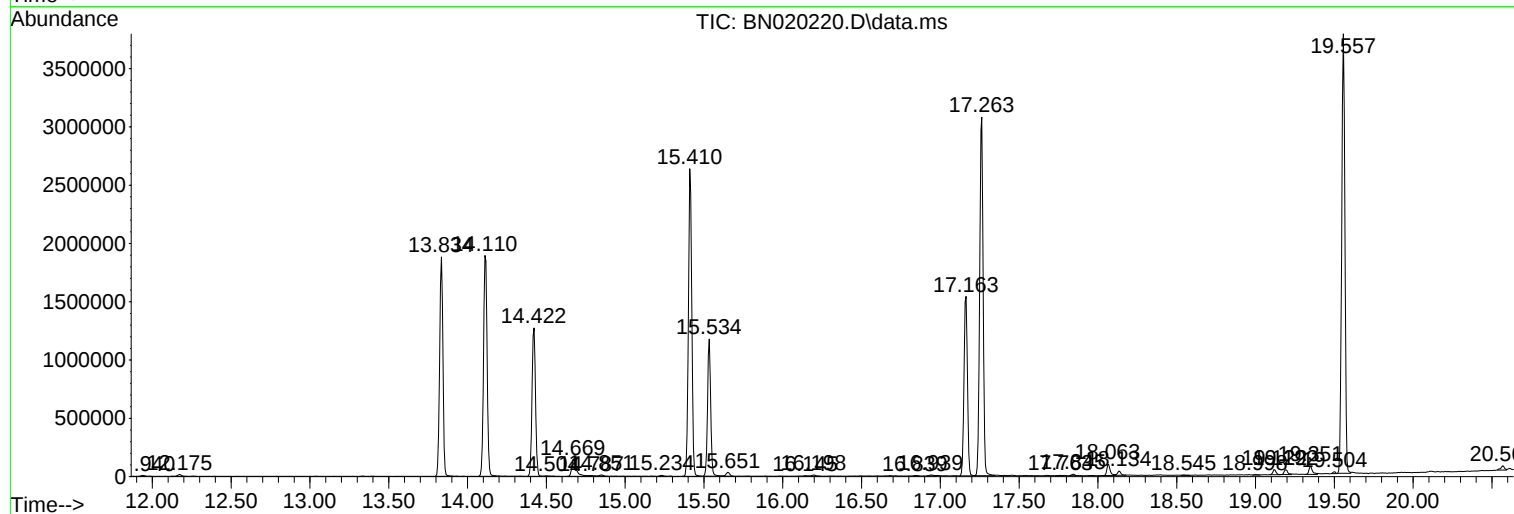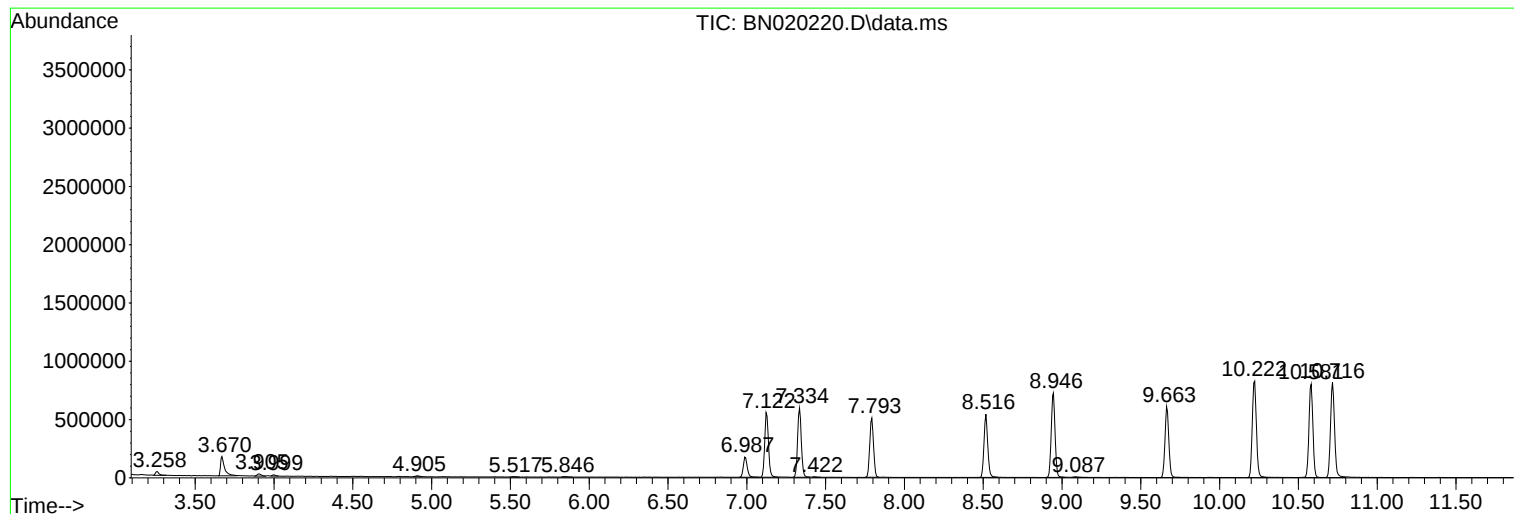

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020220.D
Acq On : 17 Jun 2022 00:33
Operator : CG/JU
Sample : N3294-10
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020220.D
Acq On : 17 Jun 2022 00:33
Operator : CG/JU
Sample : N3294-10
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------