

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
 Data File : BN020225.D
 Acq On : 17 Jun 2022 04:08
 Operator : CG/JU
 Sample : PB145553BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK553

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	41	rVB	38211	65499	1.55%	0.150%
2	3.664	94	98	119	rBV	473280	821214	19.48%	1.882%
3	3.999	152	155	167	rVB2	10770	20537	0.49%	0.047%
4	6.987	656	663	680	rBV	579440	1001416	23.76%	2.295%
5	7.122	680	686	700	rVB	483909	807984	19.17%	1.851%
6	7.334	715	722	736	rVB	624523	1051866	24.96%	2.410%
7	7.793	793	800	809	rBV	512654	863599	20.49%	1.979%
8	8.516	916	923	938	rBV	782216	1339555	31.78%	3.069%
9	8.940	988	995	1015	rBV	608408	1054495	25.02%	2.416%
10	9.663	1111	1118	1131	rBV	538566	900041	21.35%	2.062%
11	10.216	1205	1212	1227	rBV	727371	1318529	31.28%	3.021%
12	10.581	1266	1274	1285	rBV	793075	1387235	32.91%	3.179%
13	10.716	1289	1297	1311	rBV	822423	1473052	34.95%	3.375%
14	12.169	1539	1544	1553	rVB	11368	21049	0.50%	0.048%
15	13.834	1820	1827	1841	rBV	1568835	2224624	52.78%	5.097%
16	14.110	1867	1874	1887	rBV	1728338	2520891	59.81%	5.776%
17	14.422	1919	1927	1934	rBV	1237991	1955652	46.40%	4.481%
18	14.663	1961	1968	1987	rBV	556540	1077972	25.57%	2.470%
19	15.410	2088	2095	2110	rBV	2177062	3227705	76.58%	7.396%
20	15.534	2110	2116	2131	rVV	860223	1212080	28.76%	2.777%
21	15.651	2131	2136	2142	rVB	27552	38786	0.92%	0.089%
22	16.192	2225	2228	2233	rVB4	6935	10820	0.26%	0.025%
23	16.839	2332	2338	2343	rVB7	2915	5120	0.12%	0.012%
24	16.939	2350	2355	2362	rBV7	5683	13411	0.32%	0.031%
25	17.163	2386	2393	2403	rBV	1570405	2379818	56.46%	5.453%
26	17.257	2403	2409	2424	rVV2	2393357	3635081	86.24%	8.329%
27	18.069	2544	2547	2550	rBV5	3808	4476	0.11%	0.010%
28	18.692	2650	2653	2661	rBV9	2841	5974	0.14%	0.014%
29	19.122	2722	2726	2731	rVB2	28102	39850	0.95%	0.091%
30	19.192	2733	2738	2742	rBV	29104	43038	1.02%	0.099%
31	19.357	2761	2766	2770	rBV6	3717	7792	0.18%	0.018%
32	19.498	2786	2790	2793	rBV2	10780	13208	0.31%	0.030%
33	19.557	2793	2800	2812	rVV	2929863	4214984	100.00%	9.658%
34	19.916	2854	2861	2868	rBV6	15045	42362	1.01%	0.097%
35	20.569	2969	2972	2976	rVB	25814	27958	0.66%	0.064%
36	21.351	3099	3105	3116	rBV	1906162	2576113	61.12%	5.903%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020225.D
Acq On : 17 Jun 2022 04:08
Operator : CG/JU
Sample : PB145553BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK553

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	23.516	3465	3473	3480	rBV2	1822763	3757530	89.15%	8.610%
38	23.663	3490	3498	3512	rVB2	1162847	2324499	55.15%	5.326%
39	24.257	3595	3599	3605	rVB3	81349	158145	3.75%	0.362%




Sum of corrected areas: 43643960

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020225.D
Acq On : 17 Jun 2022 04:08
Operator : CG/JU
Sample : PB145553BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK553

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

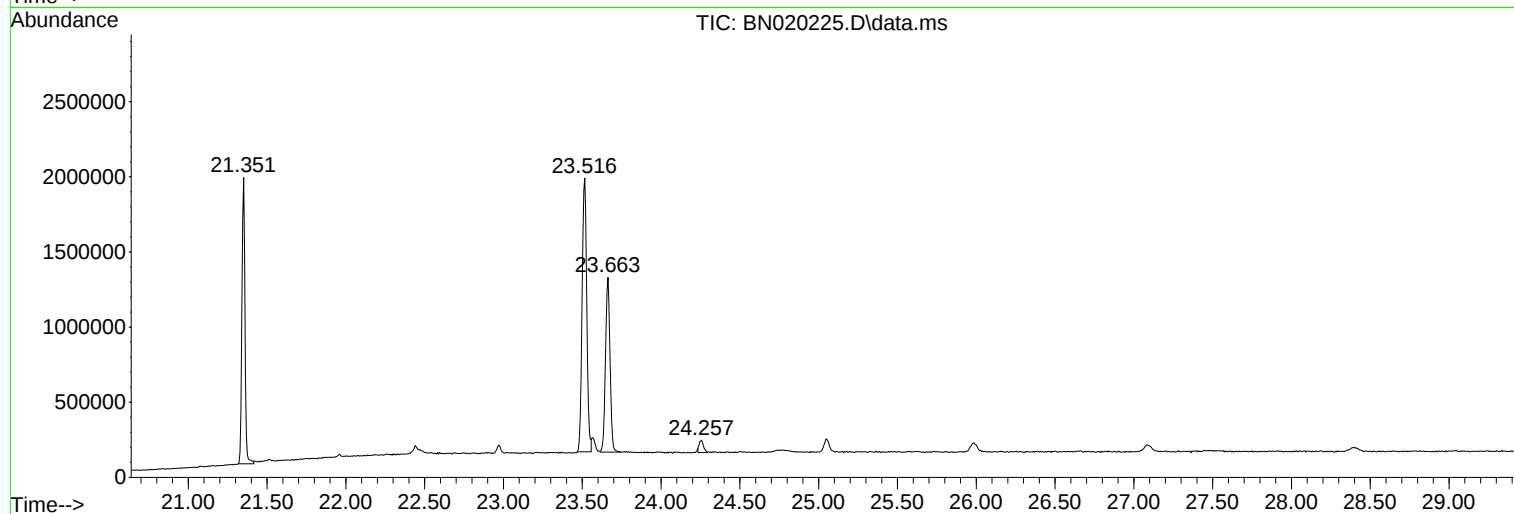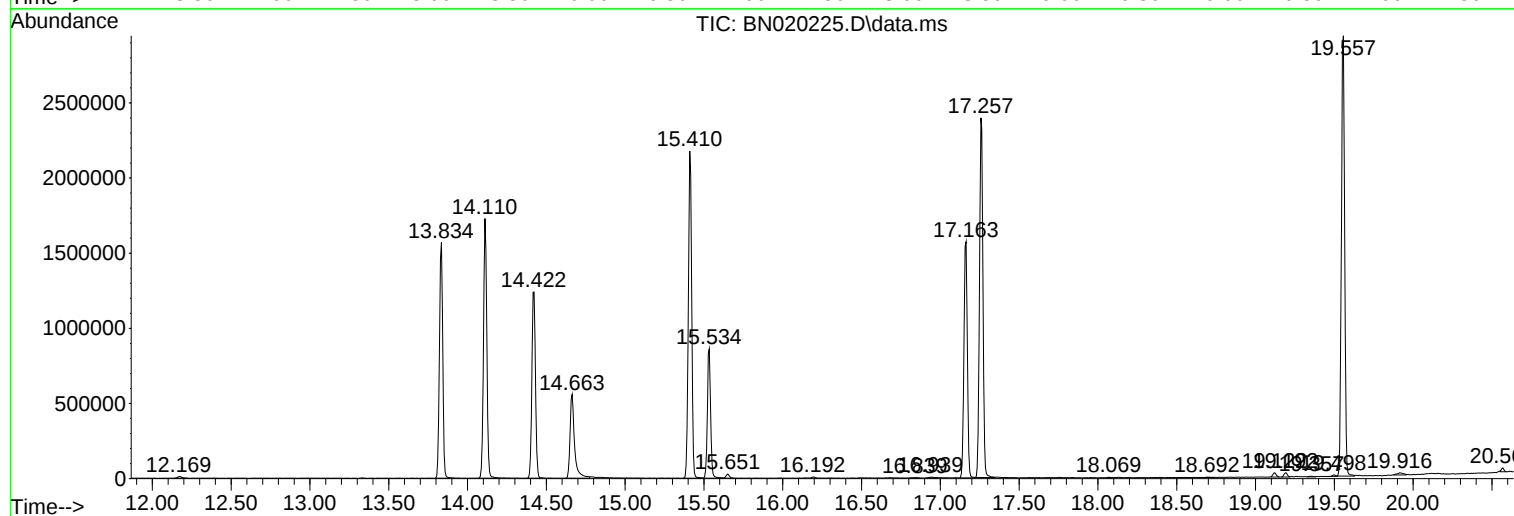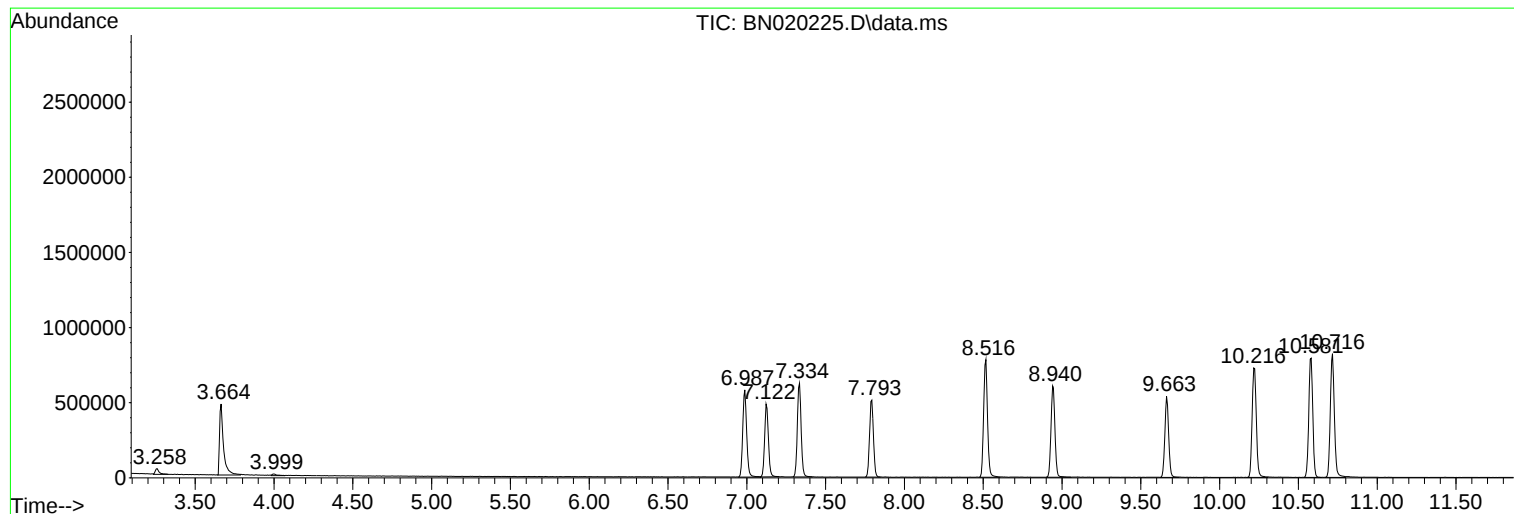

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020225.D
Acq On : 17 Jun 2022 04:08
Operator : CG/JU
Sample : PB145553BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK553

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061522\
Data File : BN020225.D
Acq On : 17 Jun 2022 04:08
Operator : CG/JU
Sample : PB145553BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK553

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc