
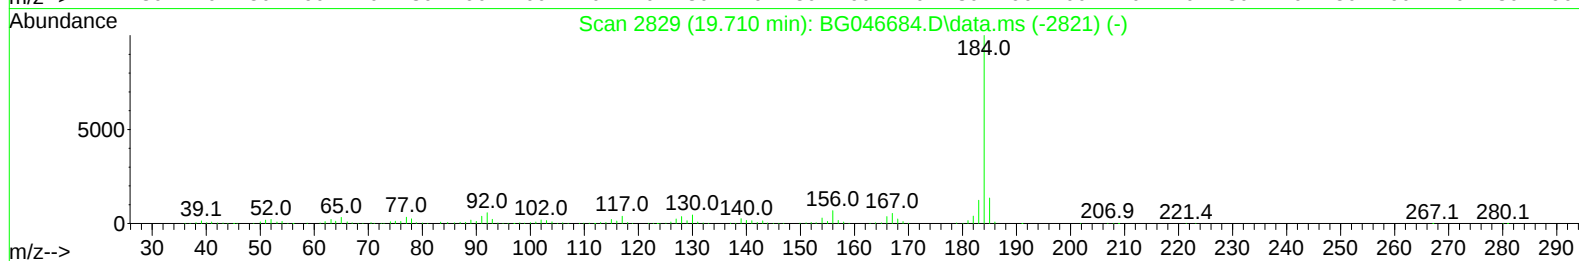
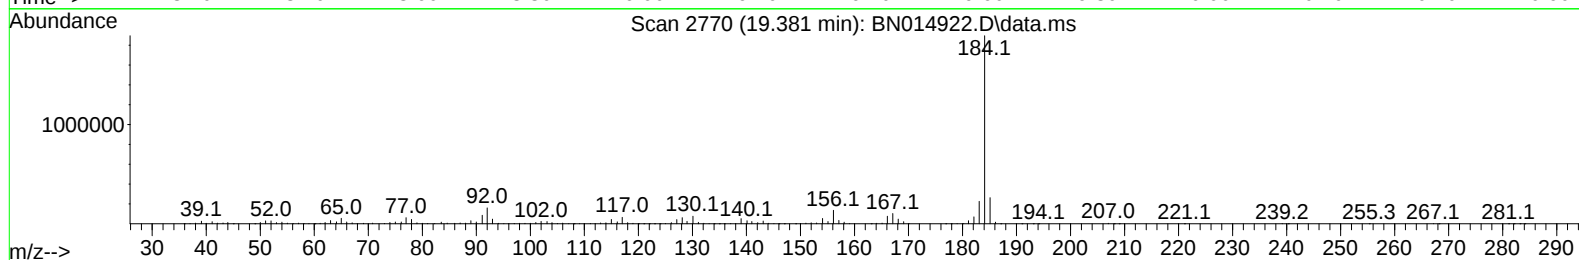


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061621\
 Data File : BN014922.D
 Acq On : 16 Jun 2021 15:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 16:38:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

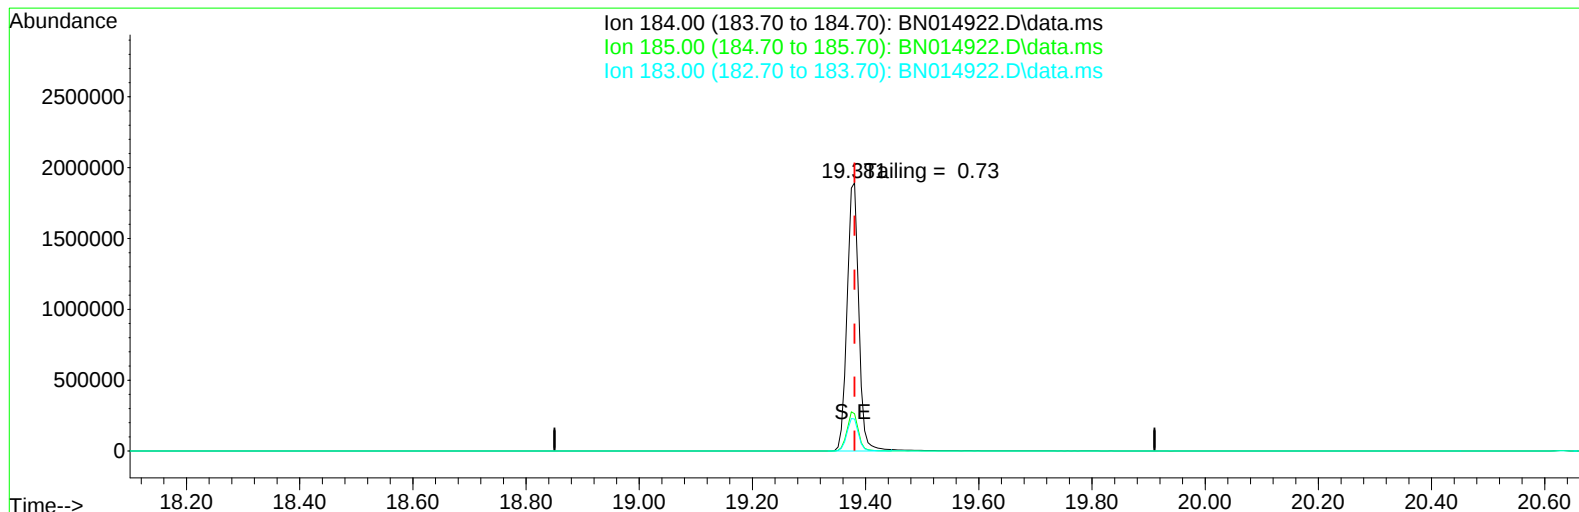

TIC: BN014922.D\data.ms

(77) Benzidine




19.381min (+ 0.000) 384546.92 ng

response 2750082

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.91
183.00	13.20	11.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061621\
 Data File : BN014922.D
 Acq On : 16 Jun 2021 15:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 16:38:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

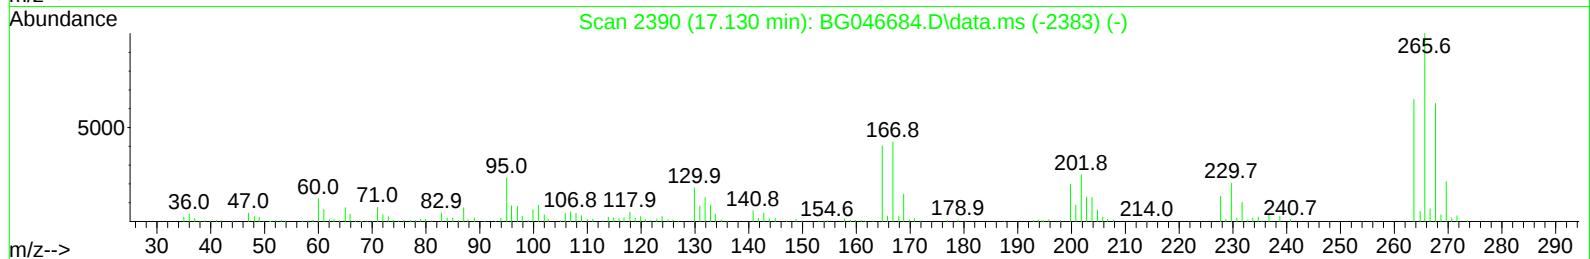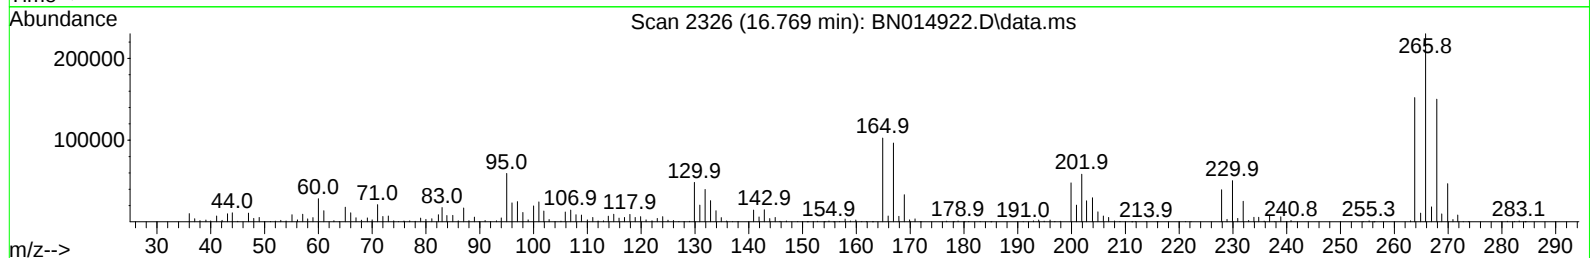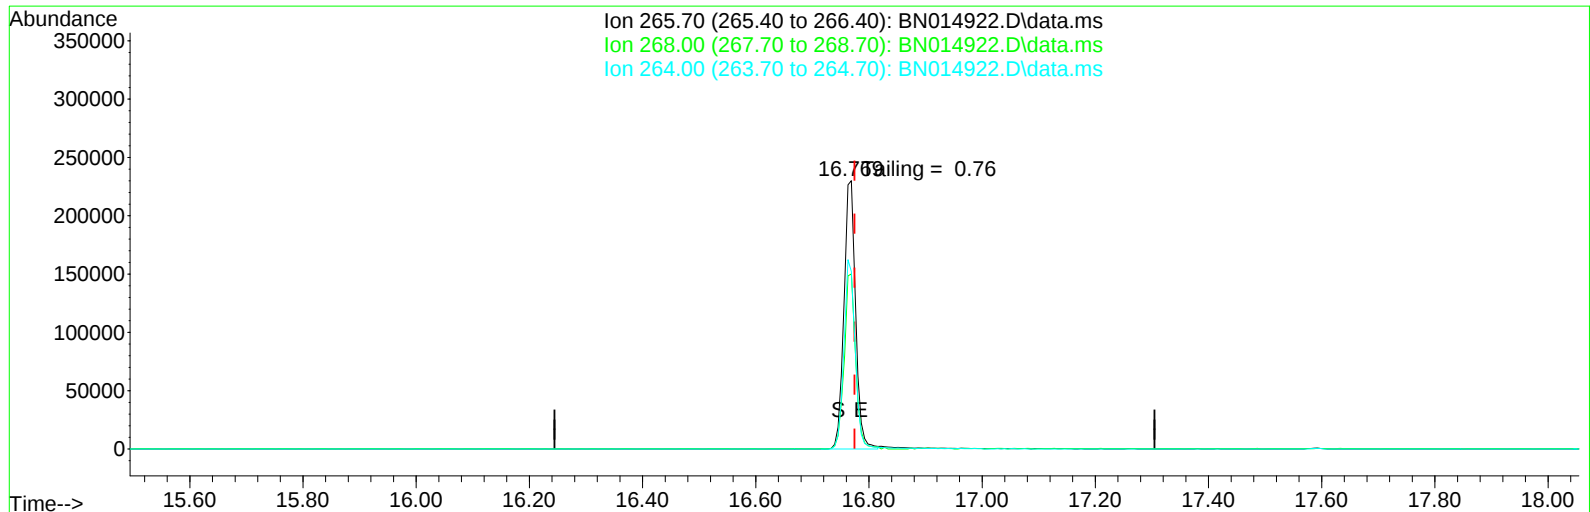

TIC: BN014922.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 25054.91 ng

response 336818

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.21
264.00	61.60	66.10
0.00	0.00	0.00