
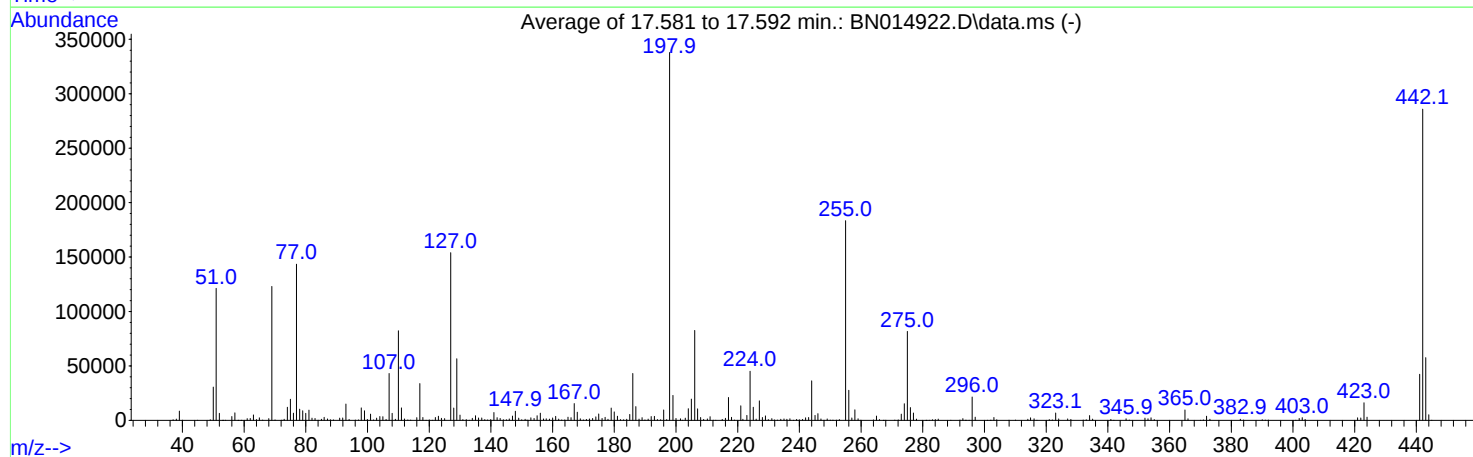


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061621\
 Data File : BN014922.D
 Acq On : 16 Jun 2021 15:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 17 01:26:44 2021

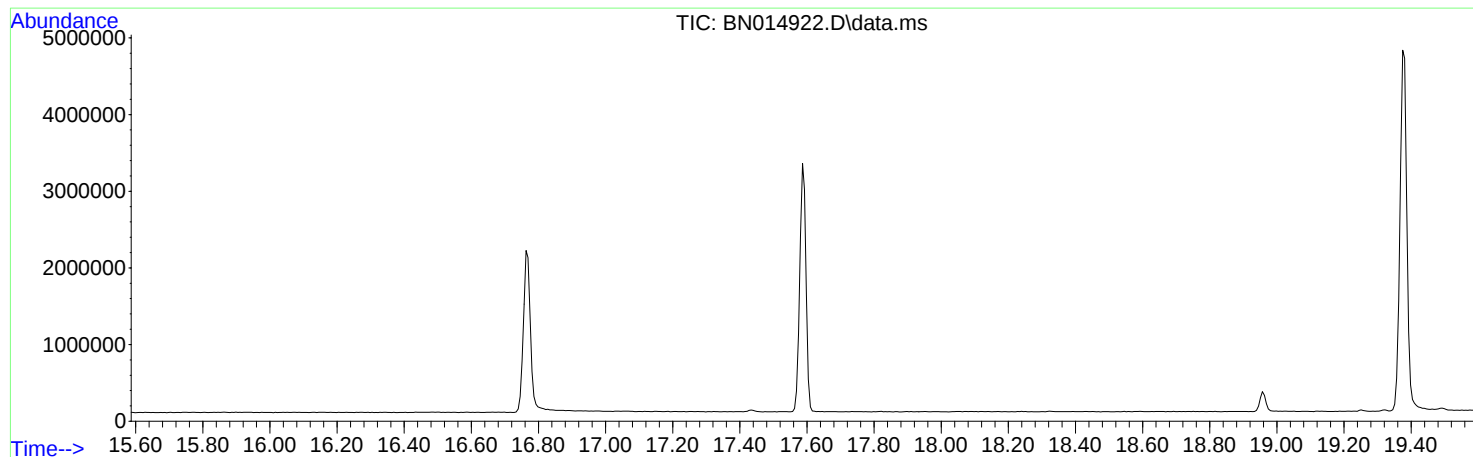




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	121241	PASS
68	69	0.00	2	1.3	1577	PASS
69	198	0.00	100	36.4	123075	PASS
70	69	0.00	2	0.4	488	PASS
127	198	10	80	45.6	153963	PASS
197	198	0.00	2	0.2	706	PASS
198	198	100	100	100.0	337877	PASS
199	198	5	9	6.8	23000	PASS
275	198	10	60	24.2	81691	PASS
365	198	1	100	2.9	9631	PASS
441	198	0.01	100	12.5	42275	PASS
442	442	50	100	100.0	285803	PASS
443	442	15	24	20.2	57651	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061621\
Data File : BN014922.D
Acq On : 16 Jun 2021 15:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 16 16:38:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

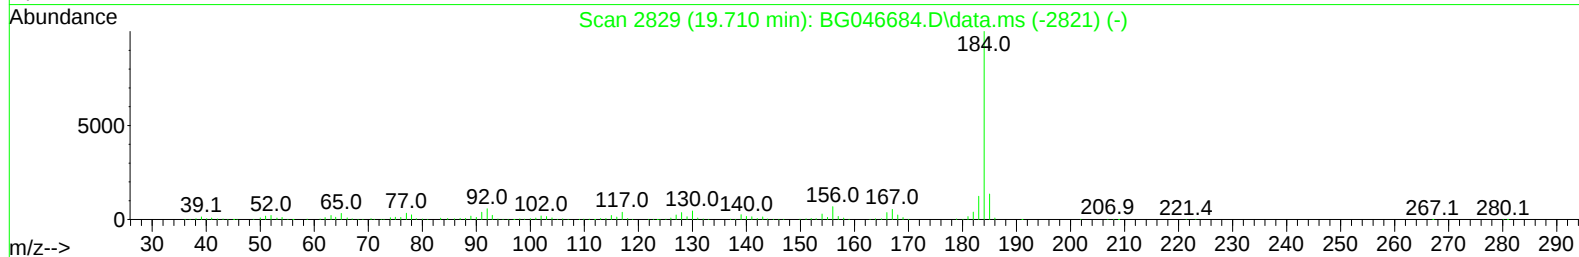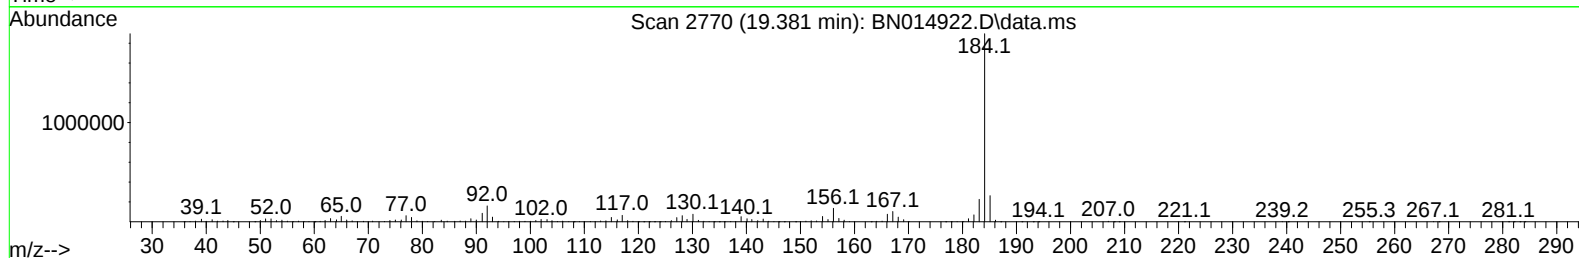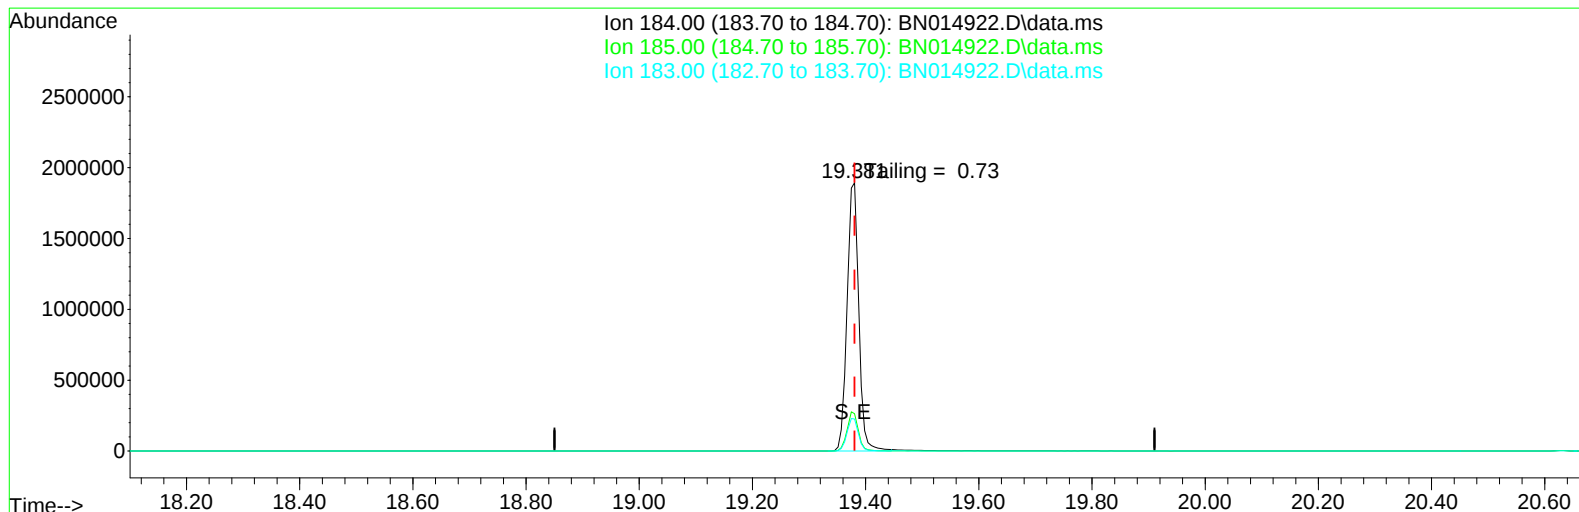

TIC: BN014922.D\data.ms

(77) Benzidine

19.381min (+ 0.000) 384546.92 ng




response 2750082

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.91
183.00	13.20	11.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061621\
 Data File : BN014922.D
 Acq On : 16 Jun 2021 15:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 16 16:38:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

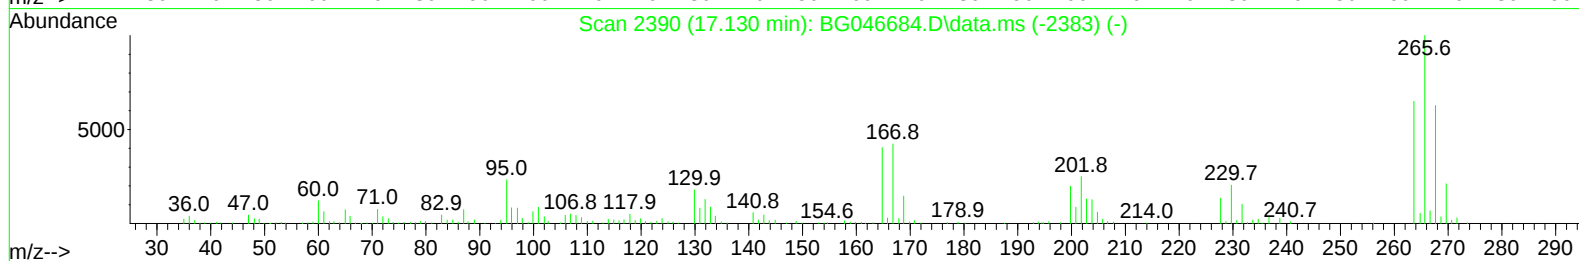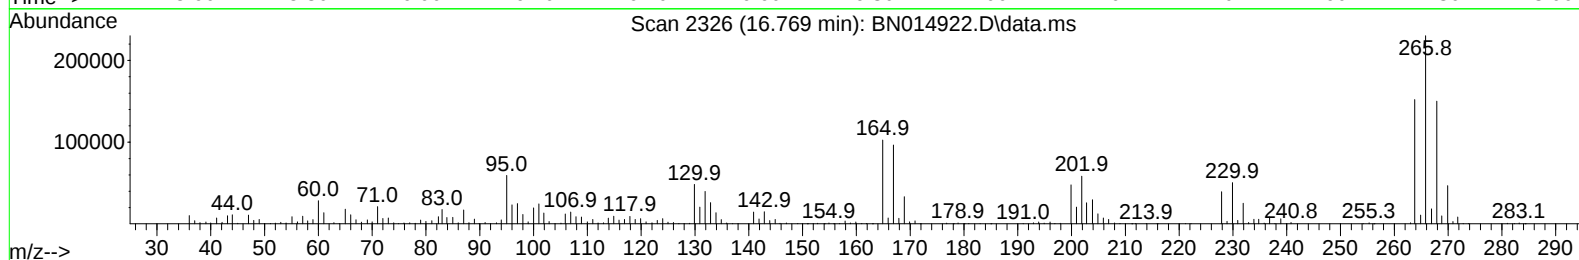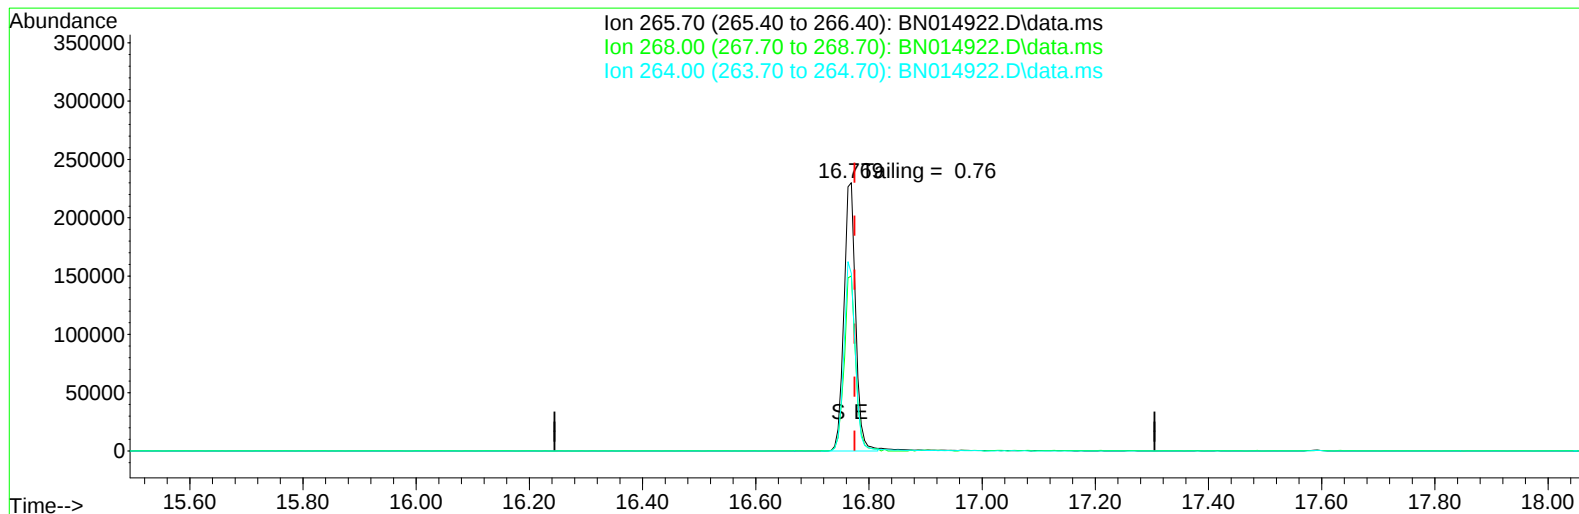

TIC: BN014922.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 25054.91 ng

response 336818

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.21
264.00	61.60	66.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/16/2021	BNA_N	<u>BN014922.D</u>
Compound Name	Response	Retention Time
DDT	1123515	20.62
DDD	13357	20.18
DDE	1948	19.67
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15305	1138820	1.34