


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061625\
Data File : BN037283.D
Acq On : 16 Jun 2025 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 16 03:00:26 2025

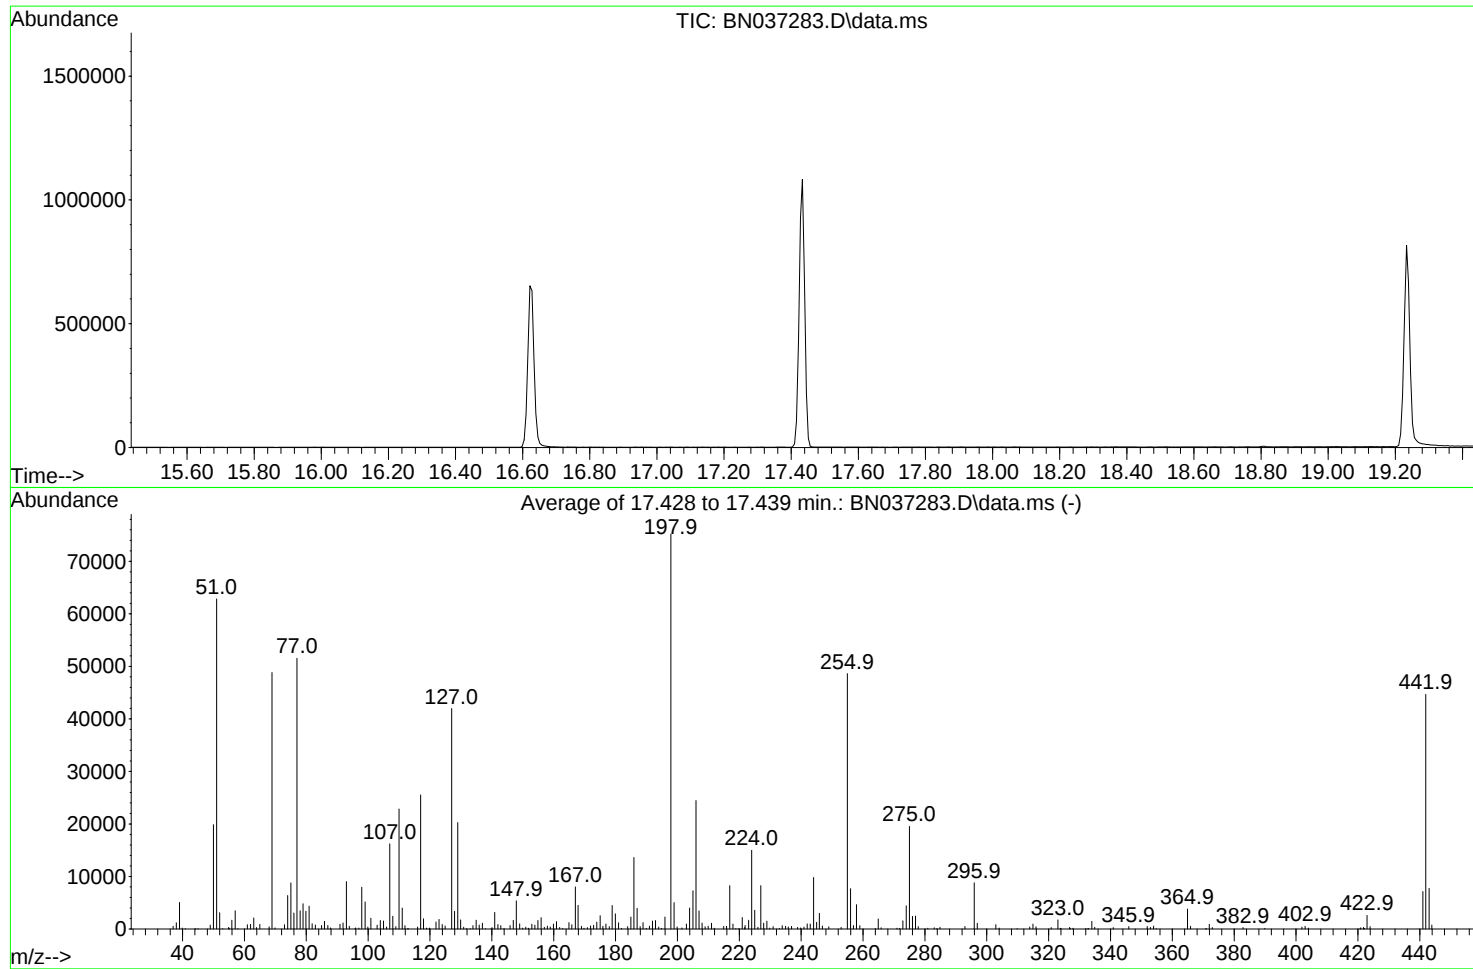




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.9	440	PASS
69	69	100	100	100.0	48840	PASS
70	69	0.00	2	0.4	216	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75176	PASS
199	198	5	9	6.7	5035	PASS
365	198	1	100	5.1	3812	PASS
441	443	0.01	150	92.0	7125	PASS
442	442	100	100	100.0	44672	PASS
443	442	15	24	17.3	7741	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061625\
Data File : BN037283.D
Acq On : 16 Jun 2025 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 16 15:21:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 16 03:00:26 2025
Response via : Initial Calibration

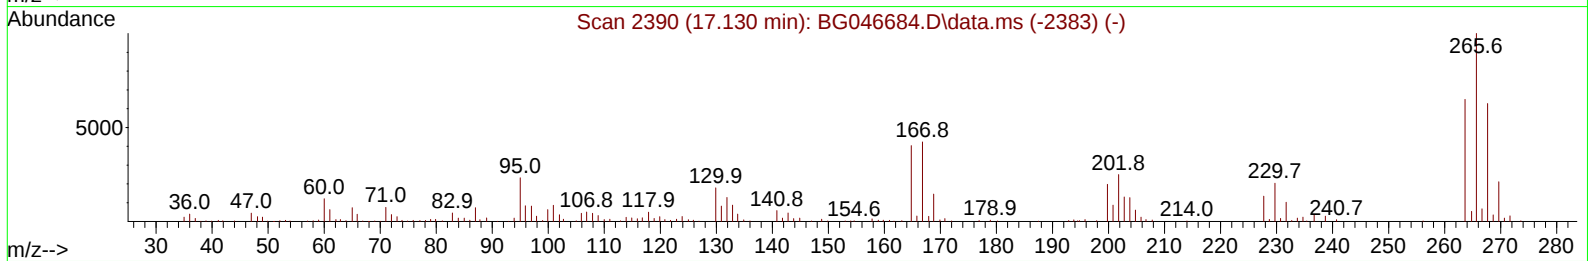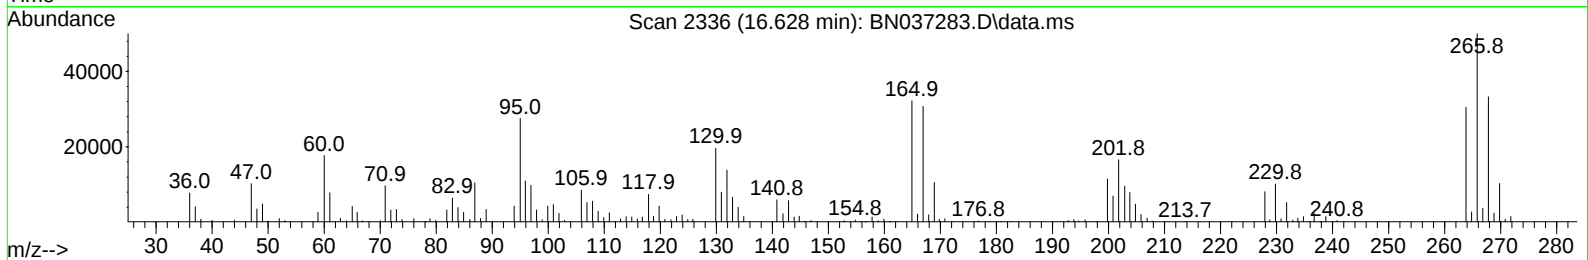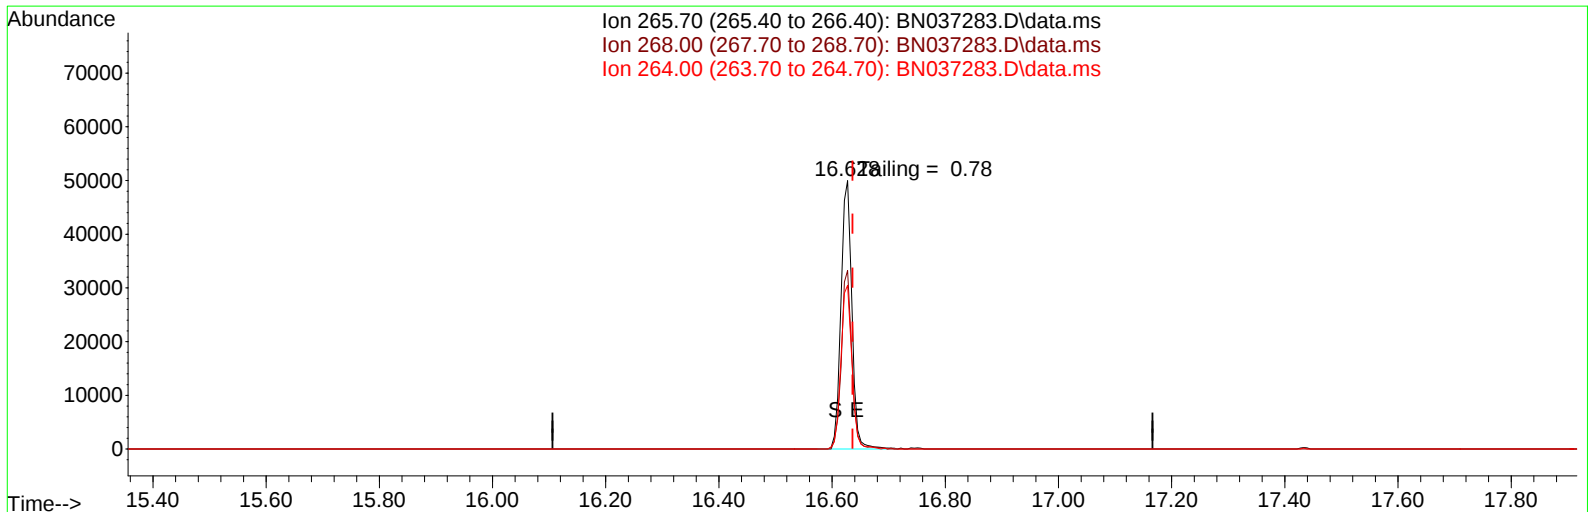

TIC: BN037283.D\data.ms

(70) Pentachlorophenol (C)

16.628min (-0.008) 14961.68 ng




response 66692

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.54
264.00	61.60	61.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061625\
Data File : BN037283.D
Acq On : 16 Jun 2025 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 16 15:21:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 16 03:00:26 2025
Response via : Initial Calibration

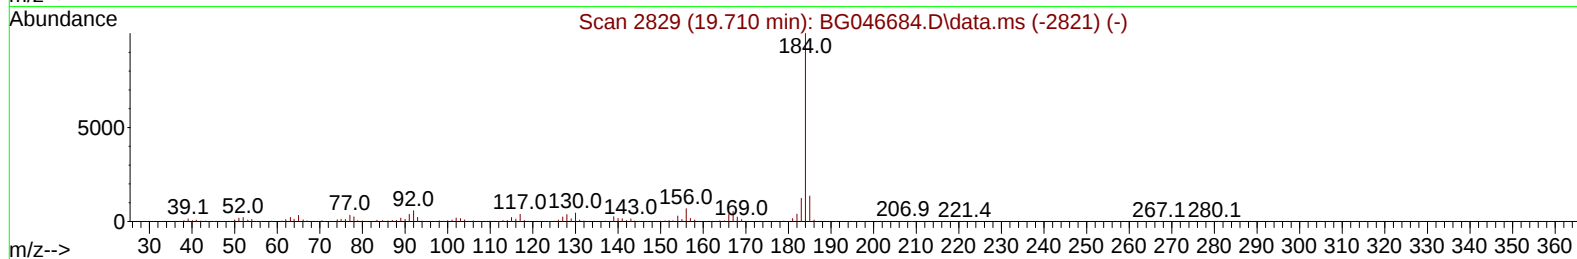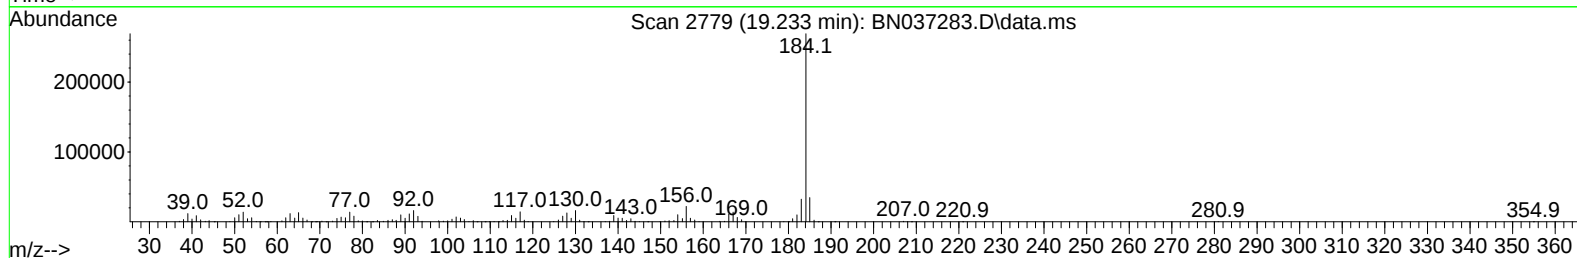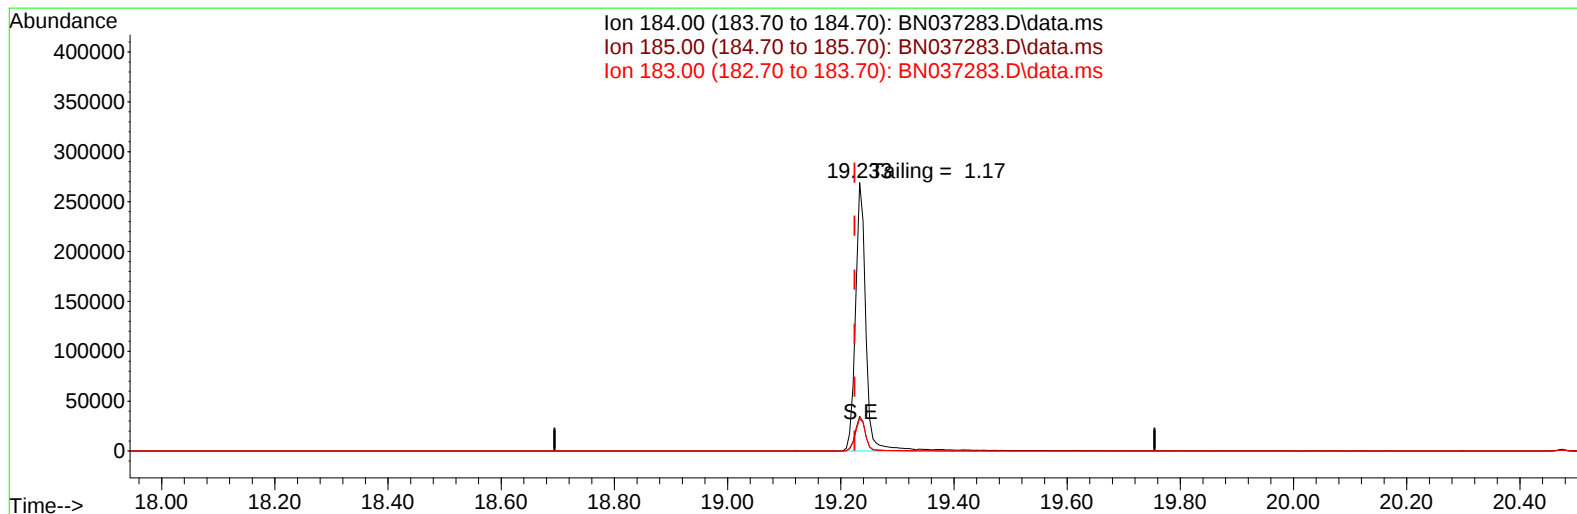

TIC: BN037283.D\data.ms

(77) Benzidine

19.233min (+ 0.009) 0.00 ng

response 337105

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.90
183.00	13.20	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/16/2025	BNA_N	<u>BN037258.D</u>
Compound Name	Response	Retention Time
DDT	229373	20.474
DDD	3011	20.086
DDE	0	0
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3011	232384	1.30

Instrument :
BNA_N
ClientSampleId :
DFTPP