

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061724\
 Data File : BN032029.D
 Acq On : 17 Jun 2024 11:38
 Operator : MA/JU
 Sample : PB161388BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK388

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.170	28	31	41	rVB	63879	92122	1.44%	0.130%
2	3.576	96	100	123	rBV	821028	1290294	20.21%	1.820%
3	3.887	150	153	158	rVB	10950	15214	0.24%	0.021%
4	6.828	646	653	667	rVB	1070781	1719180	26.92%	2.425%
5	6.993	672	681	690	rBV	893834	1409031	22.07%	1.988%
6	7.181	705	713	725	rBV	1093852	1815273	28.43%	2.561%
7	7.652	785	793	806	rBV	870354	1467286	22.98%	2.070%
8	8.358	906	913	930	rBV	1415759	2361900	36.99%	3.332%
9	8.805	980	989	1003	rBV	1056005	1796743	28.14%	2.535%
10	9.522	1104	1111	1121	rBV	921241	1520022	23.80%	2.144%
11	10.058	1192	1202	1225	rBV	1375731	2474228	38.75%	3.490%
12	10.434	1256	1266	1282	rBV	1372029	2377439	37.23%	3.354%
13	10.575	1282	1290	1309	rBV	1474104	2622856	41.07%	3.700%
14	12.028	1532	1537	1548	rBV2	21832	45667	0.72%	0.064%
15	13.257	1743	1746	1750	rBV4	4664	8203	0.13%	0.012%
16	13.716	1816	1824	1834	rBV	2635694	3925503	61.47%	5.538%
17	13.987	1863	1870	1883	rBV	3102730	4847647	75.92%	6.839%
18	14.298	1916	1923	1934	rBV	2311297	3533665	55.34%	4.985%
19	14.516	1953	1960	1982	rBV	963808	1807013	28.30%	2.549%
20	14.657	1982	1984	1990	rVB7	4863	7340	0.11%	0.010%
21	15.293	2085	2092	2103	rBV	3888090	5818680	91.12%	8.209%
22	15.428	2108	2115	2129	rBV	1018754	1487216	23.29%	2.098%
23	15.534	2129	2133	2137	rVB2	20883	33068	0.52%	0.047%
24	15.869	2183	2190	2194	rBV4	3830	7355	0.12%	0.010%
25	16.075	2222	2225	2231	rVB4	3828	6453	0.10%	0.009%
26	16.834	2351	2354	2360	rVB3	6651	7329	0.11%	0.010%
27	17.045	2383	2390	2400	rBV	2828511	4139825	64.83%	5.840%
28	17.145	2400	2407	2425	rVV2	4159348	6246901	97.83%	8.813%
29	17.339	2435	2440	2442	rBV5	5681	9057	0.14%	0.013%
30	17.439	2453	2457	2463	rVB3	5463	7958	0.12%	0.011%
31	17.951	2540	2544	2550	rVB6	7800	13055	0.20%	0.018%
32	19.010	2719	2724	2729	rBV2	54865	79975	1.25%	0.113%
33	19.081	2731	2736	2741	rBV	53939	78265	1.23%	0.110%
34	19.381	2785	2787	2792	rVB4	19207	20415	0.32%	0.029%
35	19.445	2792	2798	2813	rBV	4352527	6385578	100.00%	9.008%
36	21.286	3105	3111	3121	rBV	2170773	3228883	50.57%	4.555%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061724\
Data File : BN032029.D
Acq On : 17 Jun 2024 11:38
Operator : MA/JU
Sample : PB161388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	24.010	3566	3574	3587	rVB2	2000738	4860483	76.12%	6.857%
38	24.210	3600	3608	3620	rVB	1342210	3318084	51.96%	4.681%




Sum of corrected areas: 70885206

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061724\
Data File : BN032029.D
Acq On : 17 Jun 2024 11:38
Operator : MA/JU
Sample : PB161388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

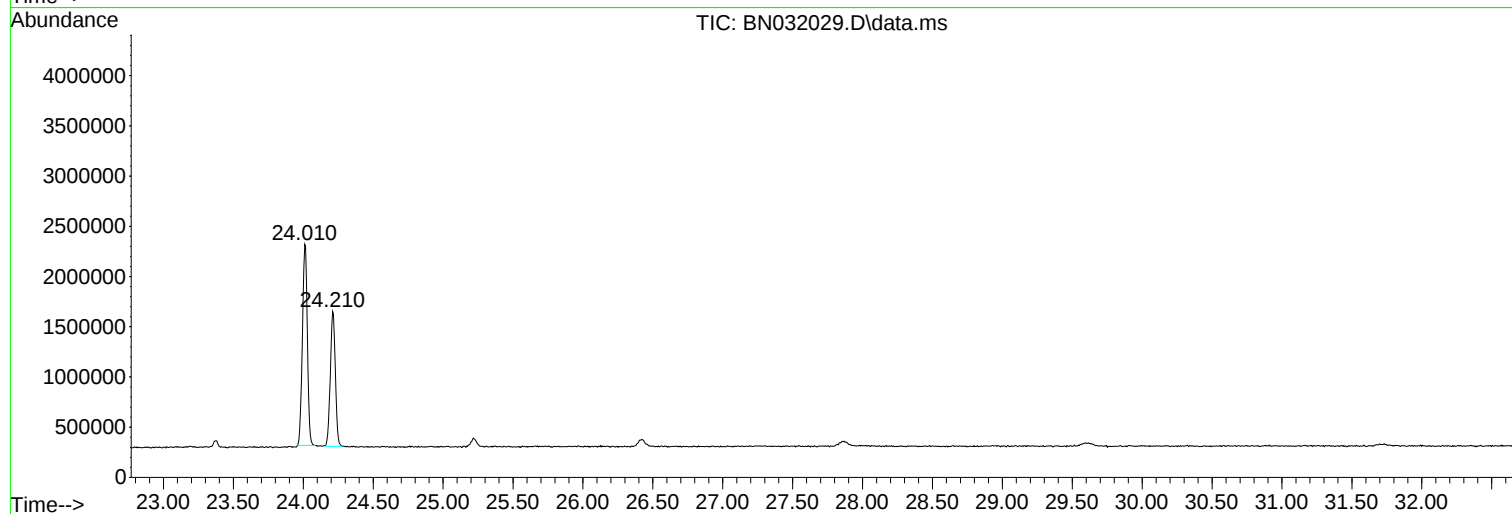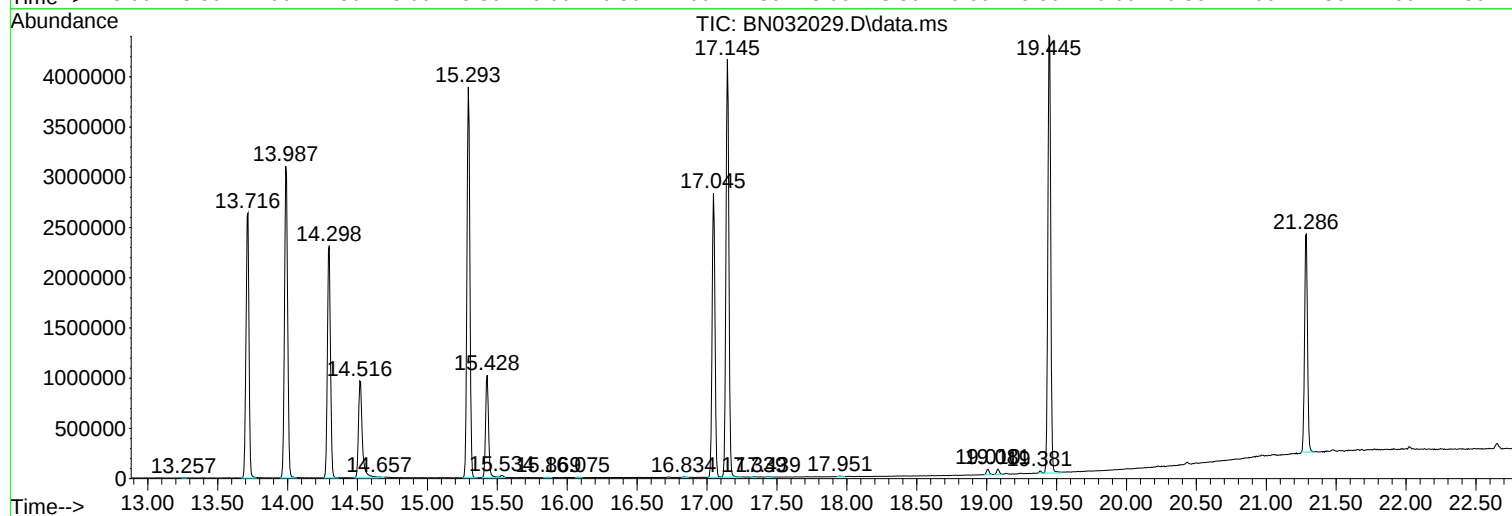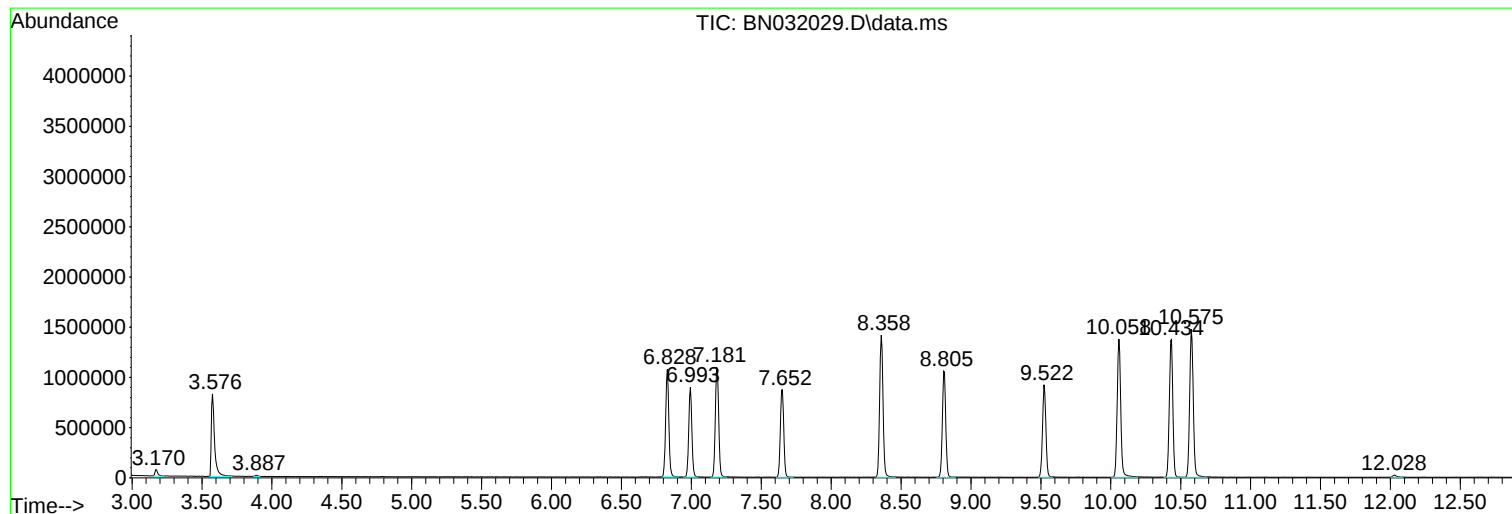

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061724\
Data File : BN032029.D
Acq On : 17 Jun 2024 11:38
Operator : MA/JU
Sample : PB161388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061724\
Data File : BN032029.D
Acq On : 17 Jun 2024 11:38
Operator : MA/JU
Sample : PB161388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------