
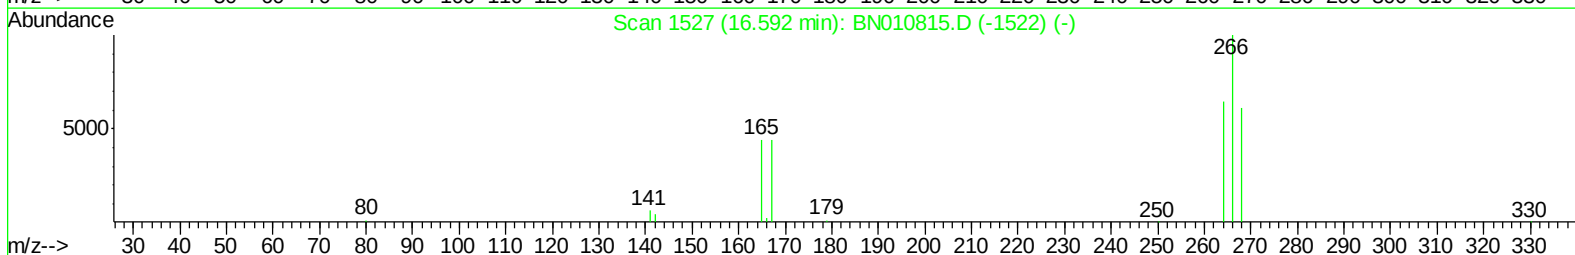
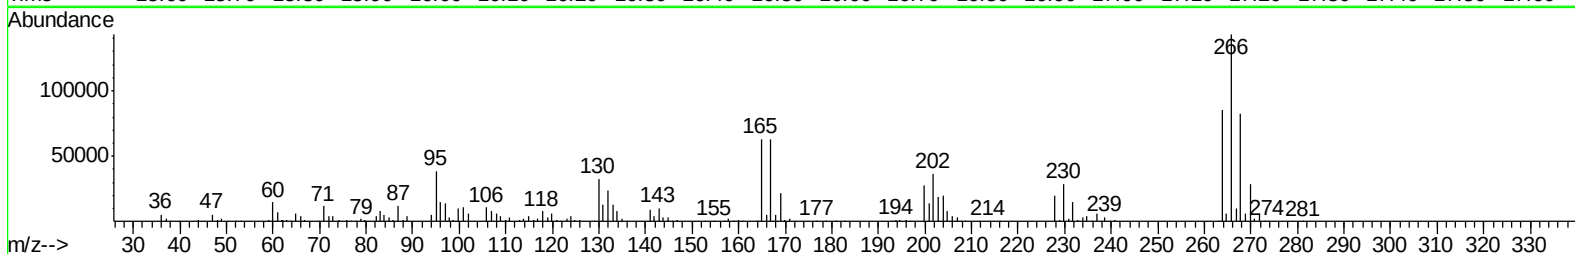


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061820\
Data File : BN010953.D
Acq On : 18 Jun 2020 12:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 04:25:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 18 14:14:42 2020
Response via : Initial Calibration

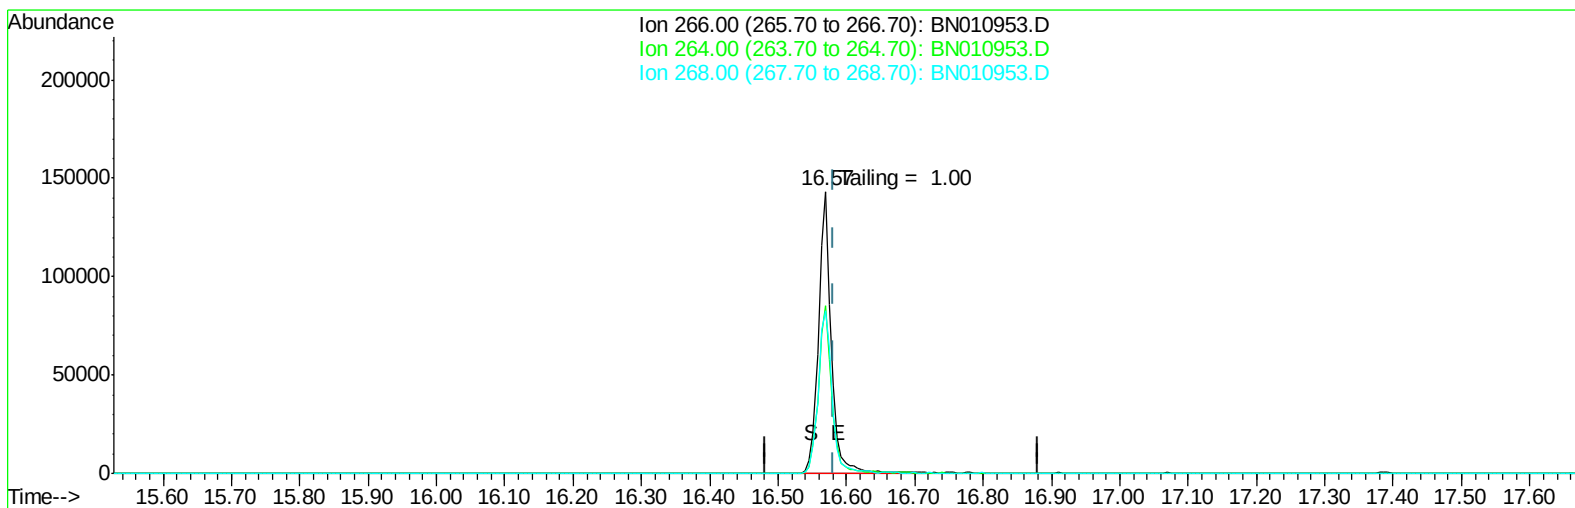

TIC: BN010953.D

(22) Pentachlorophenol

16.569min (-0.013) 0.00ng

response 186897

Ion	Exp%	Act%
266.00	100	100
264.00	68.50	59.45
268.00	69.90	57.83
0.00	0.00	0.00