
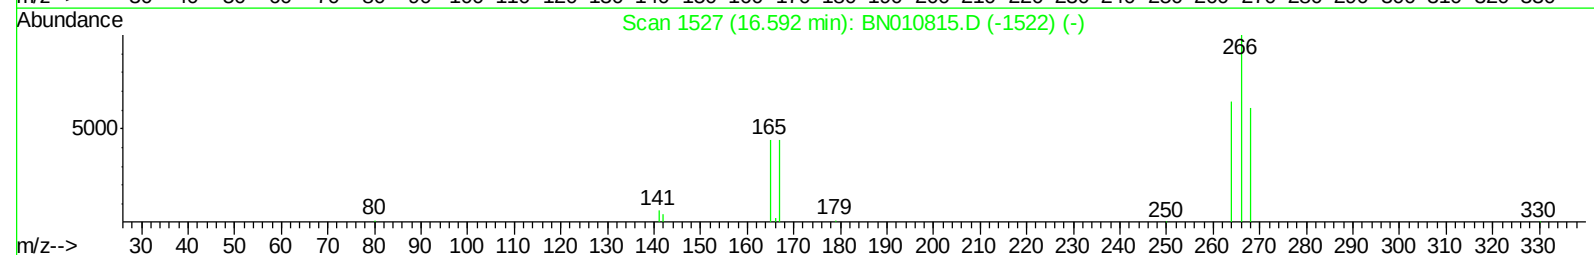
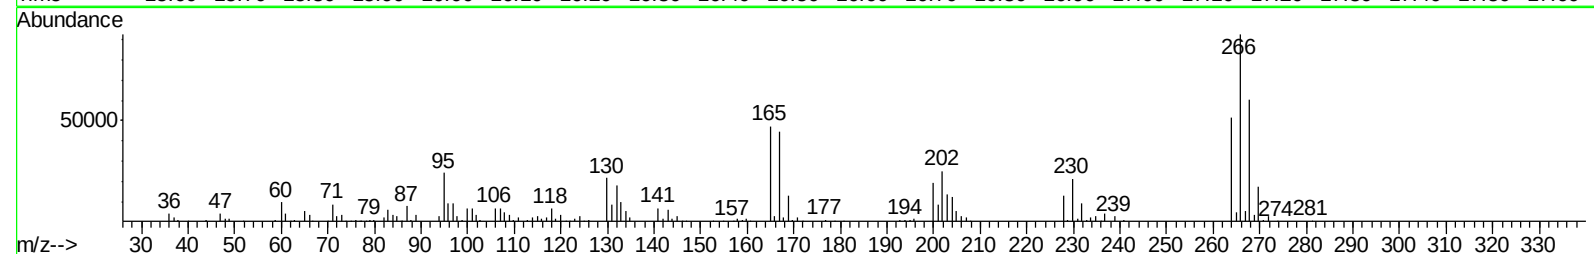


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061820\
 Data File : BN010956.D
 Acq On : 18 Jun 2020 16:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 06:15:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 18 14:14:42 2020
 Response via : Initial Calibration

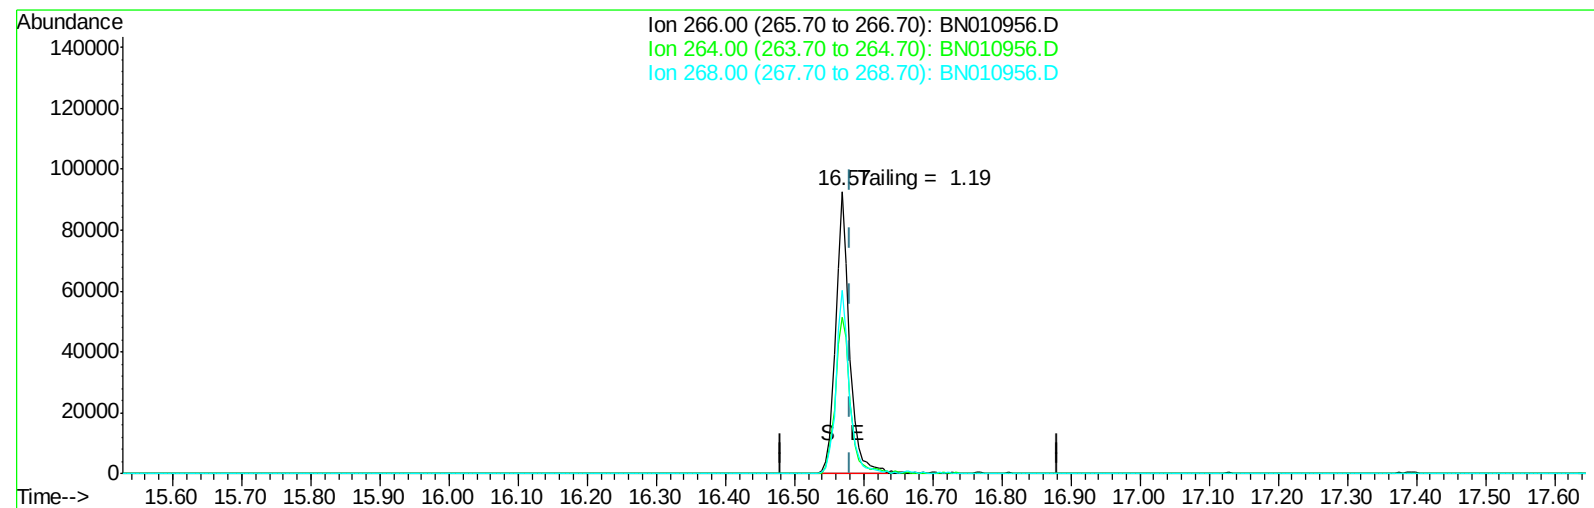

TIC: BN010956.D

(22) Pentachlorophenol

16.569min (-0.013) 0.00ng

response 128770

Ion	Exp%	Act%
266.00	100	100
264.00	68.50	55.61
268.00	69.90	65.15
0.00	0.00	0.00