


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061820\
 Data File : BN010953.D
 Acq On : 18 Jun 2020 12:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 12:43:49 2020

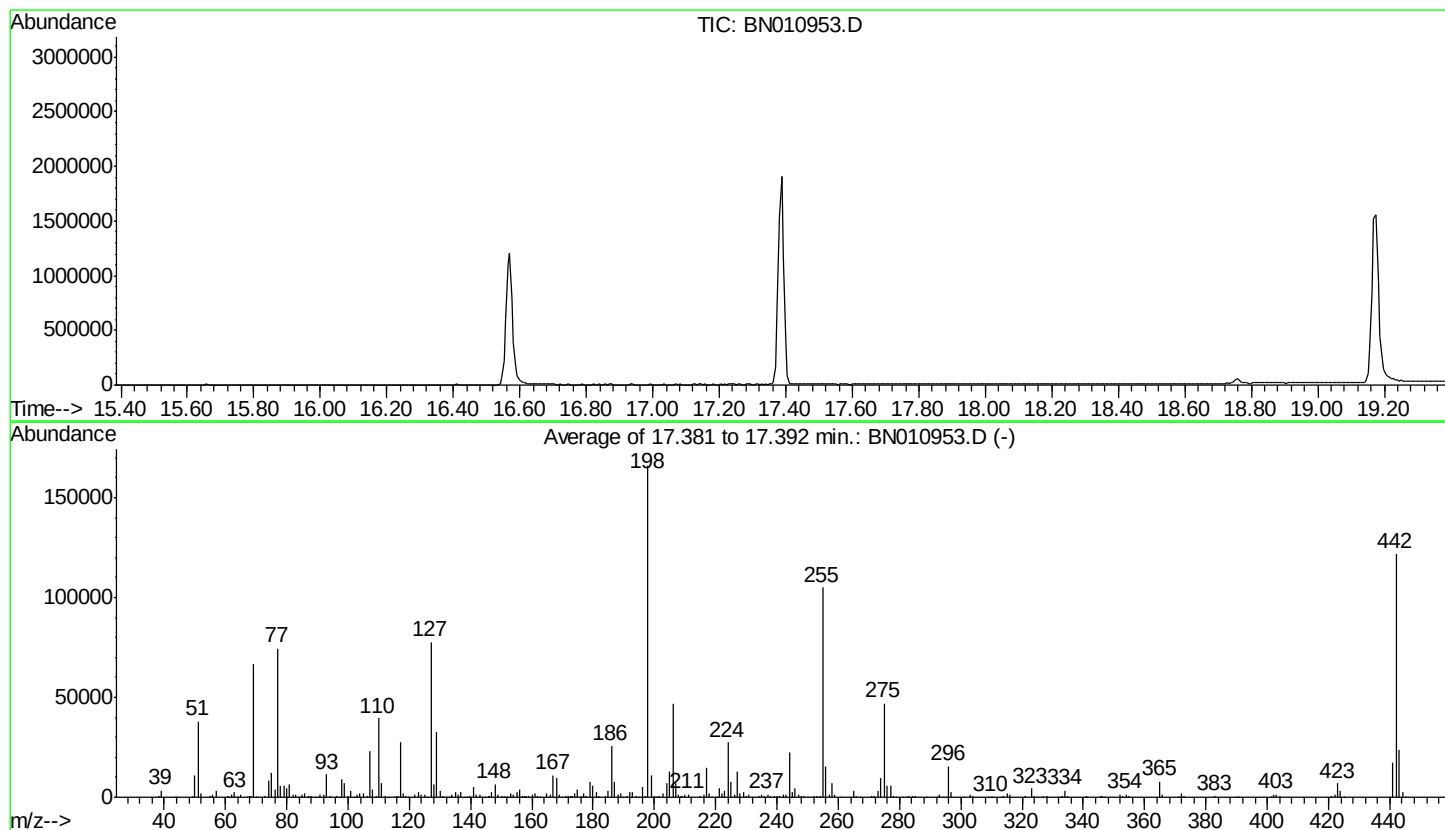

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	38032	PASS
68	69	0.00	2	1.4	933	PASS
69	198	0.00	100	40.1	66525	PASS
70	69	0.00	2	0.3	227	PASS
127	198	10	80	46.8	77730	PASS
197	198	0.00	2	0.3	504	PASS
198	198	100	100	100.0	166029	PASS
199	198	5	9	6.7	11184	PASS
275	198	10	60	28.3	46904	PASS
365	198	1	100	4.8	7980	PASS
441	198	0.01	100	10.5	17356	PASS
442	198	50	100	73.5	122021	PASS
443	442	15	24	19.7	24002	PASS