


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061820\
 Data File : BN010956.D
 Acq On : 18 Jun 2020 16:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 12:43:49 2020

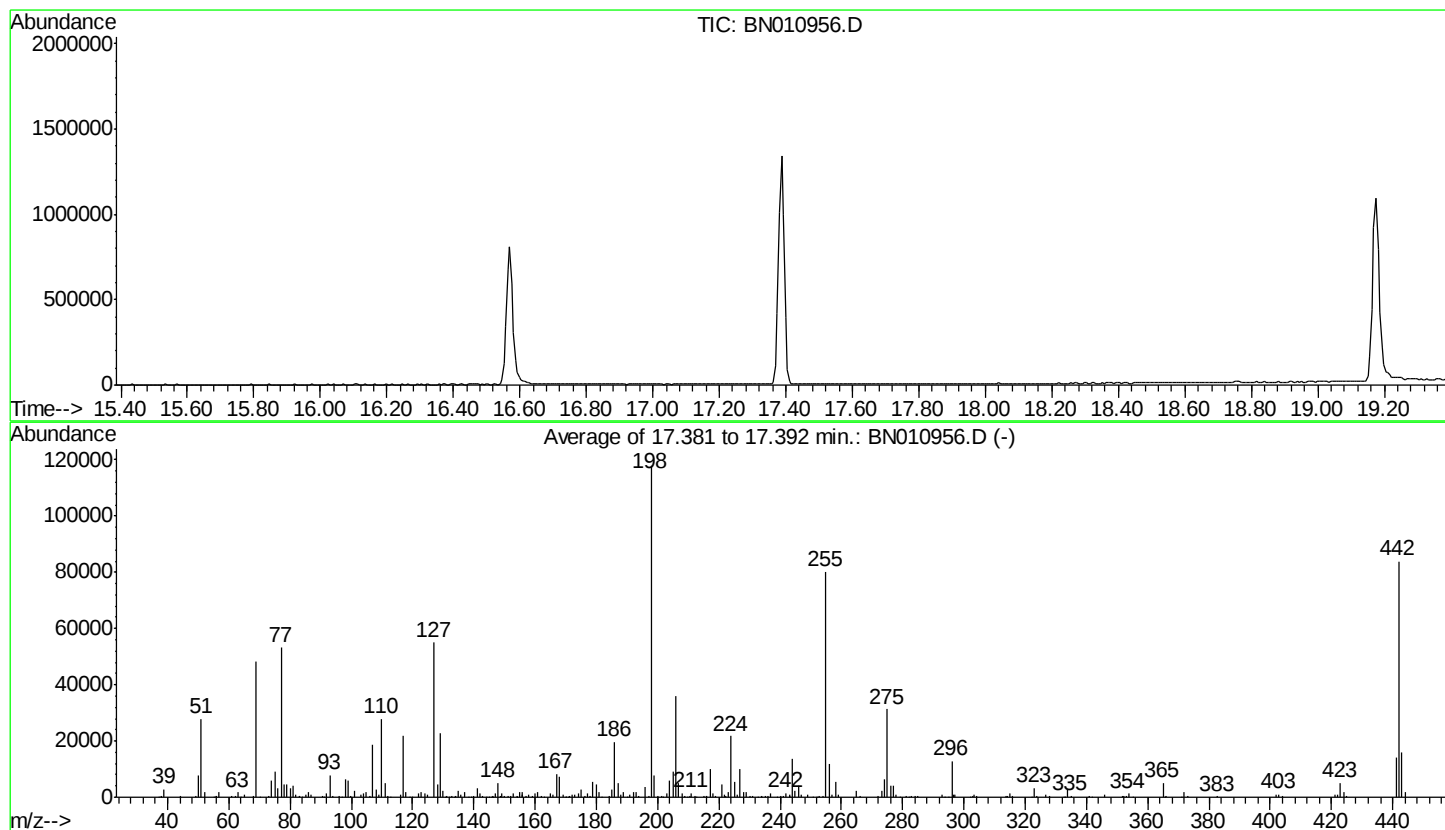

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.7	27898	PASS
68	69	0.00	2	1.3	650	PASS
69	198	0.00	100	40.9	48256	PASS
70	69	0.00	2	0.5	222	PASS
127	198	10	80	46.7	55064	PASS
197	198	0.00	2	0.6	687	PASS
198	198	100	100	100.0	117938	PASS
199	198	5	9	6.7	7918	PASS
275	198	10	60	26.6	31368	PASS
365	198	1	100	4.4	5141	PASS
441	198	0.01	100	12.0	14146	PASS
442	198	50	100	71.2	83952	PASS
443	442	15	24	18.8	15796	PASS