

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
 Data File : BN032056.D
 Acq On : 18 Jun 2024 22:08
 Operator : MA/JU
 Sample : P2696-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BJ1

Quant Time: Jun 18 22:56:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 14:06:13 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.649	152	8442	0.400	ng/ul	0.00
4) Naphthalene-d8	10.425	136	30012	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.289	164	19825	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.040	188	44419	0.400	ng/ul	0.00
17) Chrysene-d12	21.233	240	30888	0.400	ng/ul	# 0.00
23) Perylene-d12	23.455	264	33349	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	31733	3.506	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.025	152	11794	0.242	ng/ul	0.00
18) Fluoranthene-d10	19.072	212	32483	0.348	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.474	128	34743	0.435	ng/ul	99
7) 2-Methylnaphthalene	12.096	142	26595	0.478	ng/ul	97
8) 1-Methylnaphthalene	12.316	142	32823	0.570	ng/ul	97
10) Acenaphthylene	14.011	152	19040	0.225	ng/ul#	87
11) Acenaphthene	14.354	153	184735	2.921	ng/ul	99
12) Fluorene	15.344	166	215961	2.796	ng/ul	98
15) Phenanthrene	17.082	178	3883566	31.009	ng/ul	99
16) Anthracene	17.171	178	574337	5.096	ng/ul	100
19) Fluoranthene	19.104	202	3430661	30.150	ng/ul	99
20) Pyrene	19.472	202	3243462	27.215	ng/ul	99
21) Benzo(a)anthracene	21.219	228	1484258	12.529	ng/ul	98
22) Chrysene	21.271	228	1582955	13.402	ng/ul	98
24) Benzo(b)fluoranthene	22.788	252	1701478	11.614	ng/ul	97
26) Benzo(a)pyrene	23.358	252	510333	4.902	ng/ul#	94
27) Indeno(1,2,3-cd)pyrene	25.695	276	326087	2.322	ng/ul	95
28) Dibenzo(a,h)anthracene	25.705	278	128560	1.186	ng/ul	97
29) Benzo(g,h,i)perylene	26.386	276	48571	0.435	ng/ul	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032056.D
Acq On : 18 Jun 2024 22:08
Operator : MA/JU
Sample : P2696-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BJ1


Quant Time: Jun 18 22:56:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

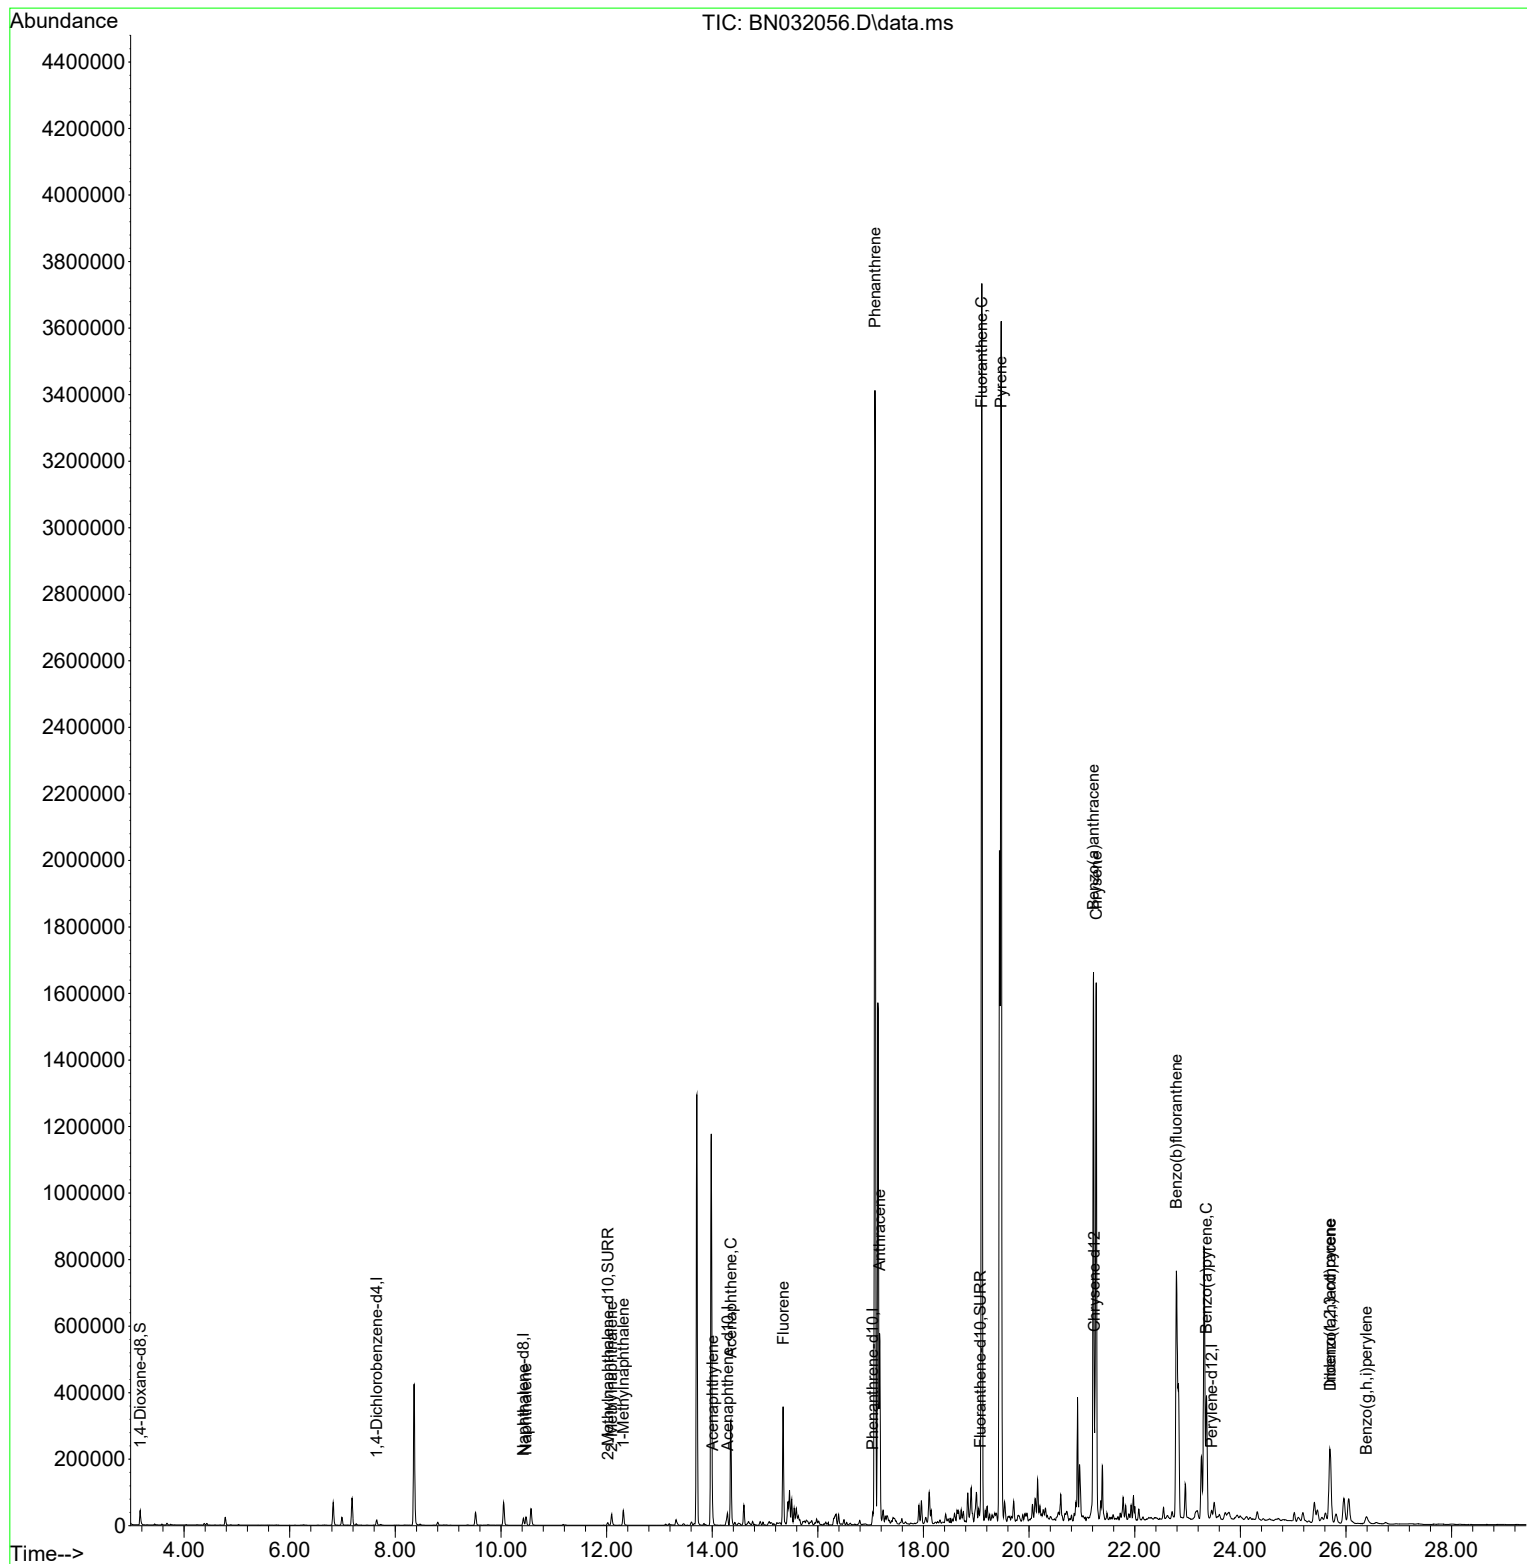






#5
Naphthalene
Concen: 0.435 ng/ul
RT: 10.474 min Scan# 1753
Delta R.T. -0.007 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08

Instrument :
BNA_N
ClientSampleId :
A4BJ1



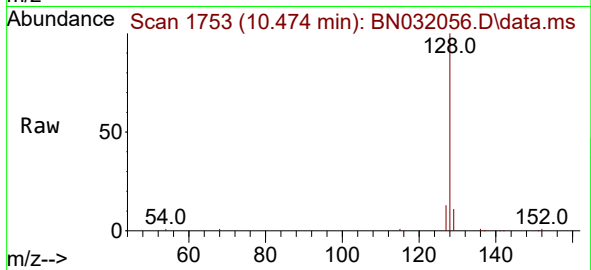



Tgt Ion:128 Resp: 34743
Ion Ratio Lower Upper
128 100
129 11.5 9.3 13.9
127 13.2 10.3 15.5

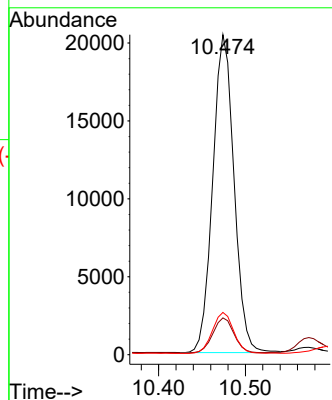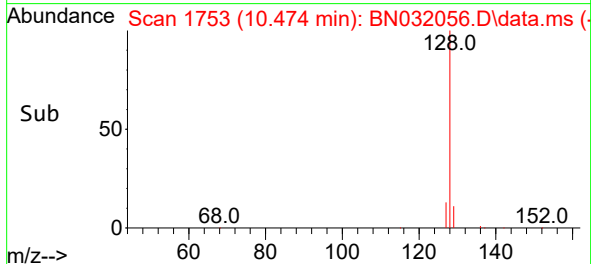

#7
2-Methylnaphthalene
Concen: 0.478 ng/ul
RT: 12.096 min Scan# 2048
Delta R.T. -0.007 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08

Tgt Ion:142 Resp: 26595
Ion Ratio Lower Upper
142 100
141 89.5 69.7 104.5


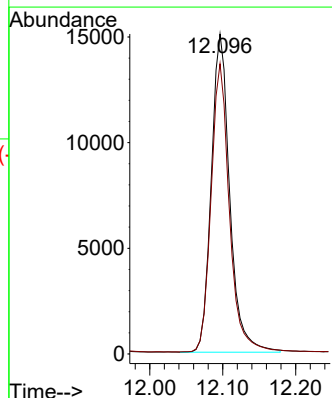

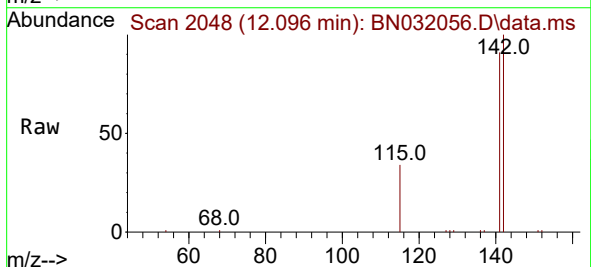


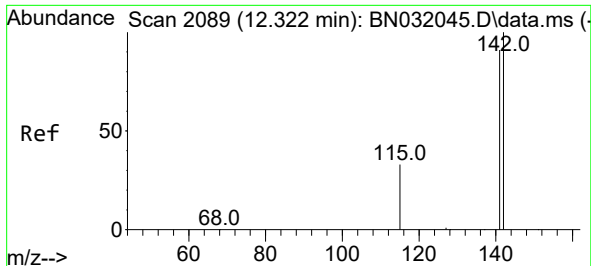

#8
1-Methylnaphthalene
Concen: 0.570 ng/ul
RT: 12.316 min Scan# 2088
Delta R.T. -0.007 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08




Instrument :
BNA_N
ClientSampleId :
A4BJ1


Tgt Ion:142 Resp: 32823
Ion Ratio Lower Upper
142 100
141 92.8 71.7 107.5

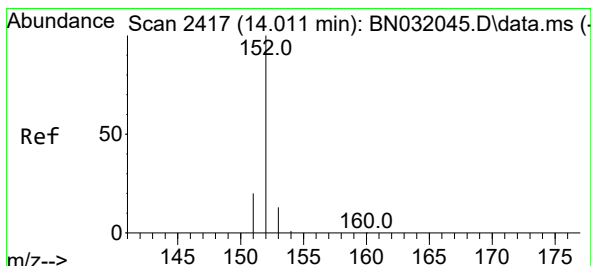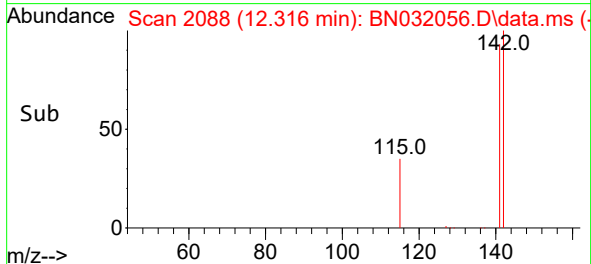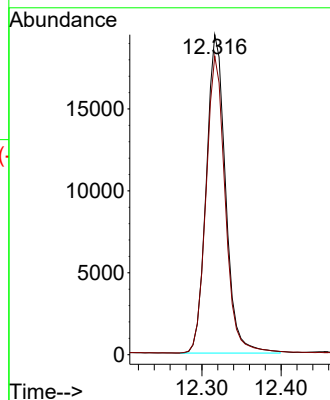

#10
Acenaphthylene
Concen: 0.225 ng/ul
RT: 14.011 min Scan# 2417
Delta R.T. -0.001 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08

Tgt Ion:152 Resp: 19040
Ion Ratio Lower Upper
152 100
151 21.5 16.1 24.1
153 24.1 10.6 16.0#

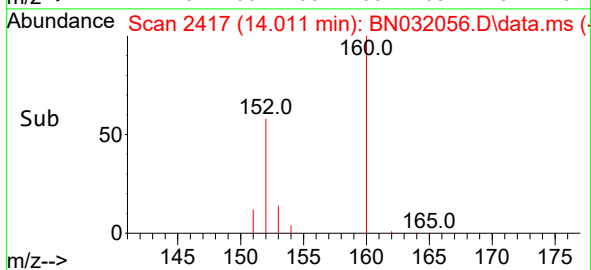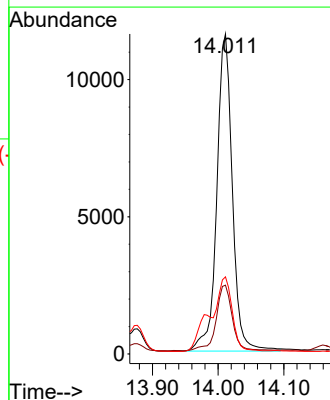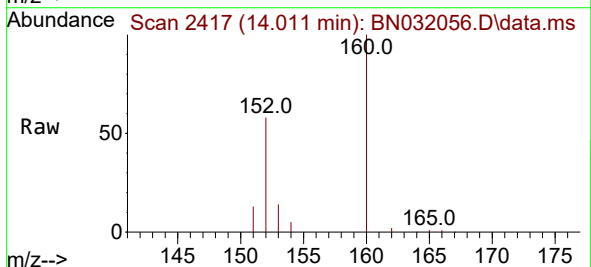



#11

Acenaphthene

Concen: 2.921 ng/ul

RT: 14.354 min Scan# 2491

Delta R.T. -0.001 min

Lab File: BN032056.D

Acq: 18 Jun 2024 22:08

Instrument :

BNA_N

ClientSampleId :

A4BJ1





Tgt Ion:153 Resp: 184735

Ion Ratio Lower Upper

153 100

152 46.9 39.4 59.2

154 88.7 71.2 106.8

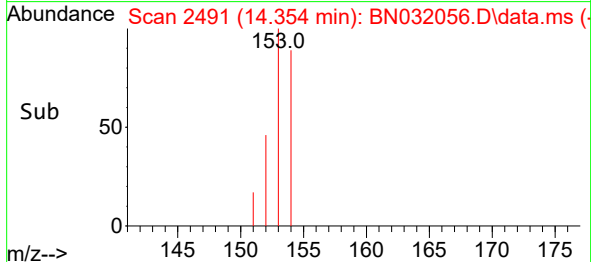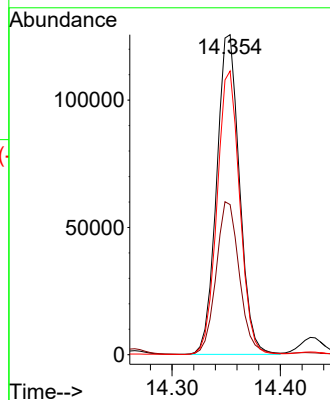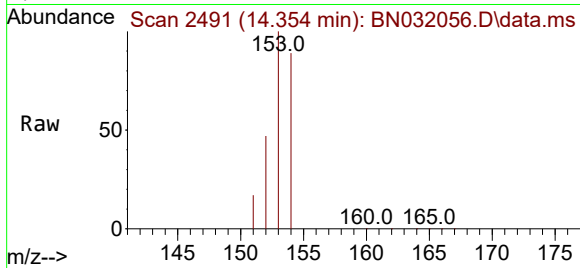

#12

Fluorene

Concen: 2.796 ng/ul

RT: 15.344 min Scan# 2705

Delta R.T. -0.001 min

Lab File: BN032056.D

Acq: 18 Jun 2024 22:08




Tgt Ion:166 Resp: 215961


Ion Ratio Lower Upper

166 100

165 96.6 79.0 118.6

167 15.0 11.0 16.6


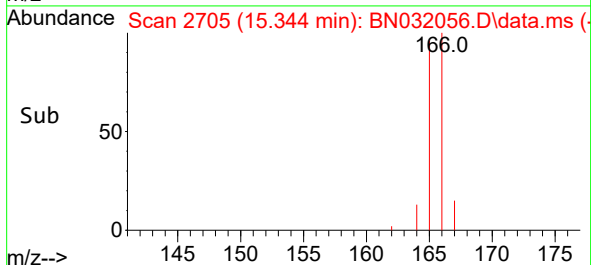
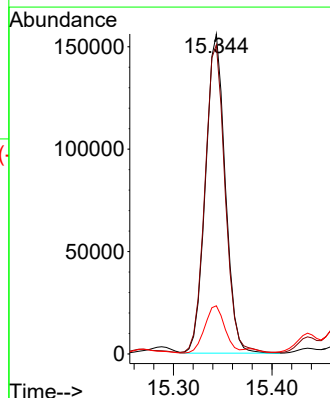
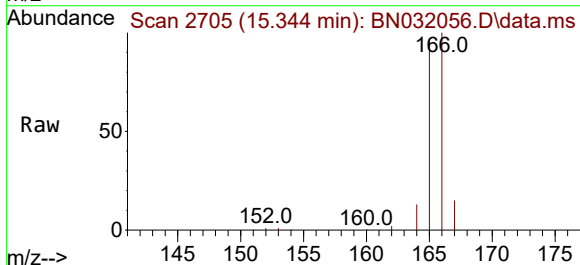


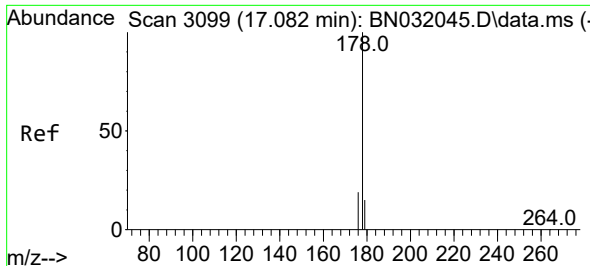

#15
Phenanthrene
Concen: 31.009 ng/ul
RT: 17.082 min Scan# 3099
Delta R.T. -0.001 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08




Instrument :
BNA_N
ClientSampleId :
A4BJ1


Tgt Ion:178 Resp: 3883566
Ion Ratio Lower Upper
178 100
179 15.9 12.5 18.7
176 19.3 15.3 22.9

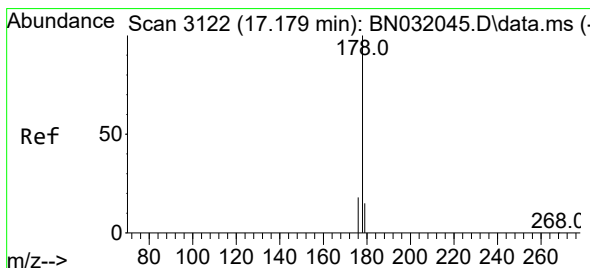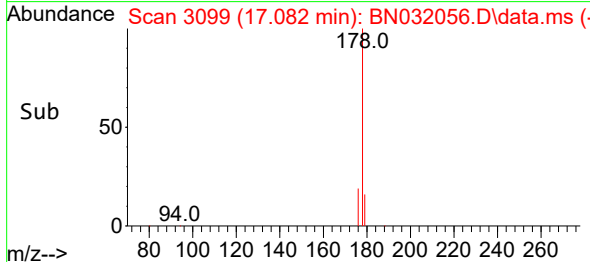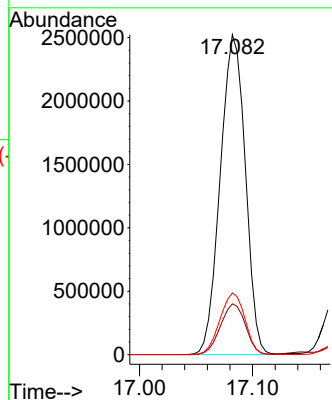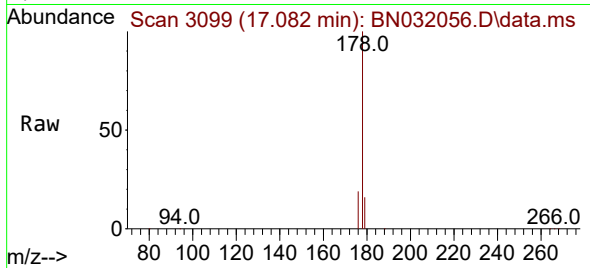

#16
Anthracene
Concen: 5.096 ng/ul
RT: 17.171 min Scan# 3120
Delta R.T. -0.005 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08

Tgt Ion:178 Resp: 574337
Ion Ratio Lower Upper
178 100
179 15.6 12.7 19.1
176 18.5 14.8 22.2


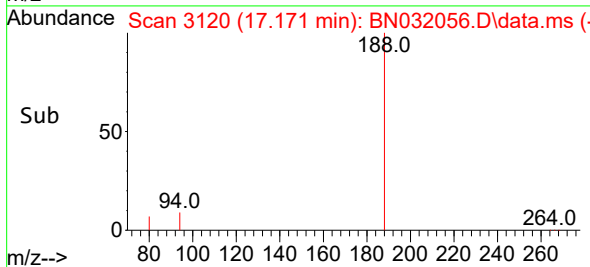
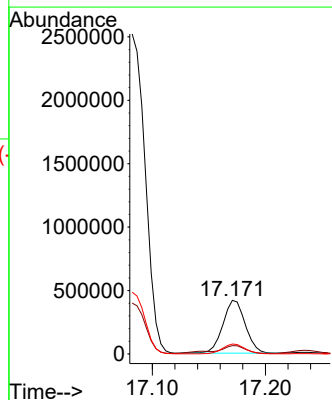
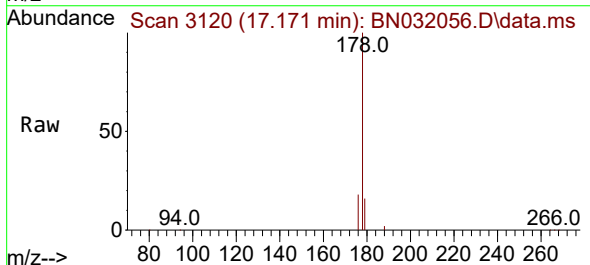




#19
Fluoranthene
Concen: 30.150 ng/ul
RT: 19.104 min Scan# 3565
Delta R.T. -0.001 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08




Instrument :
BNA_N
ClientSampleId :
A4BJ1


Tgt Ion:202 Resp: 3430661
Ion Ratio Lower Upper
202 100
101 11.3 8.8 13.2
100 8.4 6.6 9.8

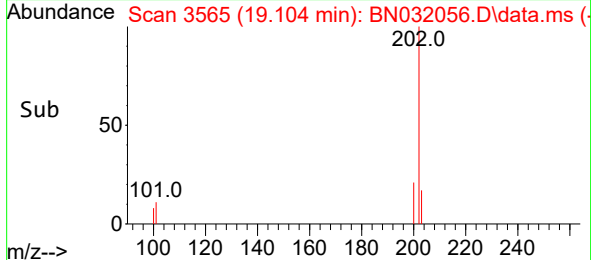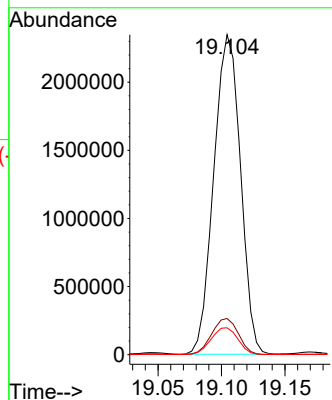

#20
Pyrene
Concen: 27.215 ng/ul
RT: 19.472 min Scan# 3644
Delta R.T. 0.003 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08

Tgt Ion:202 Resp: 3243462
Ion Ratio Lower Upper
202 100
101 12.8 10.5 15.7
100 10.2 8.6 12.8


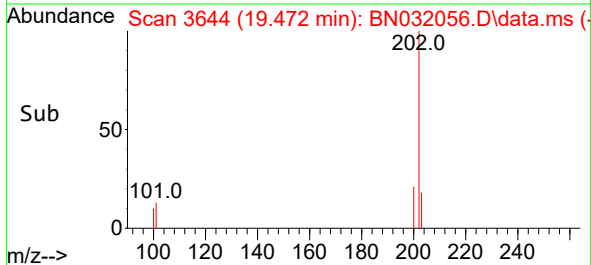
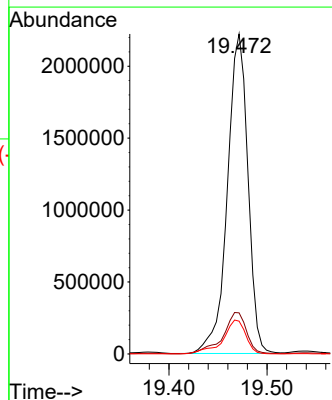
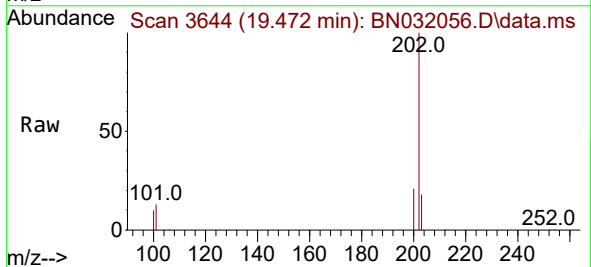


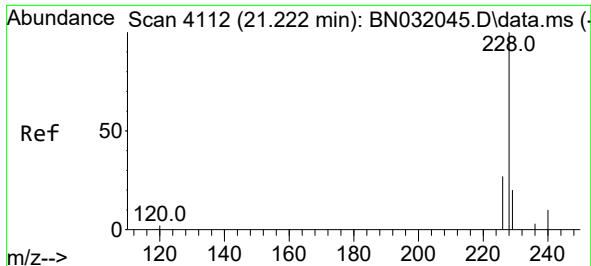

#21
Benzo(a)anthracene
Concen: 12.529 ng/ul
RT: 21.219 min Scan# 4111
Delta R.T. -0.004 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08




Instrument :
BNA_N
ClientSampleId :
A4BJ1


Tgt Ion:228 Resp: 1484258
Ion Ratio Lower Upper
228 100
229 21.0 15.7 23.5
226 27.4 21.7 32.5

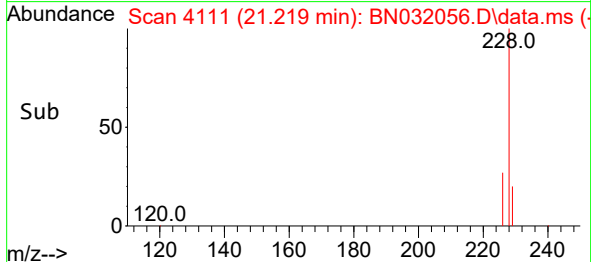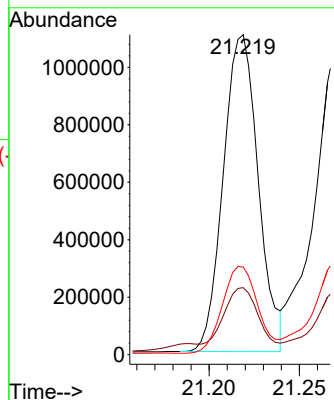

#22
Chrysene
Concen: 13.402 ng/ul
RT: 21.271 min Scan# 4129
Delta R.T. -0.004 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08


Tgt Ion:228 Resp: 1582955
Ion Ratio Lower Upper
228 100
226 30.2 23.6 35.4
229 21.2 15.6 23.4

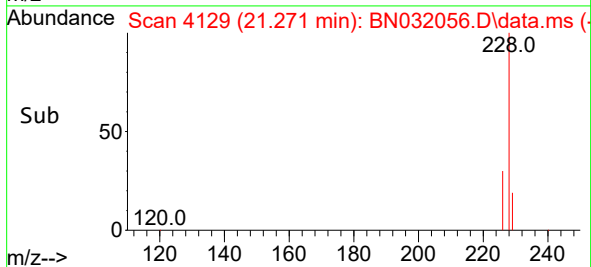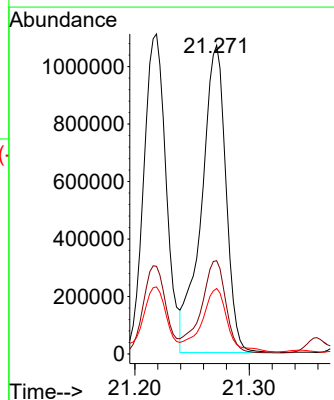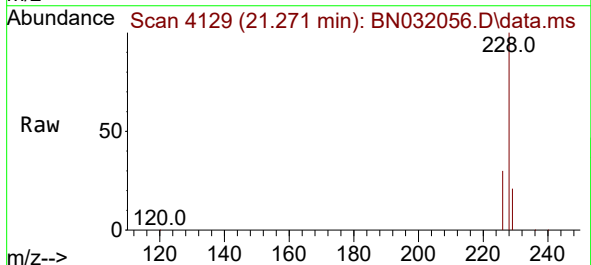






#24
Benzo(b)fluoranthene
Concen: 11.614 ng/ul
RT: 22.788 min Scan# 4648
Delta R.T. -0.004 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08

Instrument :
BNA_N
ClientSampleId :
A4BJ1



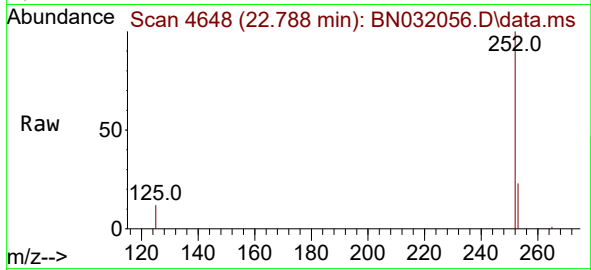



Tgt Ion:252 Resp: 1701478
Ion Ratio Lower Upper
252 100
253 23.5 0.0 47.4
125 11.6 0.0 28.8

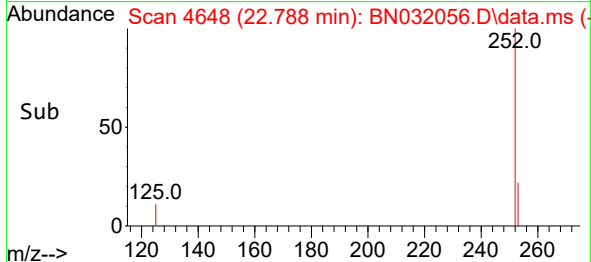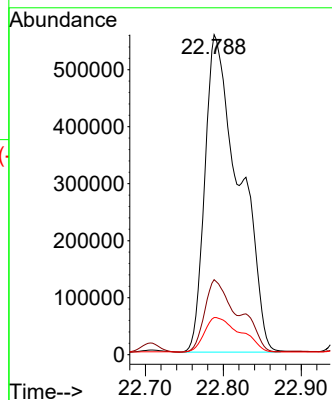

#26
Benzo(a)pyrene
Concen: 4.902 ng/ul
RT: 23.358 min Scan# 4843
Delta R.T. -0.007 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08

Tgt Ion:252 Resp: 510333
Ion Ratio Lower Upper
252 100
253 23.1 19.9 29.9
125 12.7 13.5 20.3#


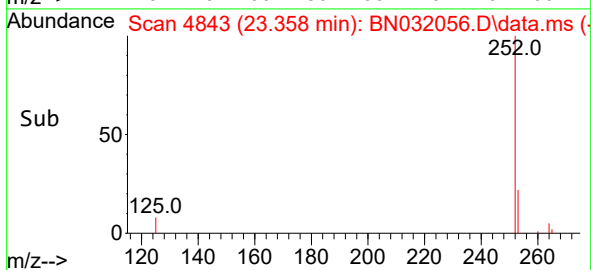
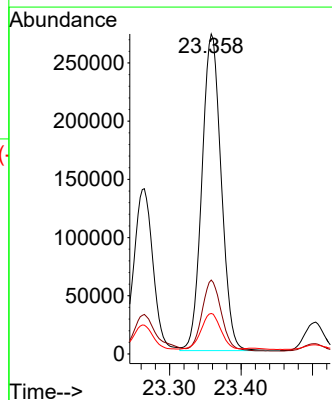
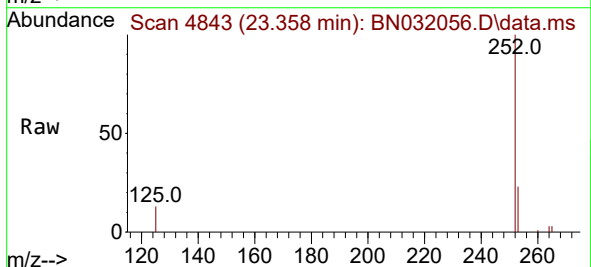


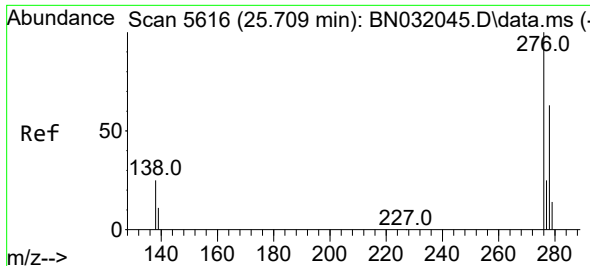

#27
Indeno(1,2,3-cd)pyrene
Concen: 2.322 ng/ul
RT: 25.695 min Scan# 5612
Delta R.T. -0.011 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08




Instrument :
BNA_N
ClientSampleId :
A4BJ1


Tgt Ion:276 Resp: 326087
Ion Ratio Lower Upper
276 100
138 23.8 21.0 31.4
227 0.2 0.2 0.2

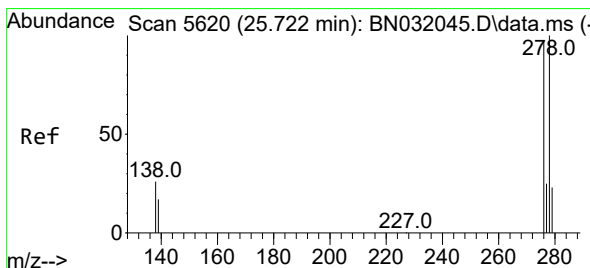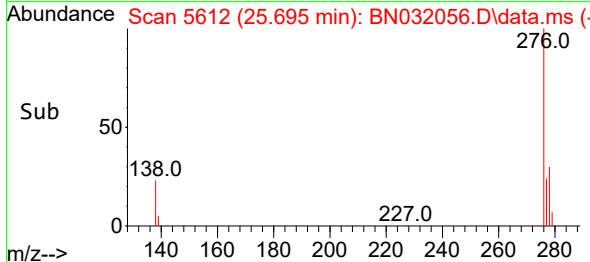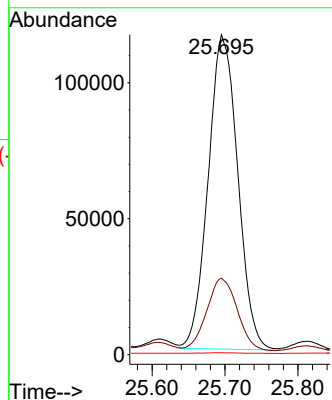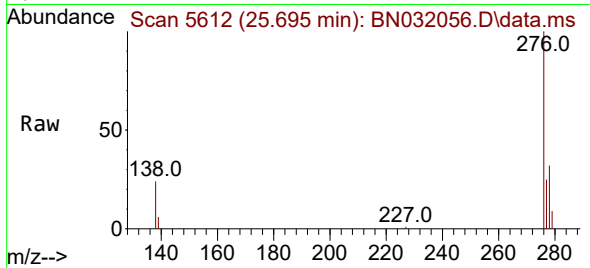

#28
Dibenzo(a,h)anthracene
Concen: 1.186 ng/ul
RT: 25.705 min Scan# 5615
Delta R.T. -0.018 min
Lab File: BN032056.D
Acq: 18 Jun 2024 22:08

Tgt Ion:278 Resp: 128560
Ion Ratio Lower Upper
278 100
139 19.9 14.9 22.3
279 27.4 20.6 31.0

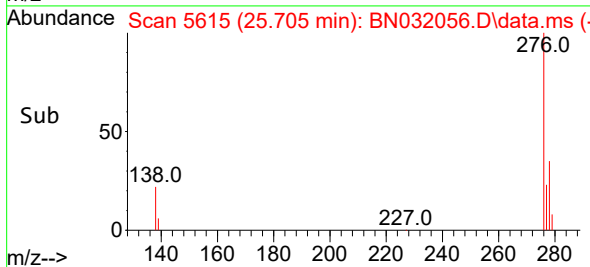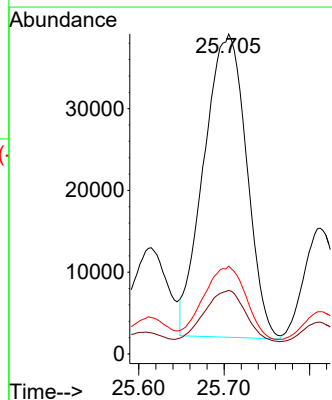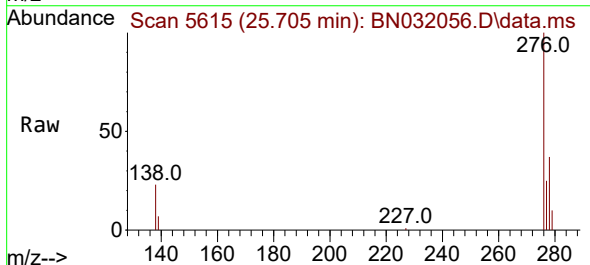

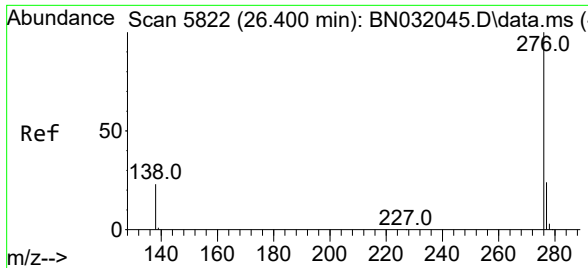

#29
 Benzo(g,h,i)perylene
 Concen: 0.435 ng/ul
 RT: 26.386 min Scan# 51
 Delta R.T. -0.011 min
 Lab File: BN032056.D
 Acq: 18 Jun 2024 22:08

Instrument :
 BNA_N
 ClientSampleId :
 A4BJ1

Tgt Ion:276	Resp:	48571
Ion	Ratio	Lower Upper
276	100	
138	28.4	19.0 28.4
277	29.7	20.4 30.6

