




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032046.D
Acq On : 18 Jun 2024 16:04
Operator : MA/JU
Sample : PB161389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

Quant Time: Jun 18 16:32:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

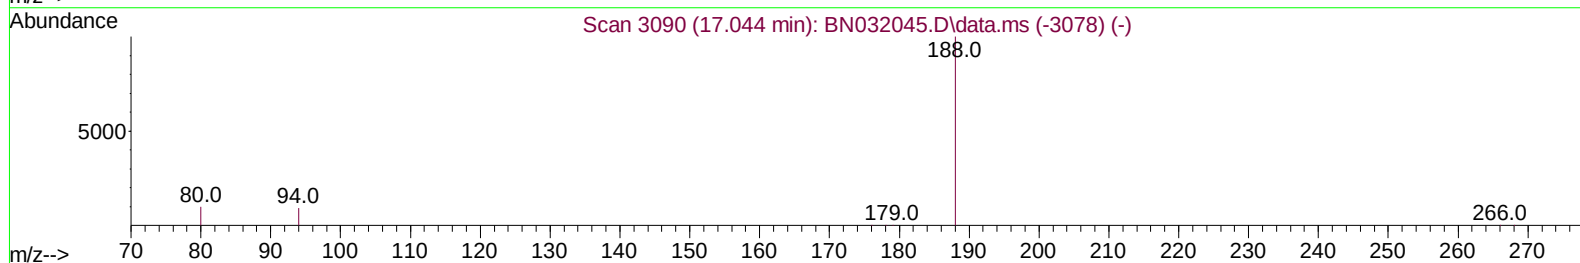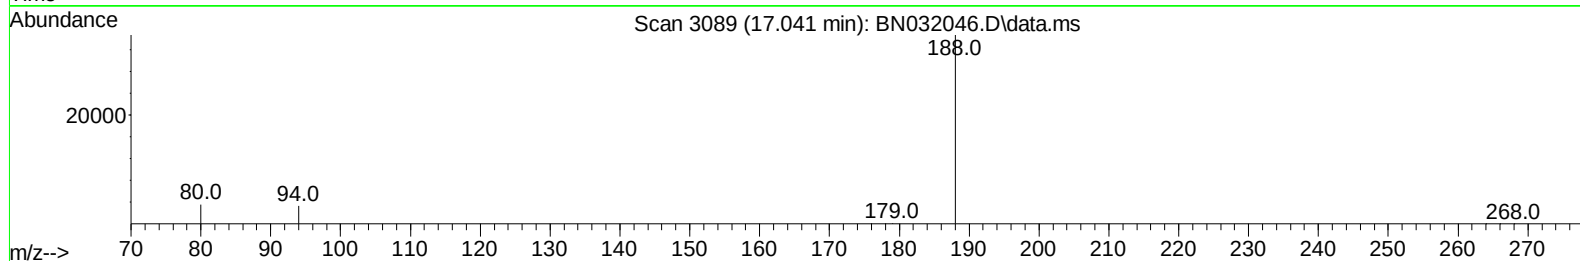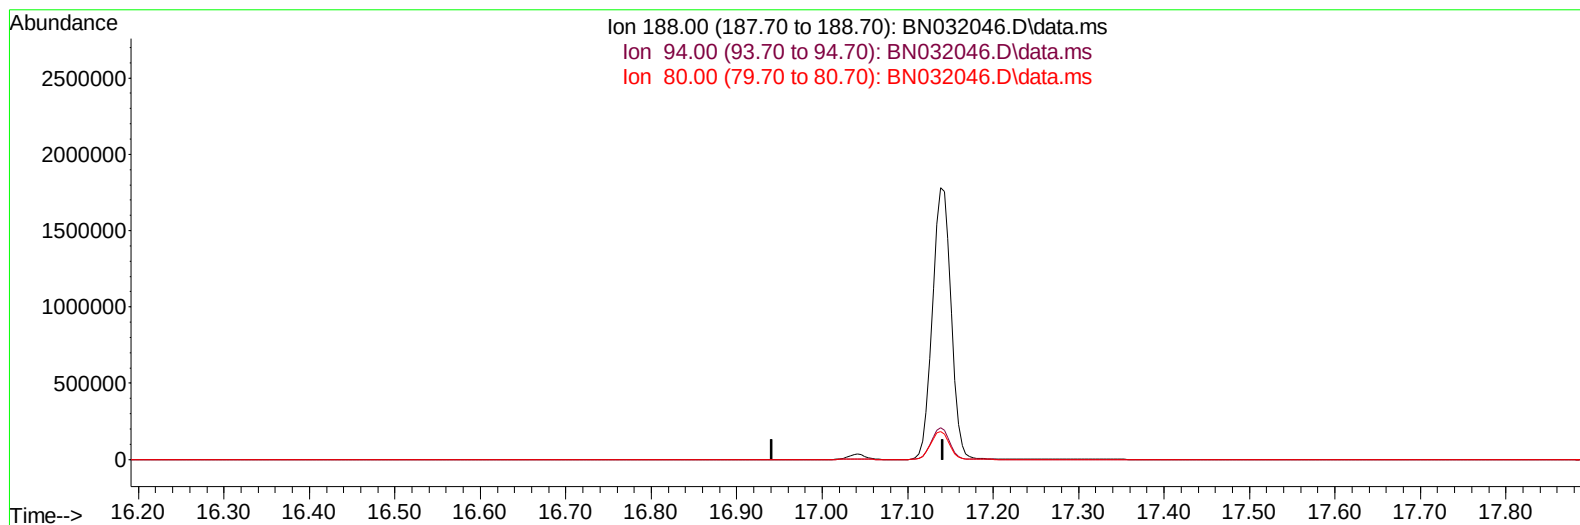

TIC: BN032046.D\data.ms

(13) Phenanthrene-d10 (I)

17.041min (-17.041) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	10.10	0.00#
80.00	10.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032046.D
Acq On : 18 Jun 2024 16:04
Operator : MA/JU
Sample : PB161389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Quant Time: Jun 18 16:32:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

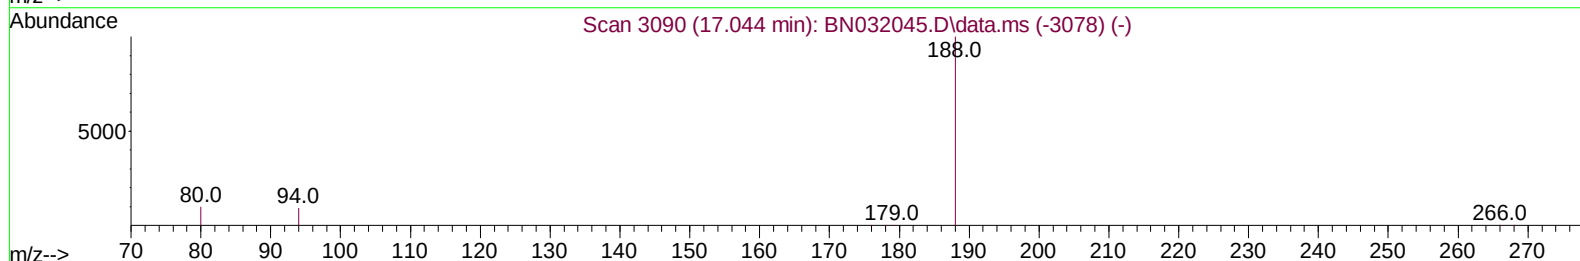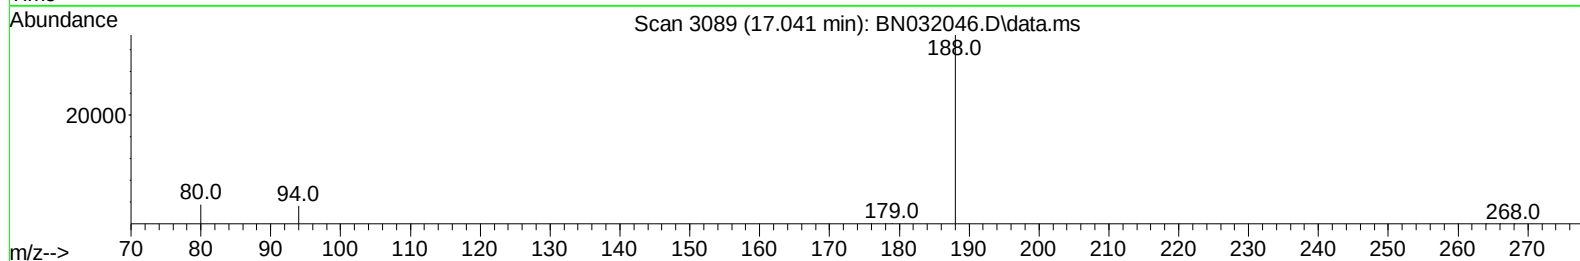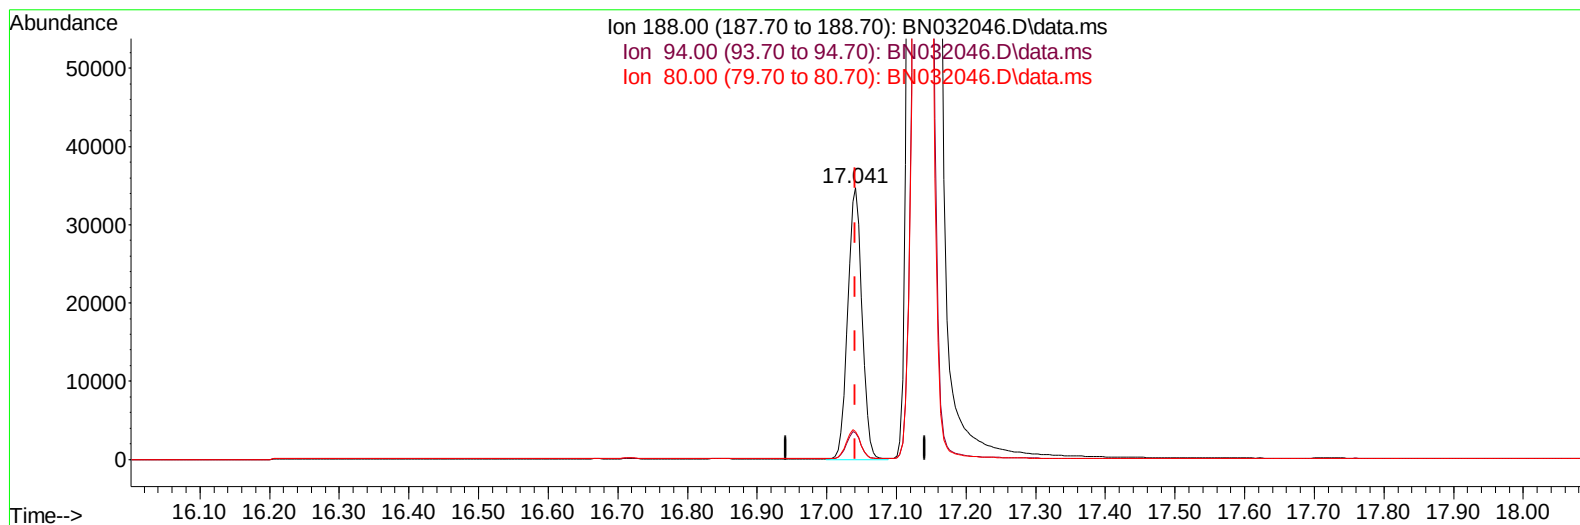

TIC: BN032046.D\data.ms

(13) Phenanthrene-d10 (I)

17.041min (+ 0.000) 0.40 ng/ul m

response 49277

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	9.73
80.00	10.80	10.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032046.D
Acq On : 18 Jun 2024 16:04
Operator : MA/JU
Sample : PB161389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

Quant Time: Jun 18 16:32:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

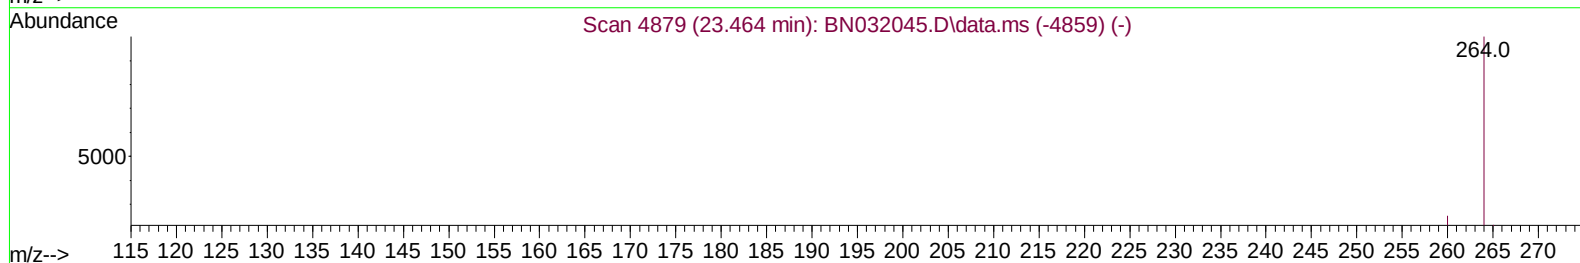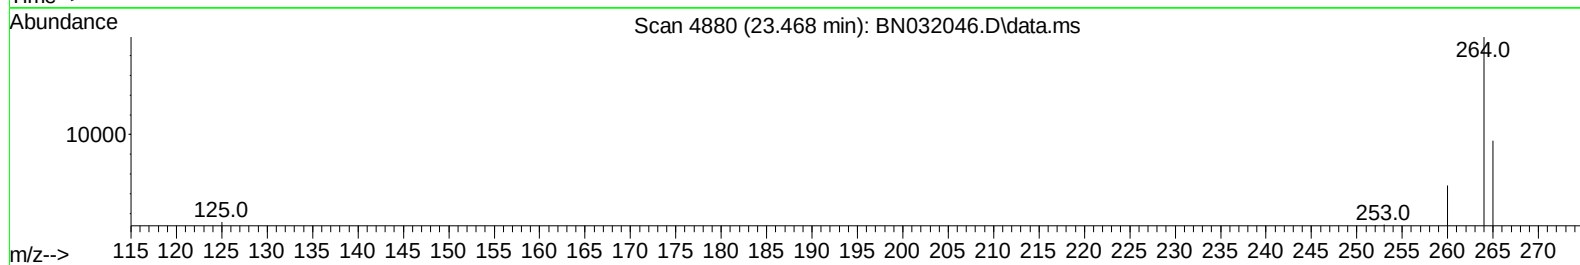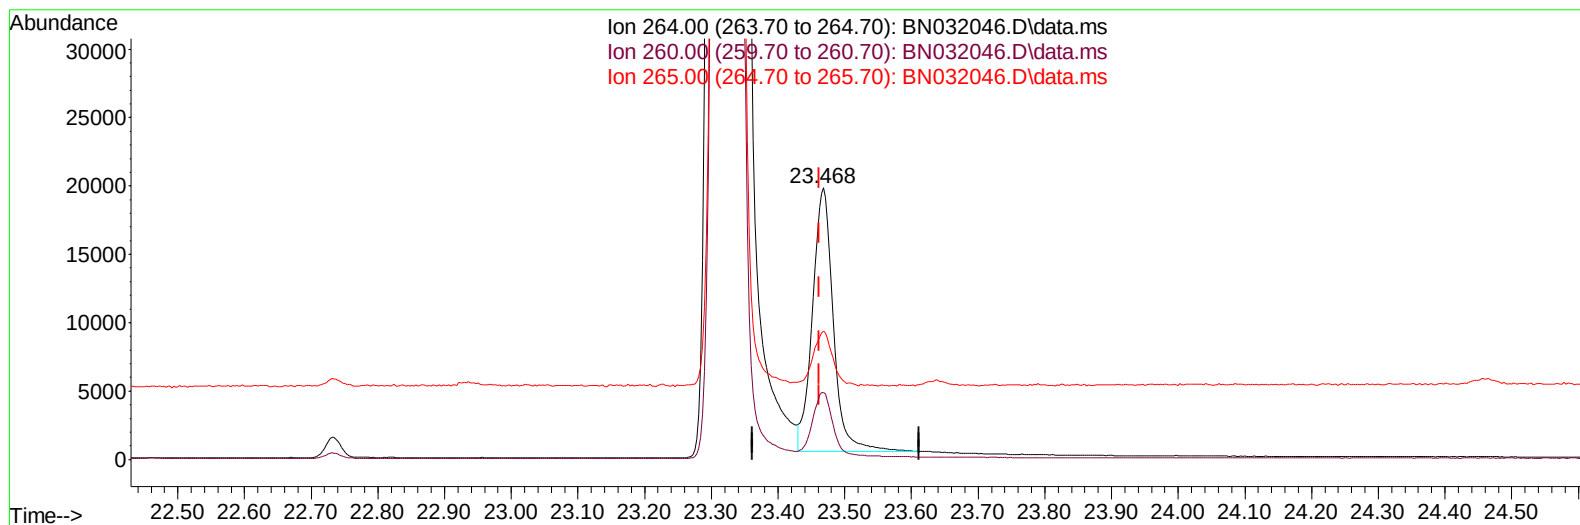

TIC: BN032046.D\data.ms

(23) Perylene-d12 (I)

23.468min (+ 0.006) 0.40 ng/ul

response 41579

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.50	24.60
265.00	53.40	47.29
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032046.D
Acq On : 18 Jun 2024 16:04
Operator : MA/JU
Sample : PB161389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Quant Time: Jun 18 16:32:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

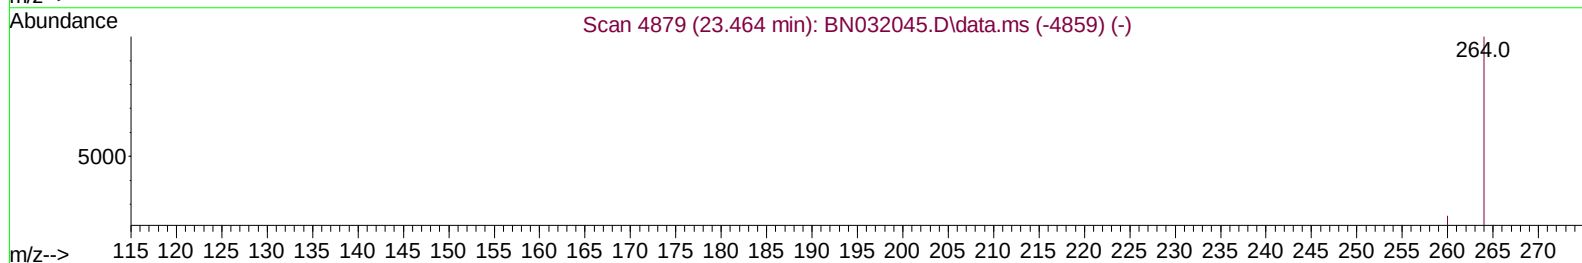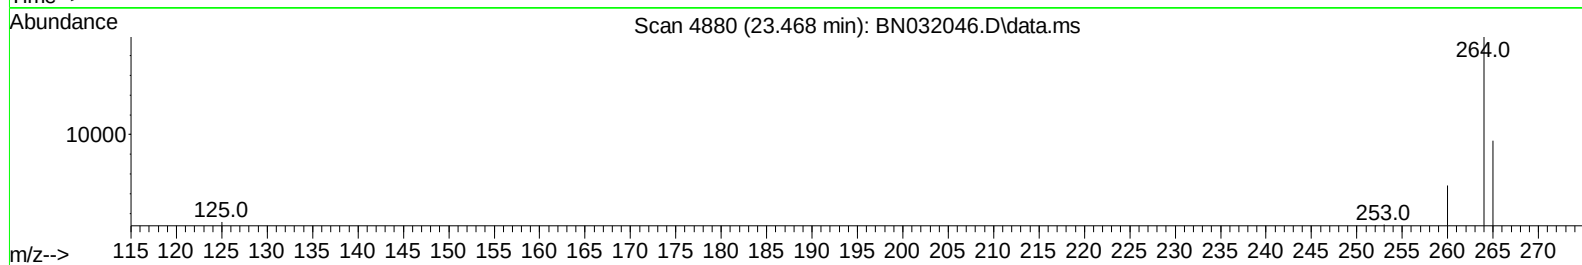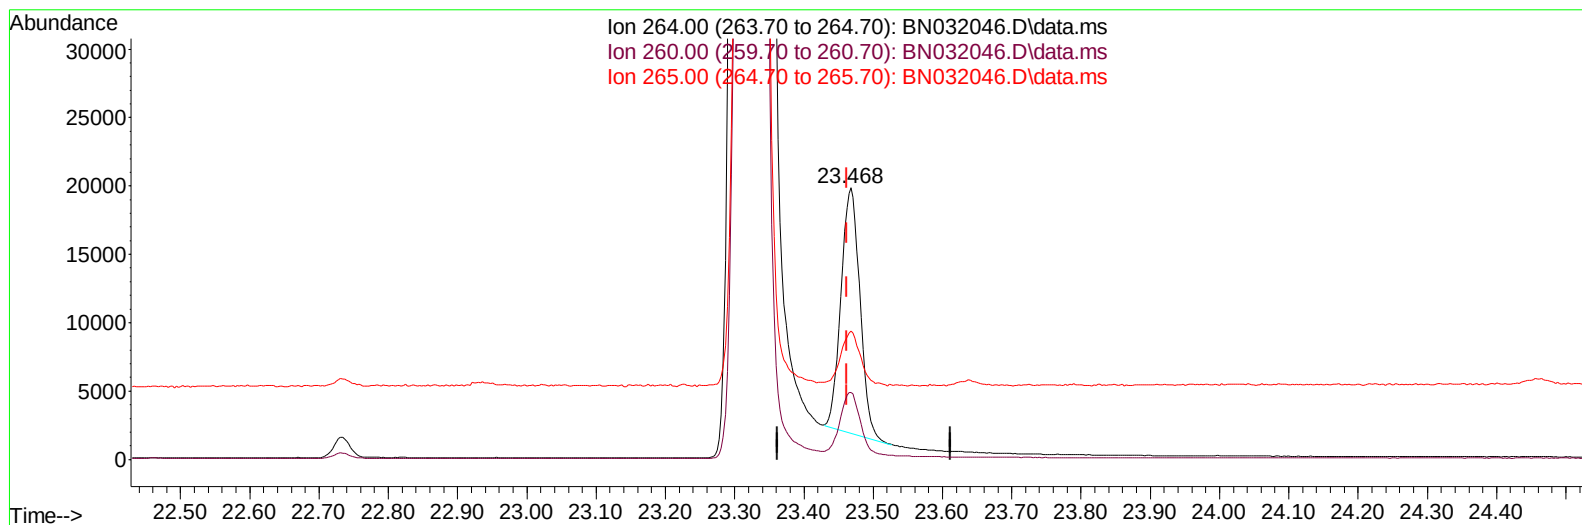

TIC: BN032046.D\data.ms

(23) Perylene-d12 (I)

23.468min (+ 0.006) 0.40 ng/ul m

response 34033

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.50	24.60
265.00	53.40	47.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
 Data File : BN032046.D
 Acq On : 18 Jun 2024 16:04
 Operator : MA/JU
 Sample : PB161389BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK389

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/19/2024
 Supervised By :mohammad ahmed 06/21/2024

Quant Time: Jun 18 16:32:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 14:06:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.650	152	10397	0.400	ng/ul	0.00
4) Naphthalene-d8	10.426	136	35594	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.290	164	22289	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.041	188	49277m	0.400	ng/ul	0.00
17) Chrysene-d12	21.244	240	37596	0.400	ng/ul	0.00
23) Perylene-d12	23.468	264	34033m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	60013	5.384	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.026	152	16672	0.288	ng/ul	0.00
18) Fluoranthene-d10	19.073	212	37085	0.326	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032046.D
Acq On : 18 Jun 2024 16:04
Operator : MA/JU
Sample : PB161389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK389

Manual IntegrationsAPPROVED

Quant Time: Jun 18 16:32:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

