




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032055.D
Acq On : 18 Jun 2024 21:32
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Manual IntegrationsAPPROVED

Quant Time: Jun 18 22:56:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

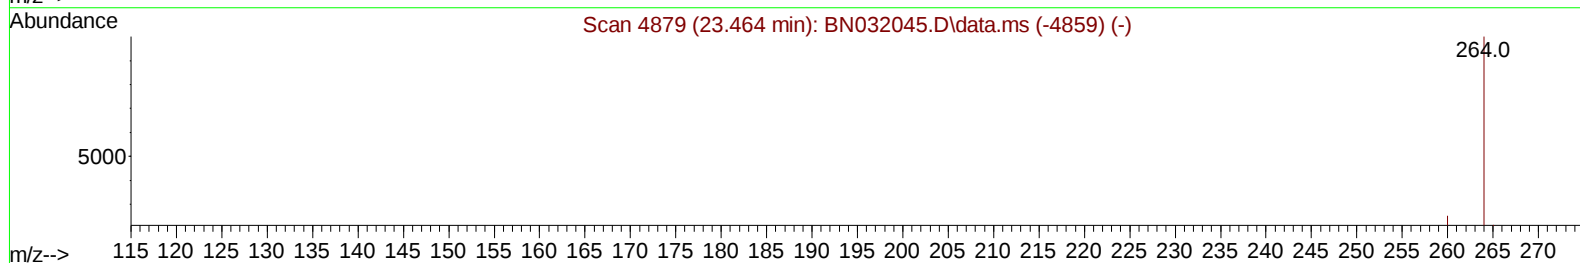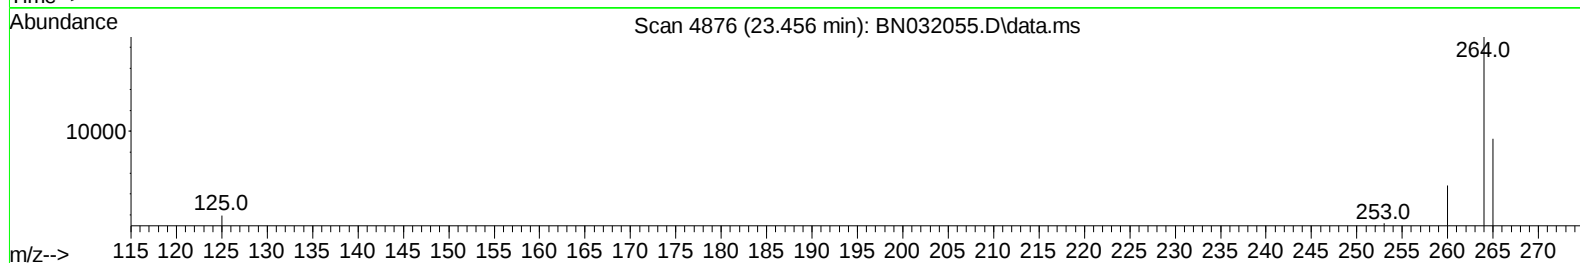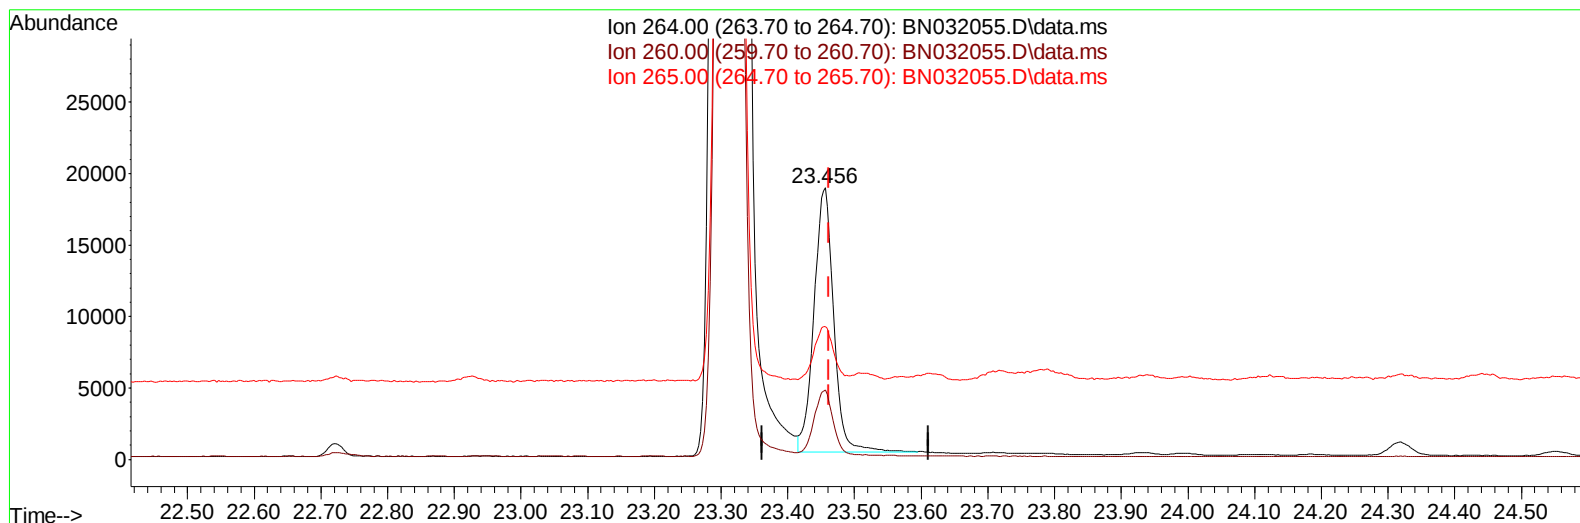

TIC: BN032055.D\data.ms

(23) Perylene-d12 (I)

23.456min (-0.006) 0.40 ng/u1

response 37615

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.50	25.49
265.00	53.40	48.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032055.D
Acq On : 18 Jun 2024 21:32
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Manual IntegrationsAPPROVED

Quant Time: Jun 18 22:56:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

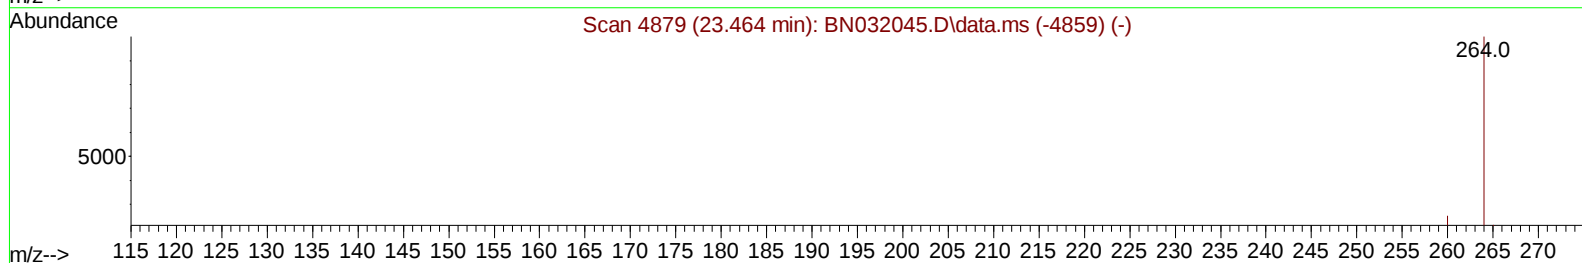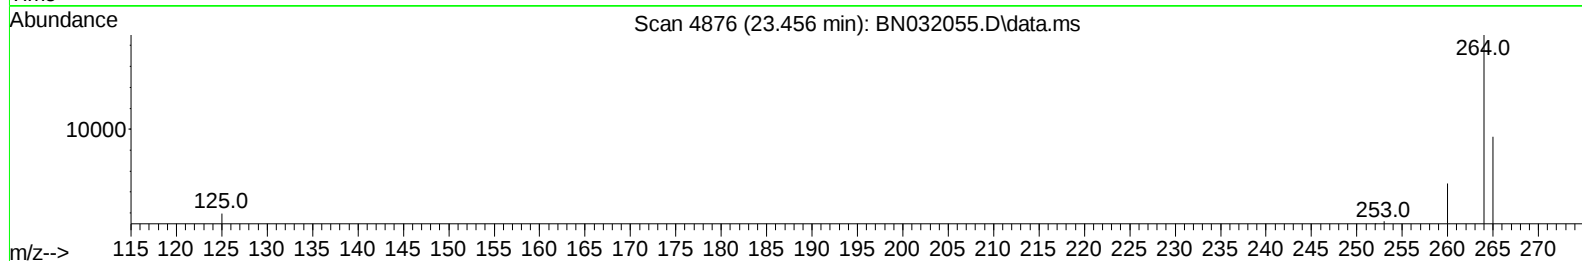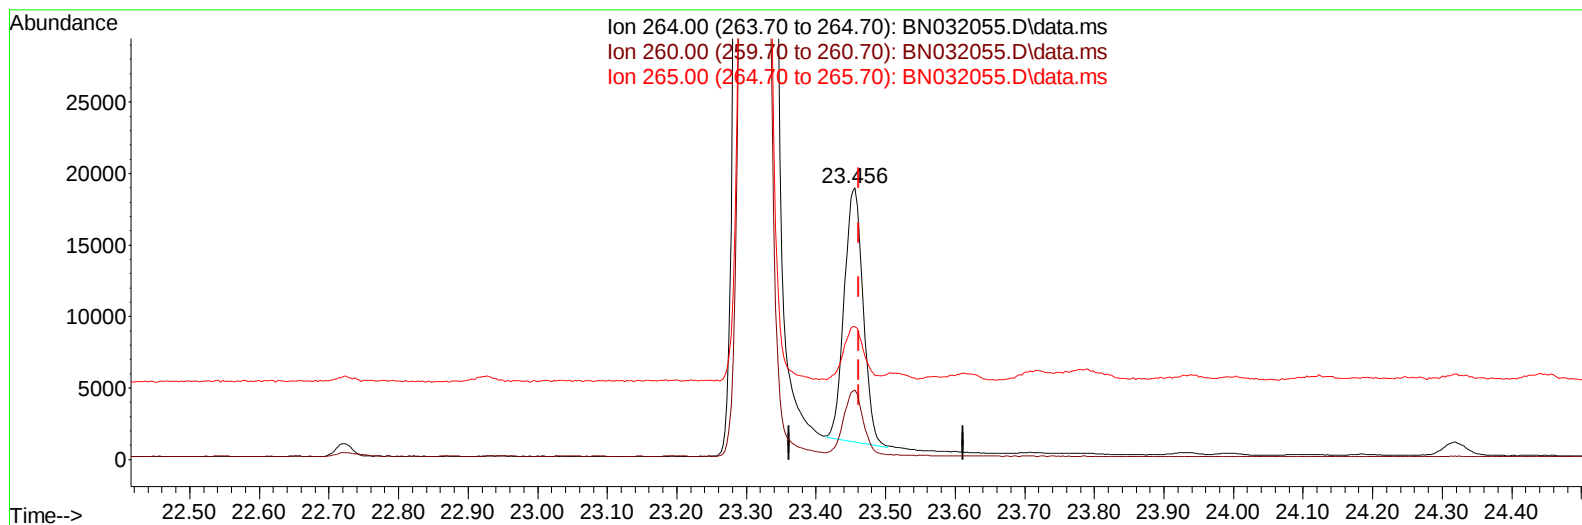

TIC: BN032055.D\data.ms

(23) Perylene-d12 (I)

23.456min (-0.006) 0.40 ng/ul m

response 33381

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.50	25.49
265.00	53.40	48.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032055.D
Acq On : 18 Jun 2024 21:32
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Manual IntegrationsAPPROVED

Quant Time: Jun 18 22:56:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

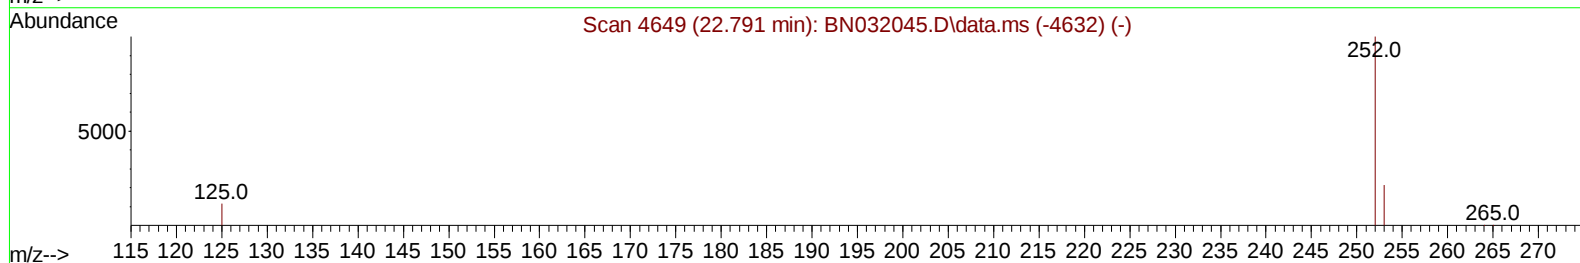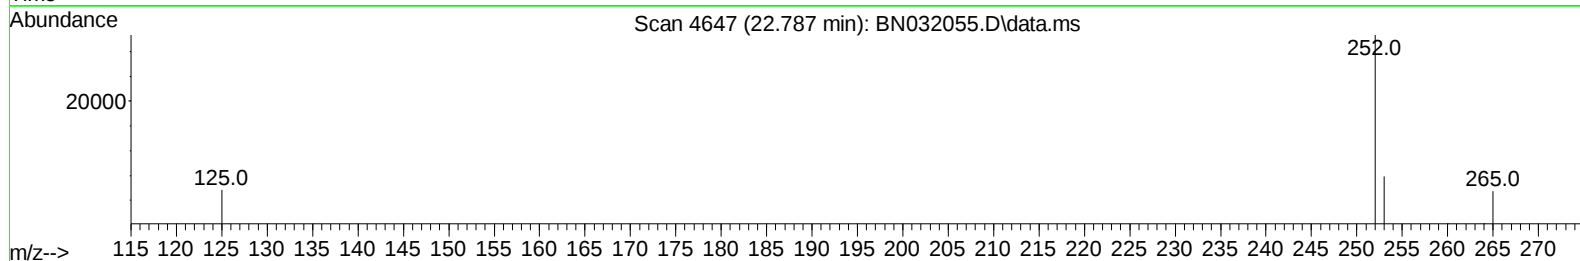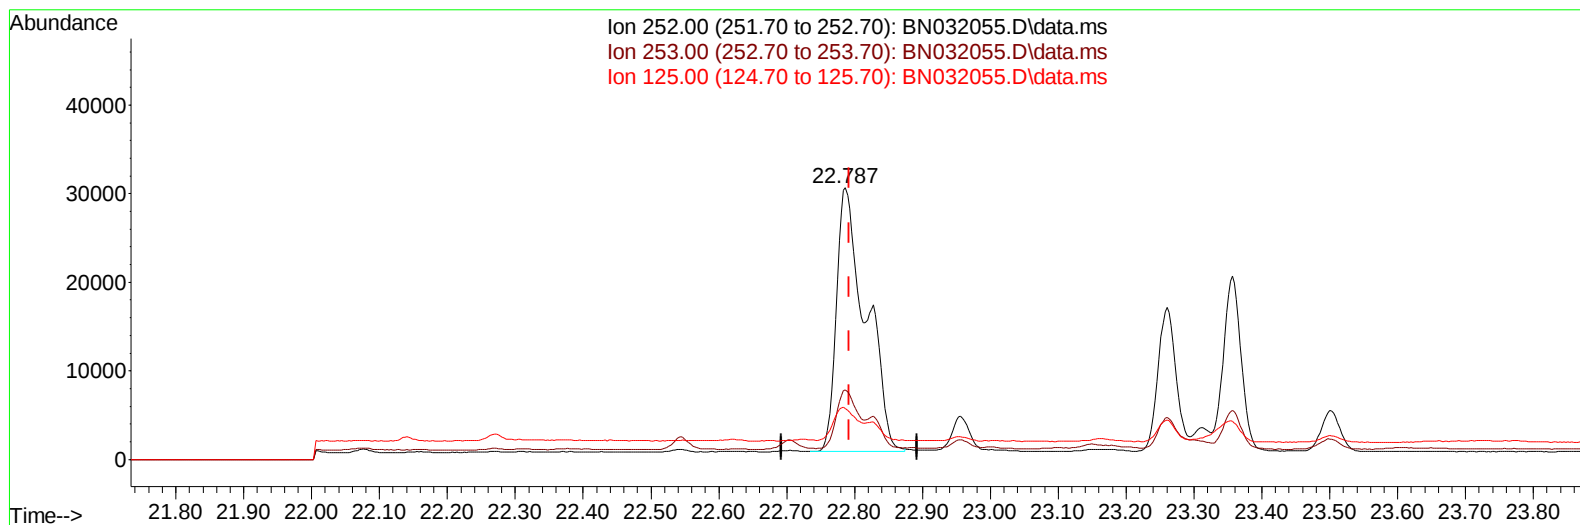

TIC: BN032055.D\data.ms

(24) Benzo(b)fluoranthene

22.787min (-0.006) 0.61 ng/u1

response 89540

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.70	25.70
125.00	14.40	18.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032055.D
Acq On : 18 Jun 2024 21:32
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Manual IntegrationsAPPROVED

Quant Time: Jun 18 22:56:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

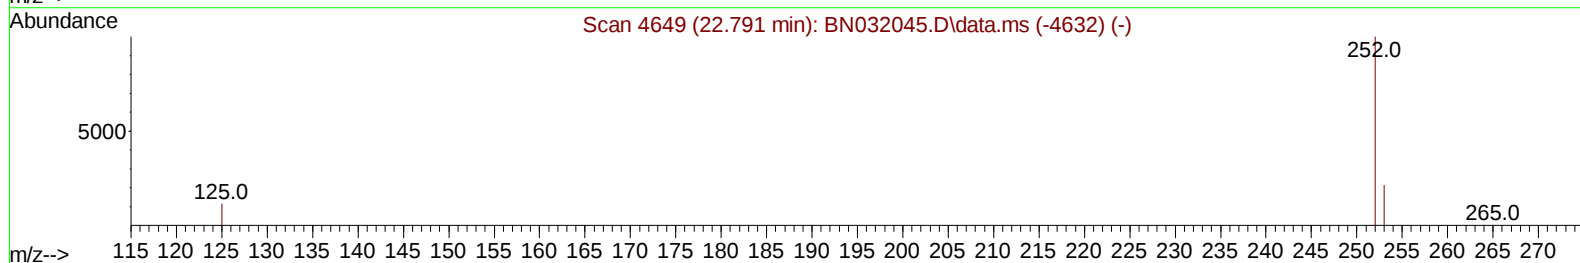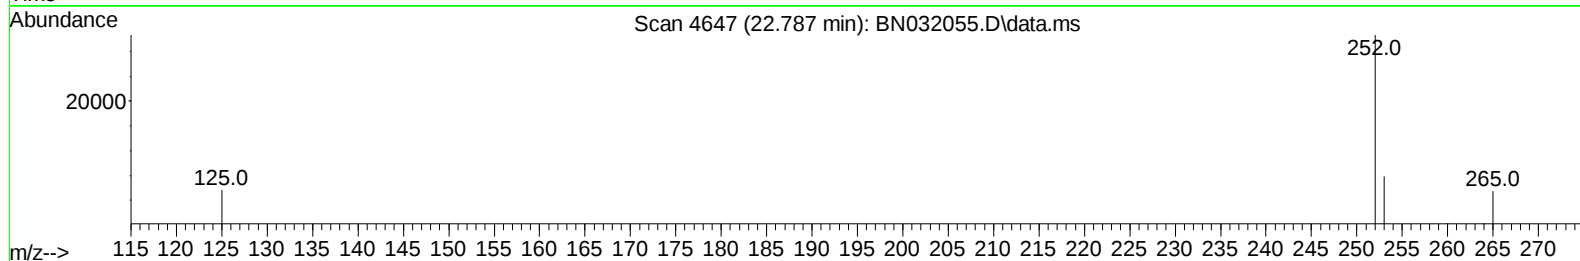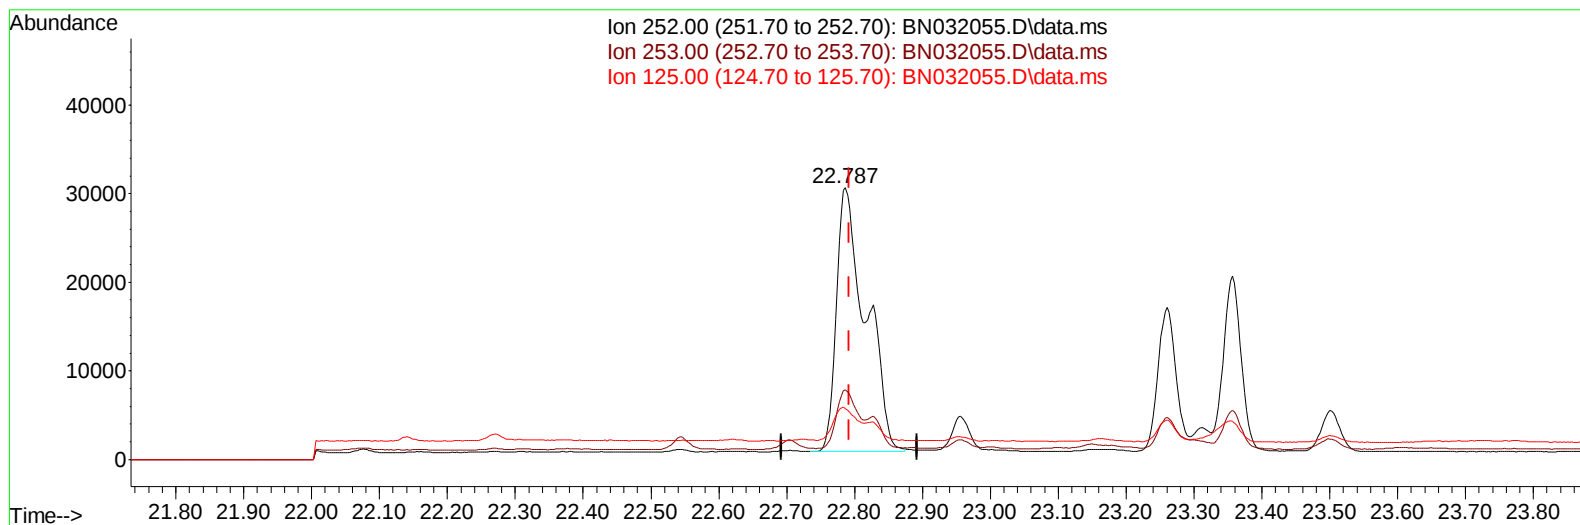

TIC: BN032055.D\data.ms

(24) Benzo(b)fluoranthene

22.787min (-0.006) 0.61 ng/u1

response 89540

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.70	25.70
125.00	14.40	18.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032055.D
Acq On : 18 Jun 2024 21:32
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Manual IntegrationsAPPROVED

Quant Time: Jun 18 22:56:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

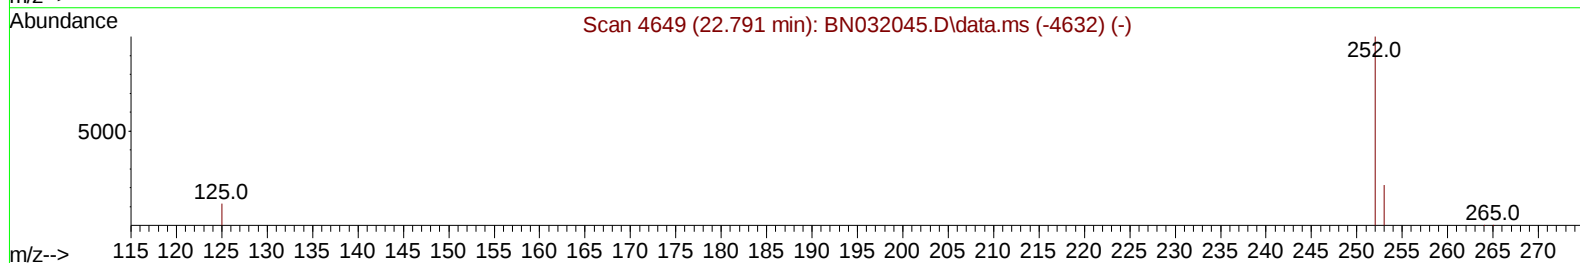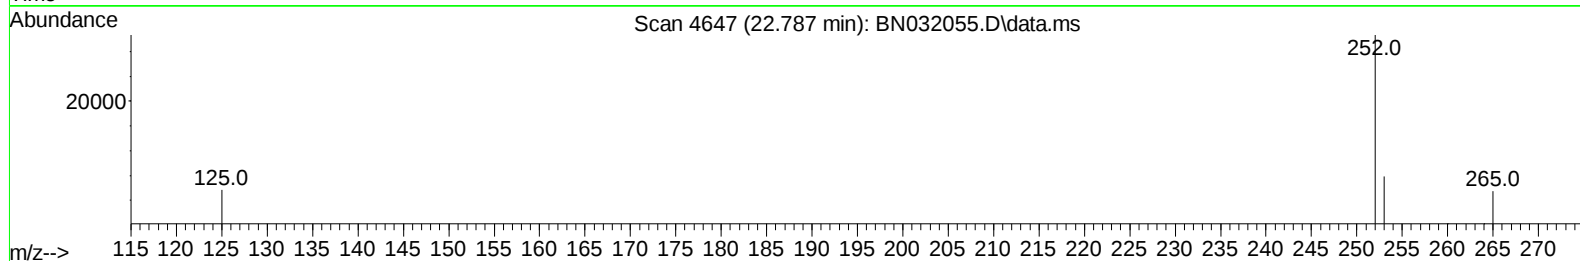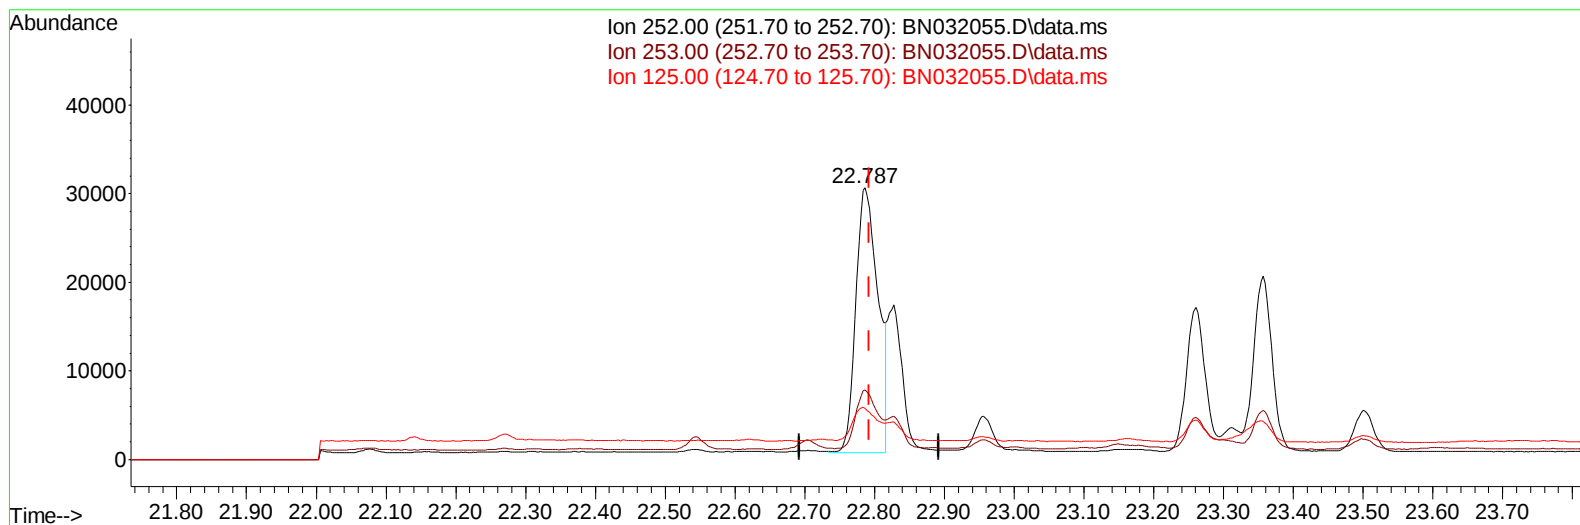

TIC: BN032055.D\data.ms

(24) Benzo(b)fluoranthene

22.787min (-0.006) 0.45 ng/u1 m

response 66043

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.70	25.70
125.00	14.40	18.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032055.D
Acq On : 18 Jun 2024 21:32
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Manual IntegrationsAPPROVED

Quant Time: Jun 18 22:56:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

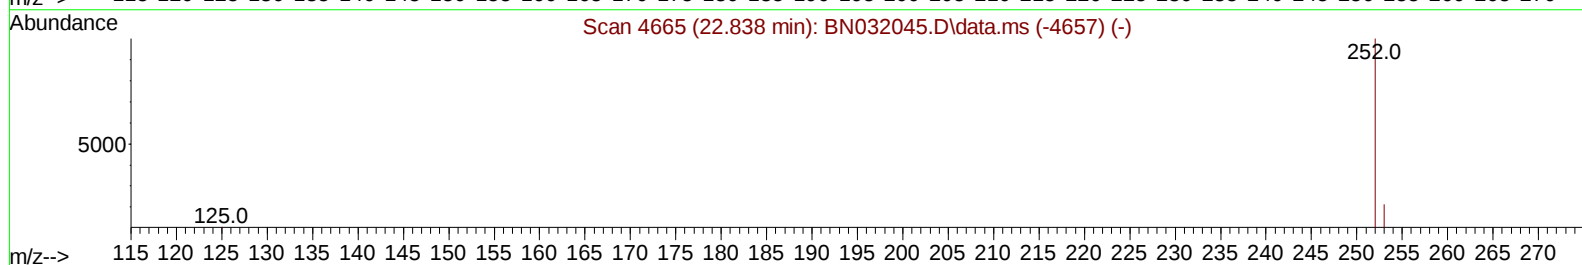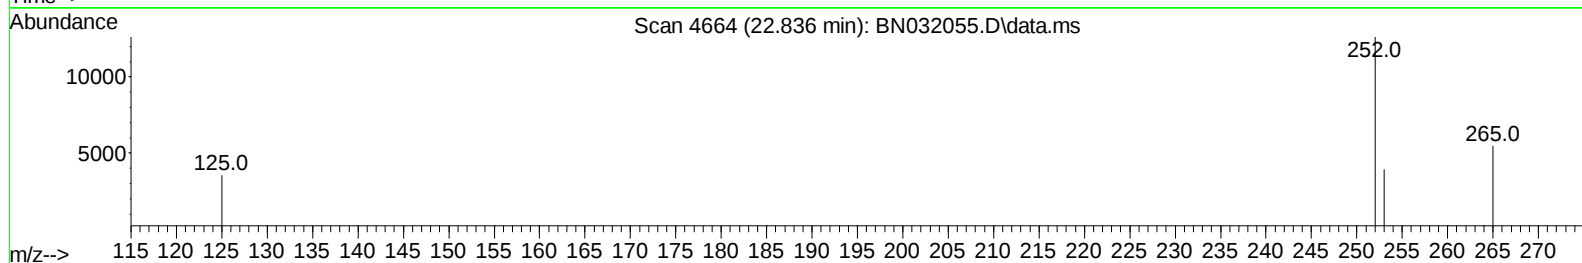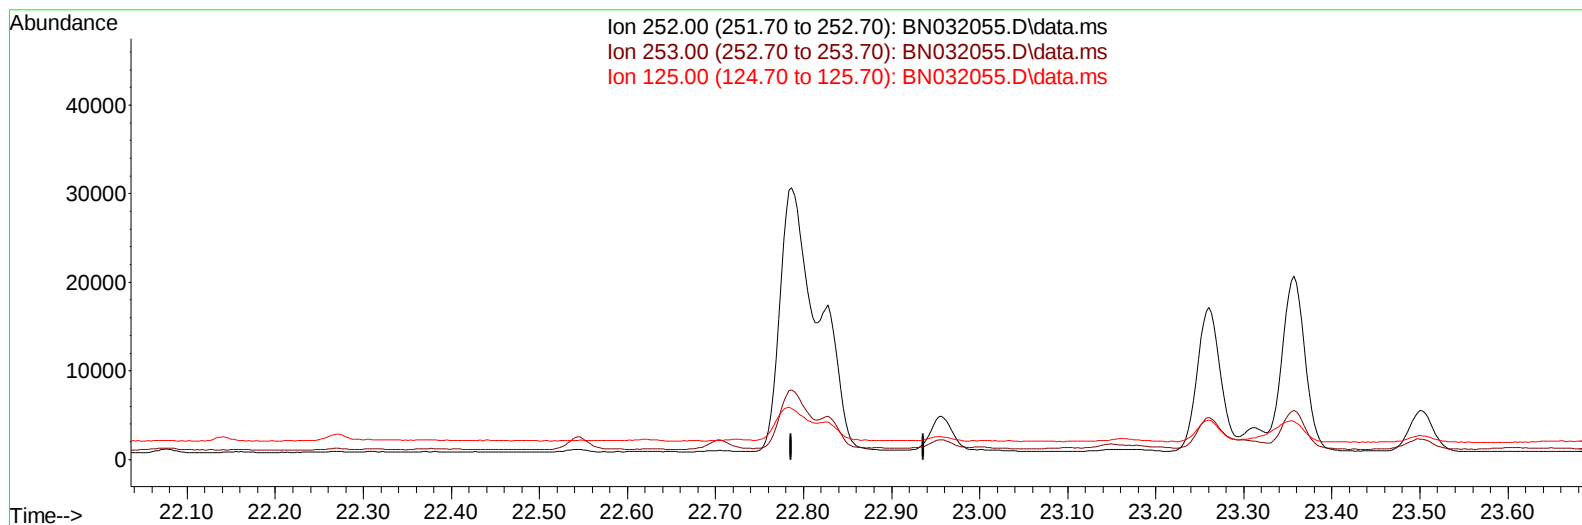

TIC: BN032055.D\data.ms

(25) Benzo(k)fluoranthene

22.836min (-22.836) 0.00 ng/u1

response 0

Ion	Exp%	Act%
252.00	100.00	0.00
253.00	23.50	0.00#
125.00	13.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032055.D
Acq On : 18 Jun 2024 21:32
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Manual IntegrationsAPPROVED

Quant Time: Jun 18 22:56:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

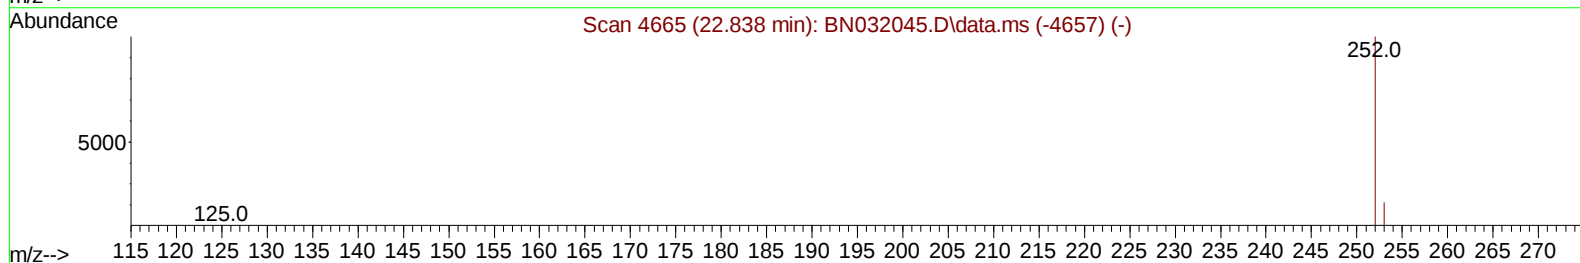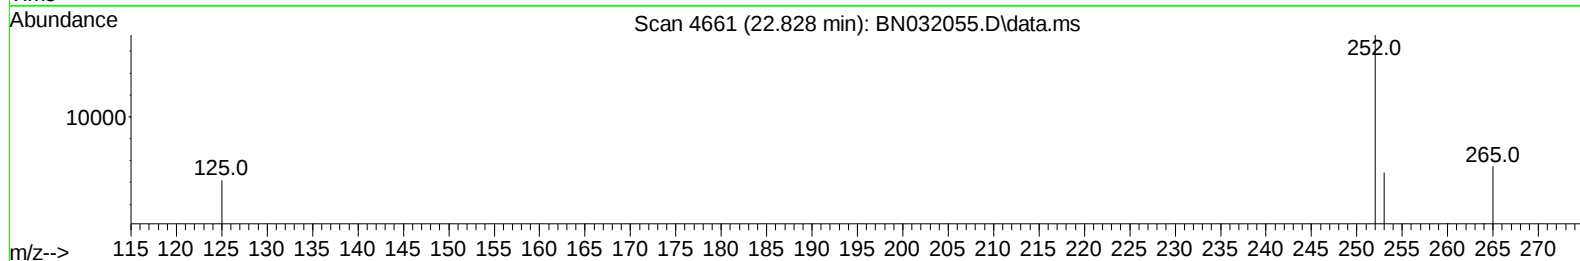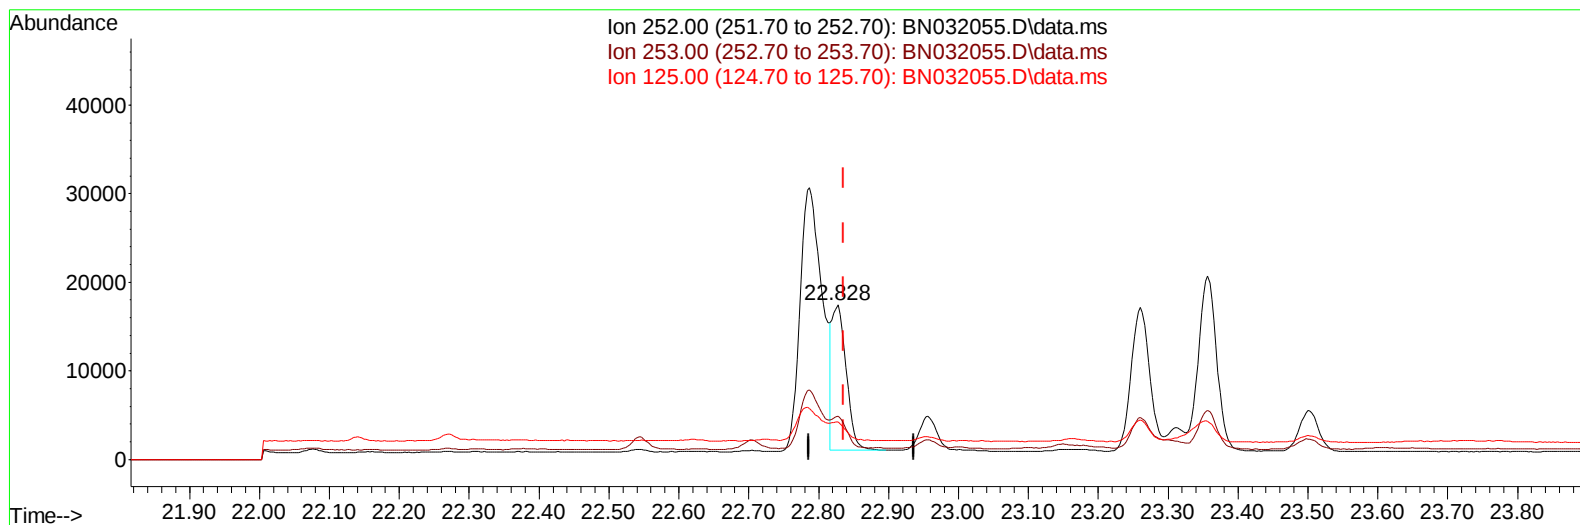

TIC: BN032055.D\data.ms

(25) Benzo(k)fluoranthene

22.828min (-0.009) 0.17 ng/u1 m

response 23418

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.50	28.14
125.00	13.90	24.16#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
 Data File : BN032055.D
 Acq On : 18 Jun 2024 21:32
 Operator : MA/JU
 Sample : P2696-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BN8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/19/2024
 Supervised By :mohammad ahmed 06/21/2024

Quant Time: Jun 18 22:56:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 14:06:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.650	152	11020	0.400	ng/ul	0.00
4) Naphthalene-d8	10.426	136	39218	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.290	164	24260	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.037	188	50398	0.400	ng/ul	0.00
17) Chrysene-d12	21.232	240	36090	0.400	ng/ul	0.00
23) Perylene-d12	23.456	264	33381m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	35277	2.986	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.021	152	11954	0.188	ng/ul	0.00
18) Fluoranthene-d10	19.073	212	24524	0.225	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.475	128	2777	0.027	ng/ul#	89
10) Acenaphthylene	14.008	152	3340	0.032	ng/ul#	87
11) Acenaphthene	14.355	153	1644	0.021	ng/ul	99
15) Phenanthrene	17.079	178	42282	0.298	ng/ul	99
16) Anthracene	17.172	178	7166	0.056	ng/ul#	92
19) Fluoranthene	19.101	202	100079	0.753	ng/ul	100
20) Pyrene	19.468	202	84676	0.608	ng/ul	98
21) Benzo(a)anthracene	21.214	228	39254	0.284	ng/ul	97
22) Chrysene	21.267	228	46101	0.334	ng/ul	97
24) Benzo(b)fluoranthene	22.787	252	66043m	0.450	ng/ul	
25) Benzo(k)fluoranthene	22.828	252	23418m	0.166	ng/ul	
26) Benzo(a)pyrene	23.357	252	36352	0.349	ng/ul#	94
27) Indeno(1,2,3-cd)pyrene	25.697	276	30989	0.220	ng/ul#	92
28) Dibenzo(a,h)anthracene	25.703	278	8154	0.075	ng/ul#	71
29) Benzo(g,h,i)perylene	26.387	276	31090	0.278	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061824\
Data File : BN032055.D
Acq On : 18 Jun 2024 21:32
Operator : MA/JU
Sample : P2696-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BN8

Manual IntegrationsAPPROVED

Quant Time: Jun 18 22:56:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 14:06:13 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/19/2024
Supervised By :mohammad ahmed 06/21/2024

