
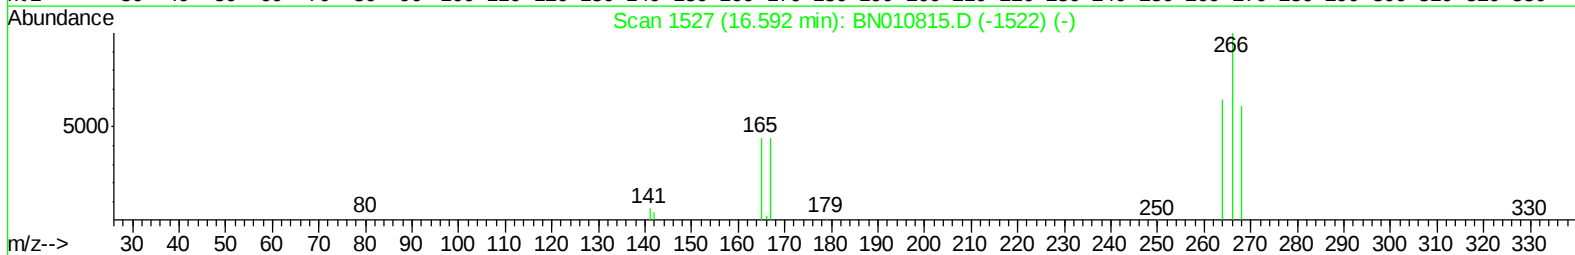
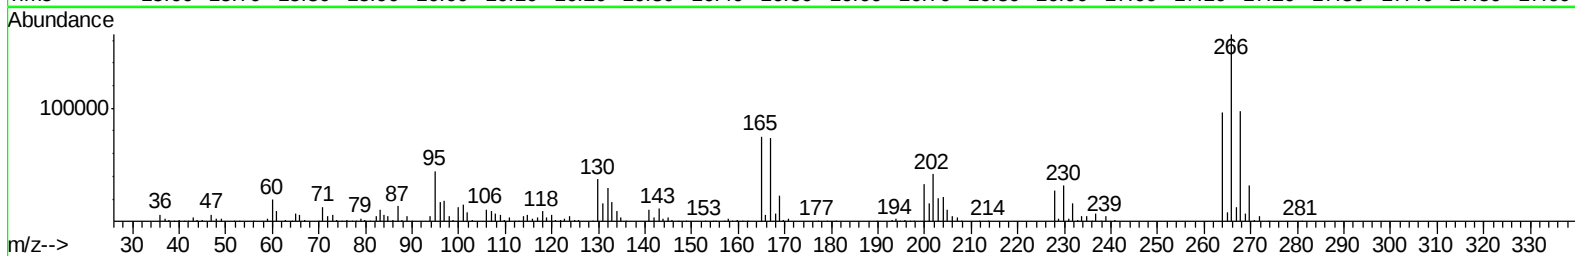


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061920\
Data File : BN010963.D
Acq On : 19 Jun 2020 11:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 07:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 19 12:43:49 2020
Response via : Initial Calibration

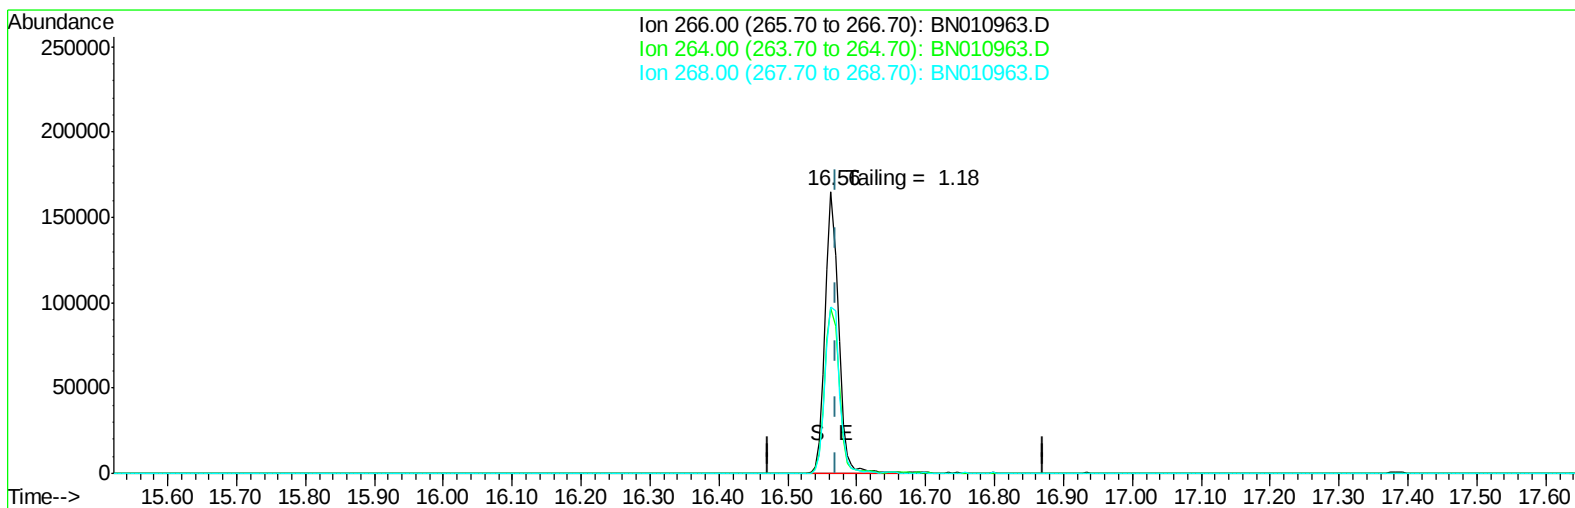

TIC: BN010963.D

(22) Pentachlorophenol

16.563min (-0.008) 0.00ng

response 221692

Ion	Exp%	Act%
266.00	100	100
264.00	68.50	58.55
268.00	69.90	58.97
0.00	0.00	0.00