

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061920\
 Data File : BN010972.D
 Acq On : 19 Jun 2020 16:23
 Operator : CG/JU
 Sample : L3043-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW203D1-20200614

Quant Time: Jun 19 17:04:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 19 12:43:49 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	2132	0.40	ng	0.00
7) Naphthalene-d8	10.28	136	6813	0.40	ng	0.00
13) Acenaphthene-d10	14.16	164	3876	0.40	ng	0.00
19) Phenanthrene-d10	16.91	188	8031	0.40	ng	0.01
27) Chrysene-d12	21.12	240	7419	0.40	ng	0.00
34) Perylene-d12	23.26	264	7792	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.18	112	713	0.17	ng	0.00
5) Phenol-d6	6.73	99	506	0.10	ng	0.00
8) Nitrobenzene-d5	8.67	82	2236	0.44	ng	0.00
11) 2-Methylnaphthalene-d10	11.88	152	4848	0.46	ng	0.00
14) 2,4,6-Tribromophenol	15.66	330	563	0.41	ng	0.01
15) 2-Fluorobiphenyl	12.78	172	7481	0.49	ng	0.00
25) Fluoranthene-d10	18.95	212	12569	0.57	ng	0.00
29) Terphenyl-d14	19.56	244	10068	0.58	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.21	88	3609	1.728	ng	Qvalue # 96
32) Bis(2-ethylhexyl)phthalate	21.06	149	1020	0.140	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061920\
Data File : BN010972.D
Acq On : 19 Jun 2020 16:23
Operator : CG/JU
Sample : L3043-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW203D1-20200614

Quant Time: Jun 19 17:04:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 19 12:43:49 2020
Response via : Initial Calibration

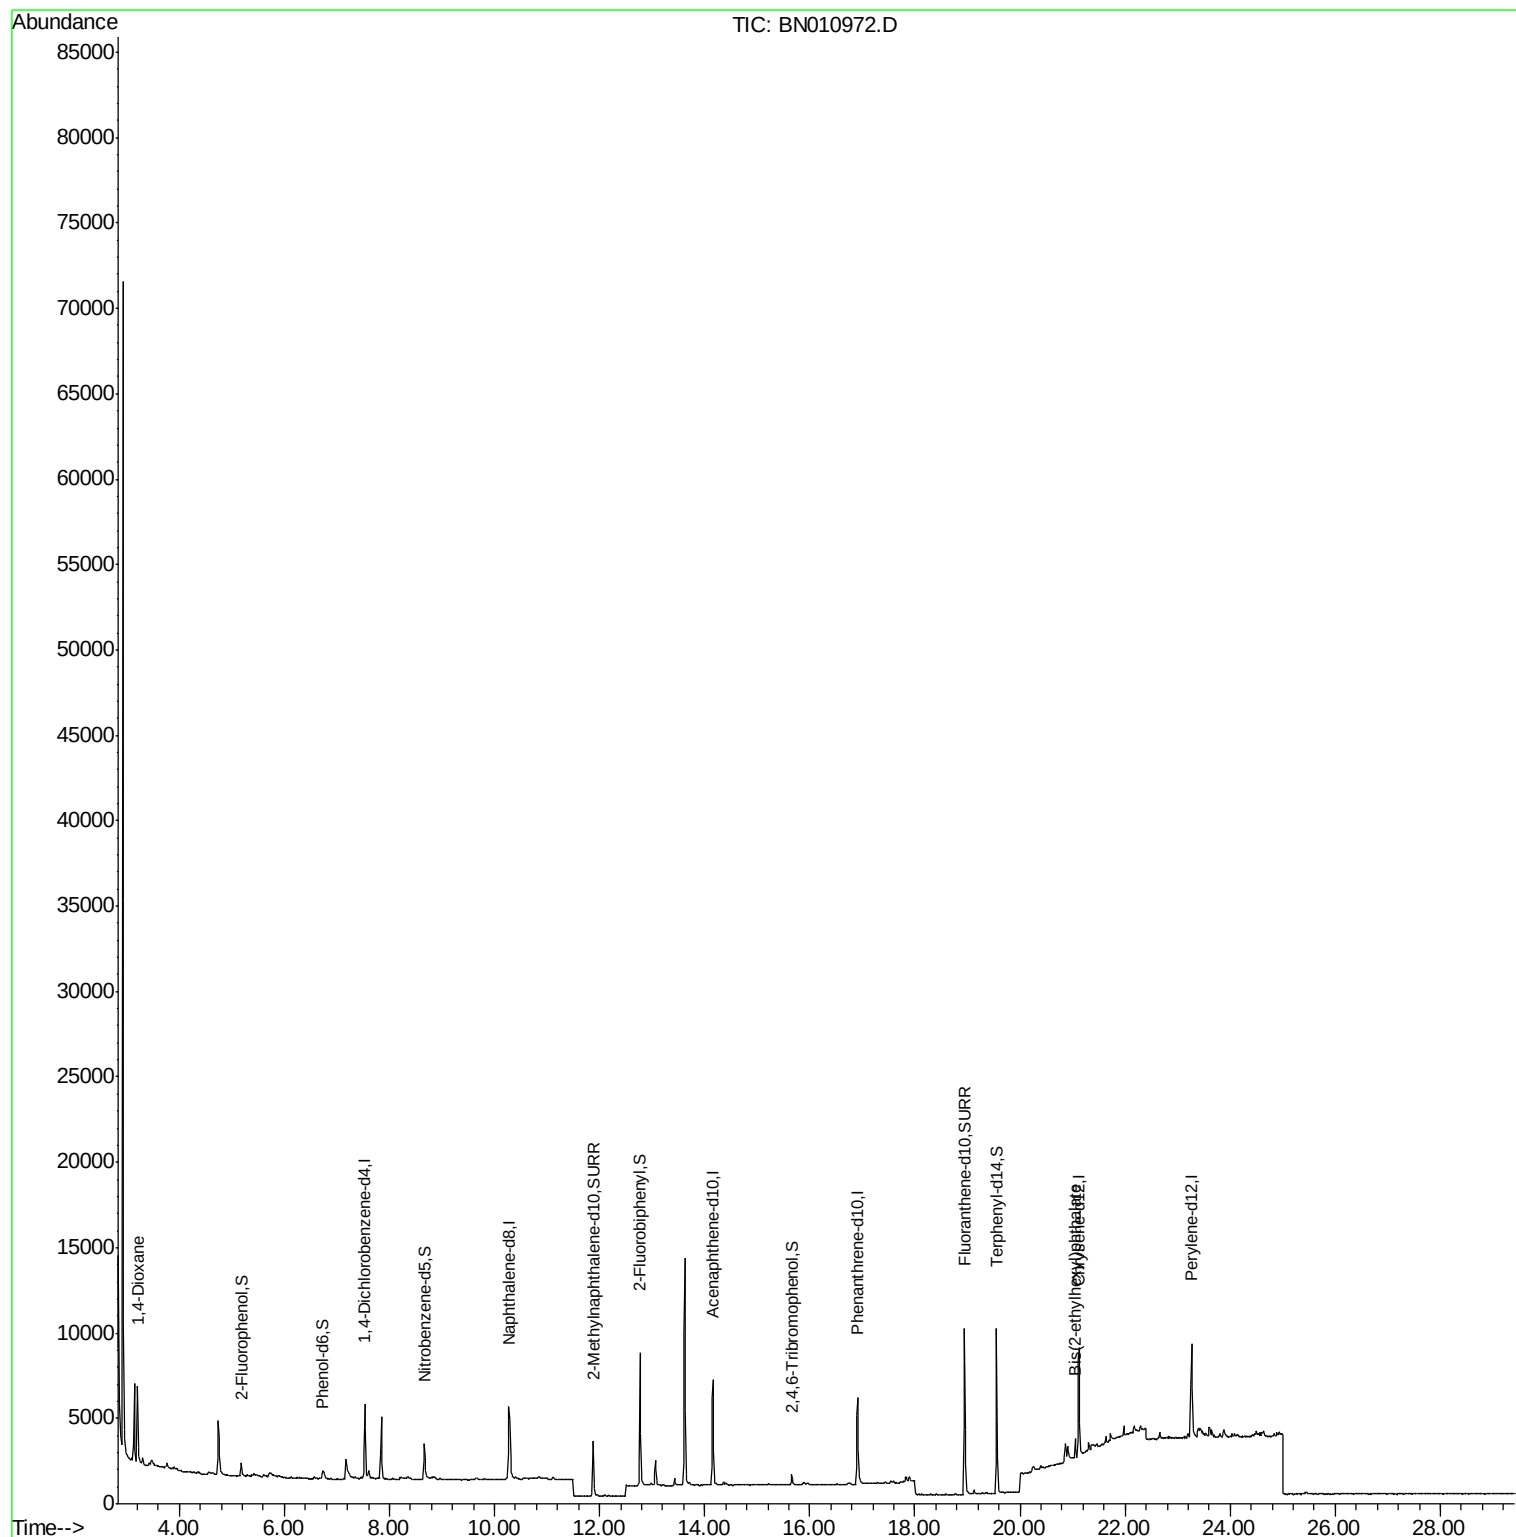


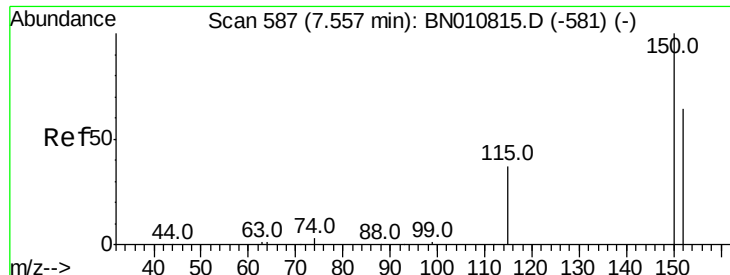




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.53 min Scan# 584
 Delta R.T. -0.00 min
 Lab File: BN010972.D
 Acq: 19 Jun 2020 16:23

Instrument :
 BNA_N
 ClientSampleId :
 MW203D1-20200614

Tot Ion:152 Resp: 2132
 Ion Ratio Lower Upper
 152 100
 150 154.1 123.8 185.6
 115 60.9 49.2 73.8

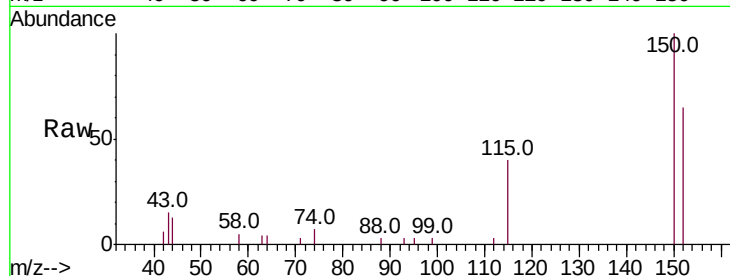


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

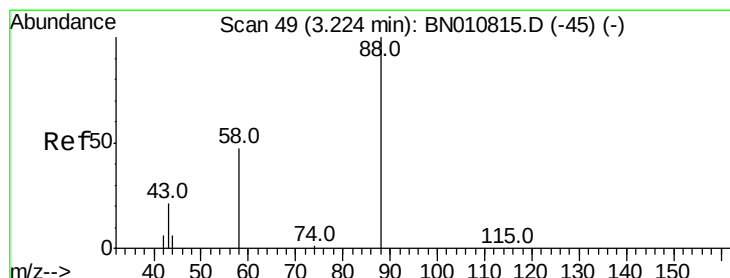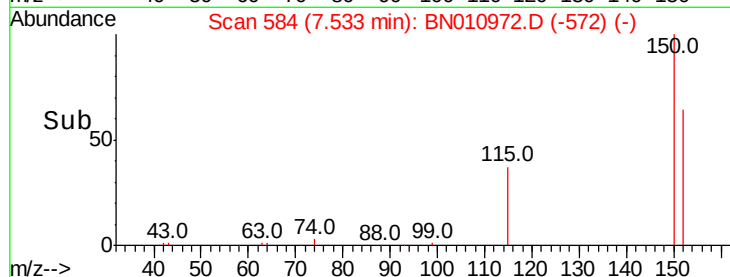
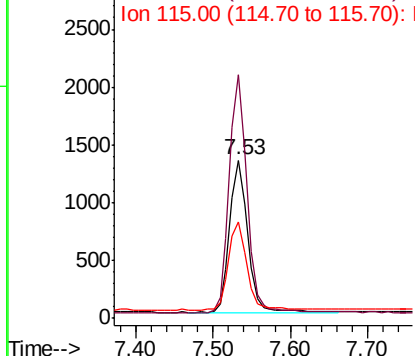



#2
 1,4-Dioxane
 Concen: 1.728 ng
 RT: 3.21 min Scan# 47
 Delta R.T. -0.01 min
 Lab File: BN010972.D
 Acq: 19 Jun 2020 16:23

Tgt Ion: 88 Resp: 3609
 Ion Ratio Lower Upper
 88 100
 58 46.2 38.2 57.4
 43 23.2 15.1 22.7#

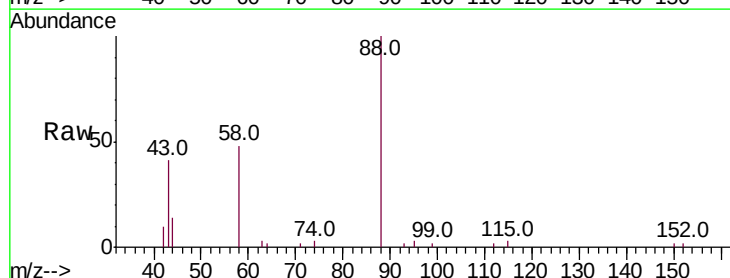

Abundance Ion 88.00 (87.70 to 88.70): BNC
 Ion 58.00 (57.70 to 58.70): BNC
 Ion 43.00 (42.70 to 43.70): BNC

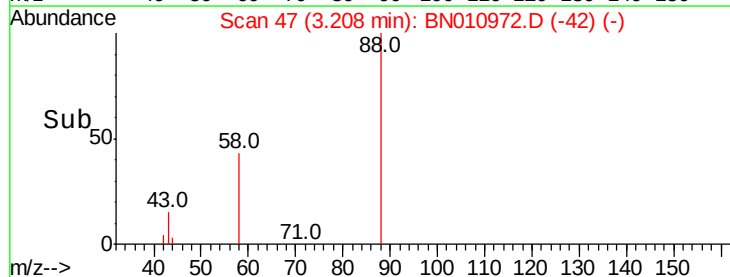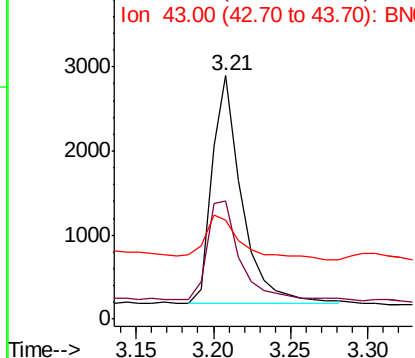

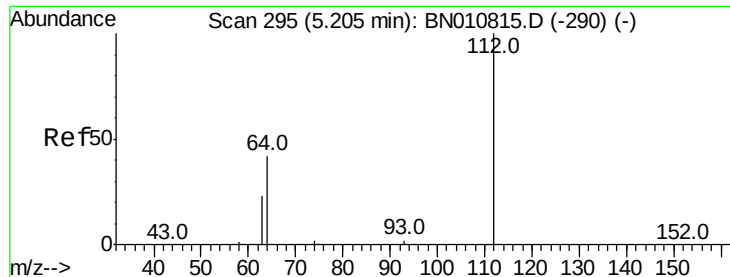

#4

2-Fluorophenol

Concen: 0.173 ng

RT: 5.18 min Scan# 292

Delta R.T. -0.00 min

Lab File: BN010972.D

Acq: 19 Jun 2020 16:23

Instrument :

BNA_N

ClientSampleId :

MW203D1-20200614


Tot Ion:112 Resp: 713

Ion Ratio Lower Upper

112 100

64 48.4 37.4 56.0




63 26.9 22.2 33.4

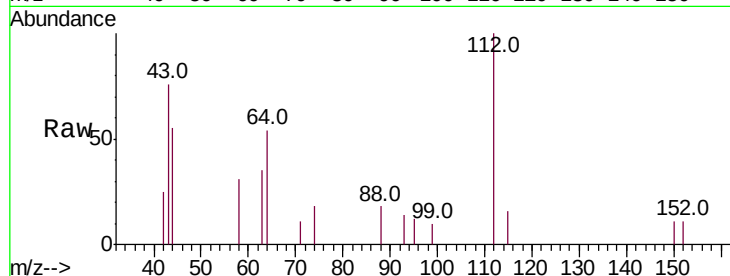

Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): BNO

Ion 63.00 (62.70 to 63.70): BNO

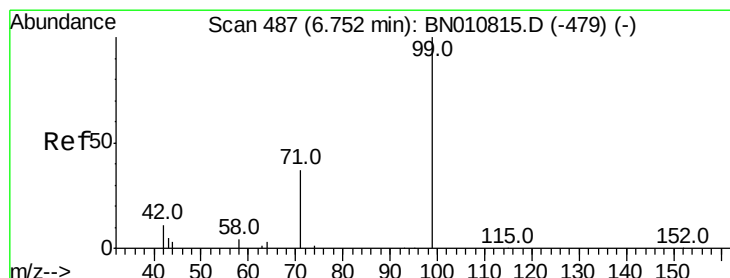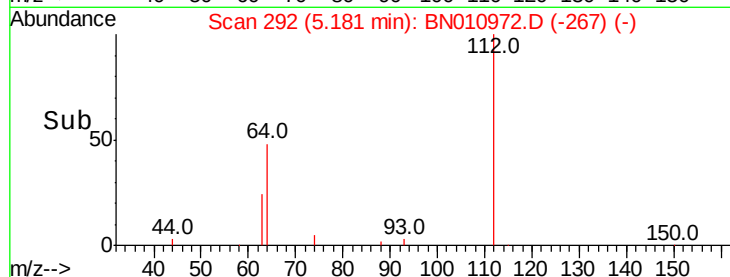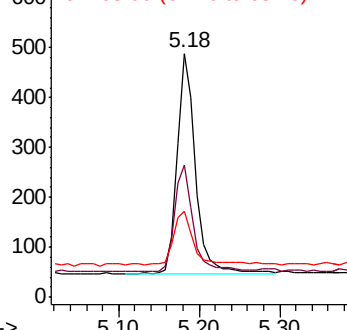

#5

Phenol-d6

Concen: 0.104 ng

RT: 6.73 min Scan# 484

Delta R.T. -0.00 min

Lab File: BN010972.D

Acq: 19 Jun 2020 16:23


Tgt Ion: 99 Resp: 506

Ion Ratio Lower Upper

99 100

42 16.0 11.1 16.7



71 38.3 31.4 47.2

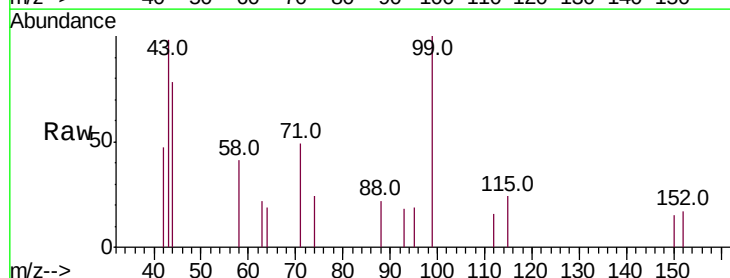


Abundance Ion 99.00 (98.70 to 99.70): BNO

Ion 42.00 (41.70 to 42.70): BNO

Ion 71.00 (70.70 to 71.70): BNO

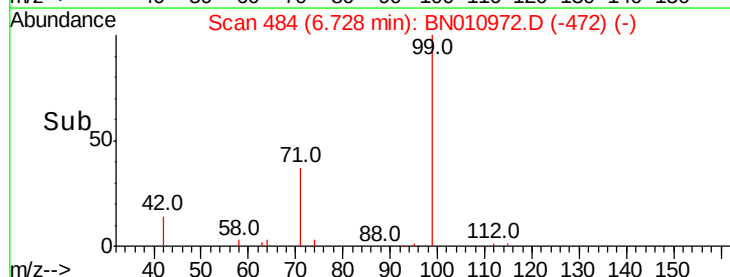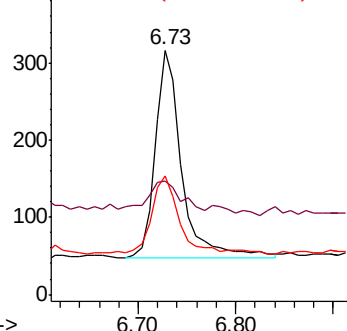



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.28 min Scan# 836

Delta R.T. -0.00 min

Lab File: BN010972.D

Acq: 19 Jun 2020 16:23

Instrument :

BNA_N

ClientSampleId :

MW203D1-20200614

Tot Ion:136 Resp: 6813



Ion Ratio Lower Upper

136 100

137 12.5 9.7 14.5

54 6.2 4.9 7.3

68 6.9 4.7 7.1





Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

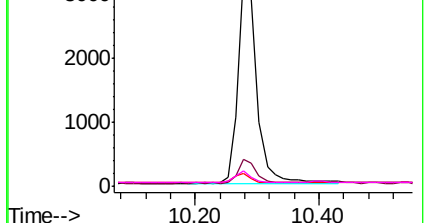

#8

Nitrobenzene-d5

Concen: 0.443 ng

RT: 8.67 min Scan# 709

Delta R.T. -0.00 min

Lab File: BN010972.D

Acq: 19 Jun 2020 16:23



Tgt Ion: 82 Resp: 2236

Ion Ratio Lower Upper

82 100

128 45.5 35.4 53.0


54 34.4 28.2 42.4




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC




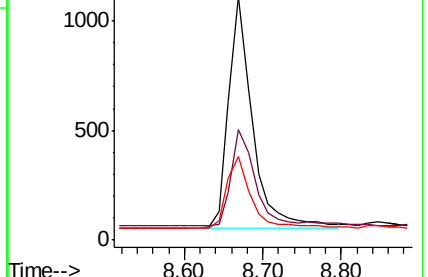




#11
2-Methylnaphthalene-d10
Concen: 0.459 ng
RT: 11.88 min Scan# 1016
Delta R.T. -0.00 min
Lab File: BN010972.D
Acq: 19 Jun 2020 16:23




Instrument :
BNA_N
ClientSampleId :
MW203D1-20200614


Tot Ion:152 Resp: 4848
Ion Ratio Lower Upper
152 100
151 19.1 15.3 22.9

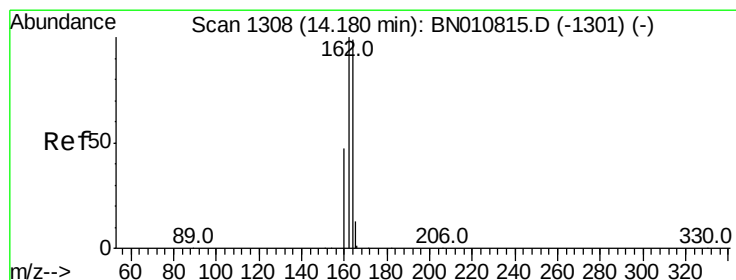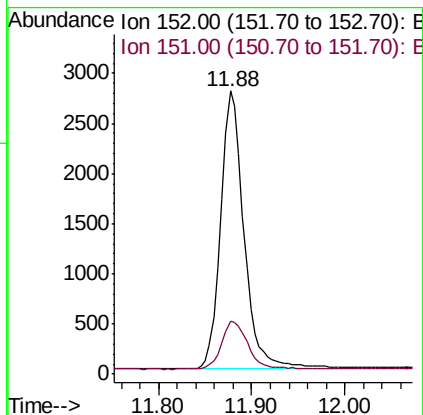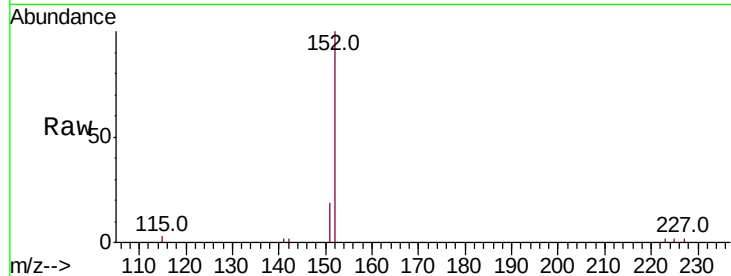

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.16 min Scan# 1306
Delta R.T. -0.00 min
Lab File: BN010972.D
Acq: 19 Jun 2020 16:23

Tgt Ion:164 Resp: 3876
Ion Ratio Lower Upper
164 100
162 98.4 81.0 121.6
160 45.7 38.9 58.3


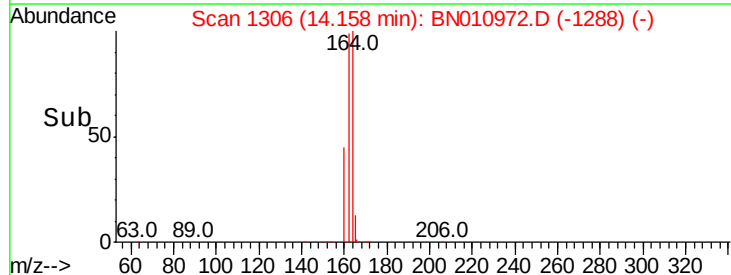
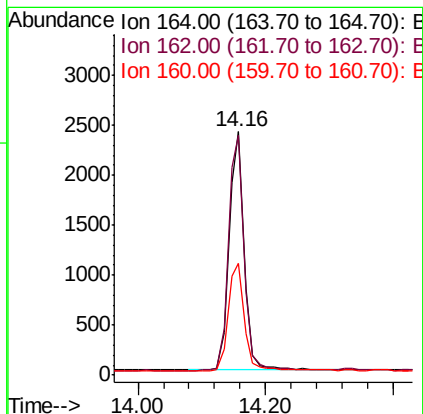
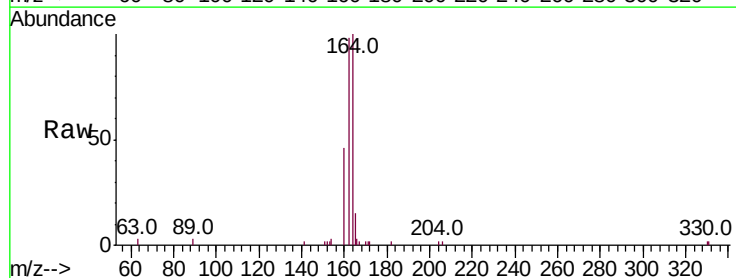




#14
 2,4,6-Tribromophenol
 Concen: 0.406 ng
 RT: 15.66 min Scan# 1441
 Delta R.T. 0.01 min
 Lab File: BN010972.D
 Acq: 19 Jun 2020 16:23




Instrument :
 BNA_N
 ClientSampleId :
 MW203D1-20200614


Tot Ion:330 Resp: 563
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 42.5 33.2 49.8

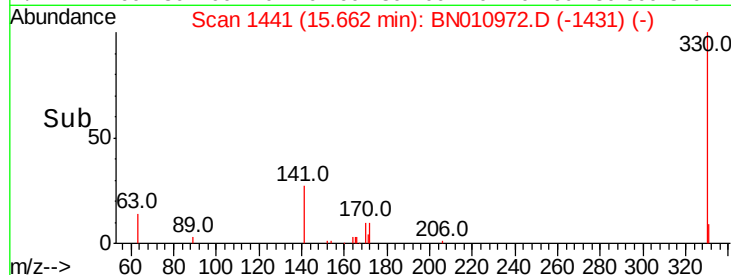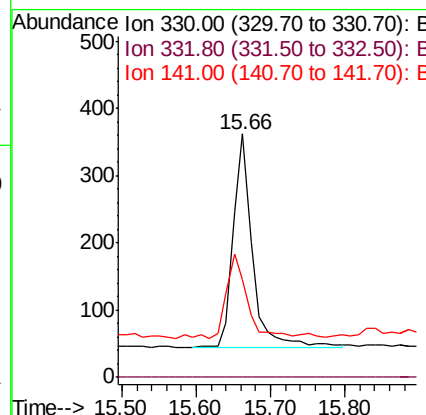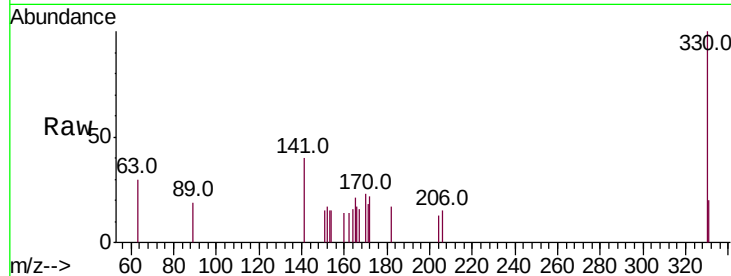

#15
 2-Fluorobiphenyl
 Concen: 0.489 ng
 RT: 12.78 min Scan# 1182
 Delta R.T. -0.00 min
 Lab File: BN010972.D
 Acq: 19 Jun 2020 16:23

Tgt Ion:172 Resp: 7481
 Ion Ratio Lower Upper
 172 100
 171 35.3 28.5 42.7
 170 23.4 19.7 29.5

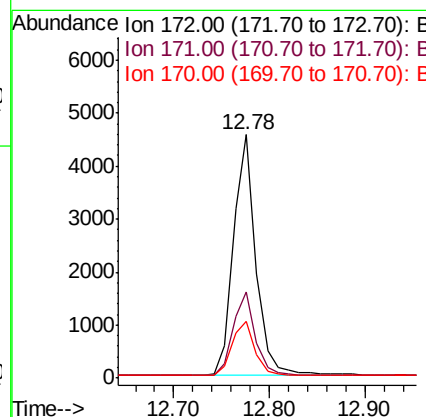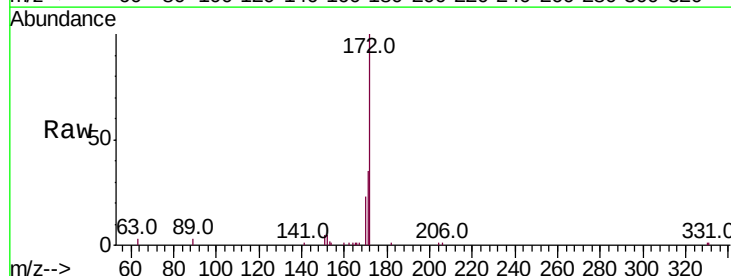

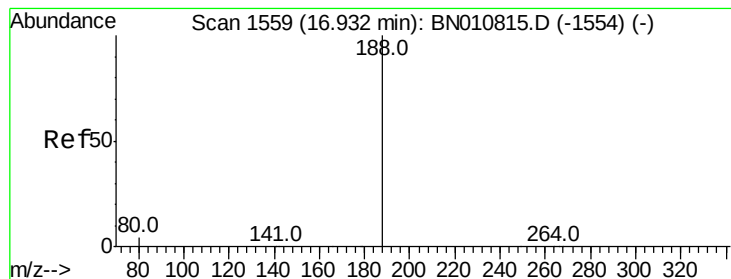

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.91 min Scan# 1557

Delta R.T. 0.01 min

Lab File: BN010972.D

Acq: 19 Jun 2020 16:23

Instrument :

BNA_N

ClientSampleId :

MW203D1-20200614


Tot Ion:188 Resp: 8031

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 7.1 4.5 6.7#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNO

Ion 80.00 (79.70 to 80.70): BNO

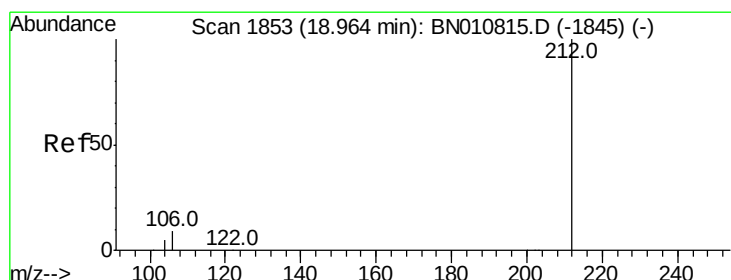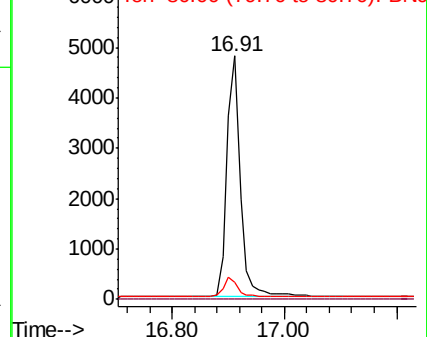

#25

Fluoranthene-d10

Concen: 0.567 ng

RT: 18.95 min Scan# 1850

Delta R.T. 0.00 min

Lab File: BN010972.D

Acq: 19 Jun 2020 16:23


Tgt Ion:212 Resp: 12569

Ion Ratio Lower Upper

212 100

106 9.6 6.6 10.0



104 5.7 4.0 6.0




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

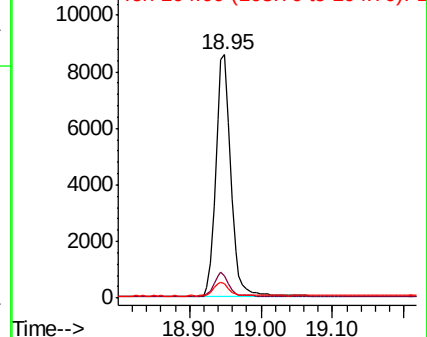



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.12 min Scan# 2168

Delta R.T. -0.00 min

Lab File: BN010972.D

Acq: 19 Jun 2020 16:23

Instrument :

BNA_N

ClientSampleId :

MW203D1-20200614


Tot Ion:240 Resp: 7419

Ion Ratio Lower Upper

240 100

120 7.4 7.5 11.3#




236 27.5 22.3 33.5



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

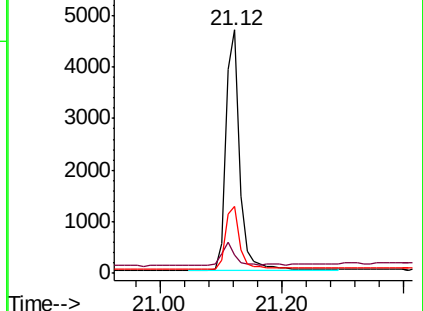

#29

Terphenyl-d14

Concen: 0.580 ng

RT: 19.56 min Scan# 1973

Delta R.T. -0.00 min

Lab File: BN010972.D

Acq: 19 Jun 2020 16:23


Tgt Ion:244 Resp: 10068

Ion Ratio Lower Upper

244 100

212 8.7 7.4 11.2



122 9.8 7.5 11.3




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

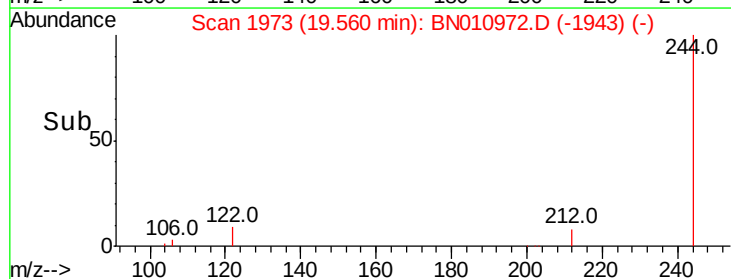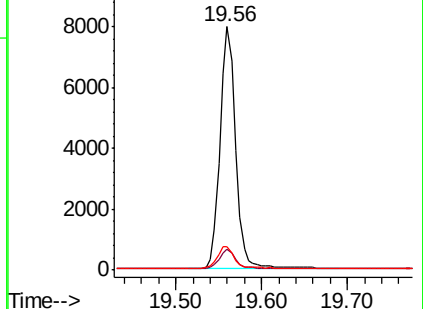



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.140 ng

RT: 21.06 min Scan# 2162

Delta R.T. -0.00 min

Lab File: BN010972.D

Acq: 19 Jun 2020 16:23

Instrument :

BNA_N

ClientSampleId :

MW203D1-20200614


Tot Ion:149 Resp: 1020

Ion Ratio Lower Upper

149 100

167 26.8 24.1 36.1




279 5.5 4.6 7.0



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

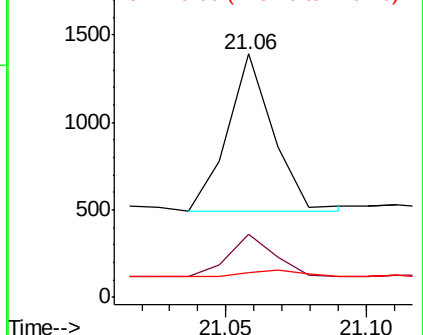

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.26 min Scan# 2539

Delta R.T. -0.00 min

Lab File: BN010972.D

Acq: 19 Jun 2020 16:23


Tgt Ion:264 Resp: 7792

Ion Ratio Lower Upper

264 100

260 24.9 20.4 30.6

265 84.1 75.0 112.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

