

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061920\
 Data File : BN010980.D
 Acq On : 19 Jun 2020 21:10
 Operator : CG/JU
 Sample : L3043-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW202D1-20200613

Quant Time: Jun 20 06:17:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 19 12:43:49 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	2126	0.40	ng	0.00
7) Naphthalene-d8	10.28	136	6670	0.40	ng	0.00
13) Acenaphthene-d10	14.15	164	3744	0.40	ng	0.00
19) Phenanthrene-d10	16.91	188	7826	0.40	ng	0.00
27) Chrysene-d12	21.11	240	7005	0.40	ng	0.00
34) Perylene-d12	23.26	264	8107	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.18	112	695	0.17	ng	0.00
5) Phenol-d6	6.73	99	468	0.10	ng	0.00
8) Nitrobenzene-d5	8.67	82	2174	0.44	ng	0.00
11) 2-Methylnaphthalene-d10	11.88	152	3012	0.29	ng	0.00
14) 2,4,6-Tribromophenol	15.66	330	523	0.39	ng	0.00
15) 2-Fluorobiphenyl	12.77	172	5833	0.39	ng	0.00
25) Fluoranthene-d10	18.95	212	7991	0.37	ng	0.00
29) Terphenyl-d14	19.56	244	8749	0.53	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.21	88	743	0.357	ng	# 85
32) Bis(2-ethylhexyl)phthalate	21.06	149	462	0.067	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061920\
Data File : BN010980.D
Acq On : 19 Jun 2020 21:10
Operator : CG/JU
Sample : L3043-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW202D1-20200613

Quant Time: Jun 20 06:17:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 19 12:43:49 2020
Response via : Initial Calibration

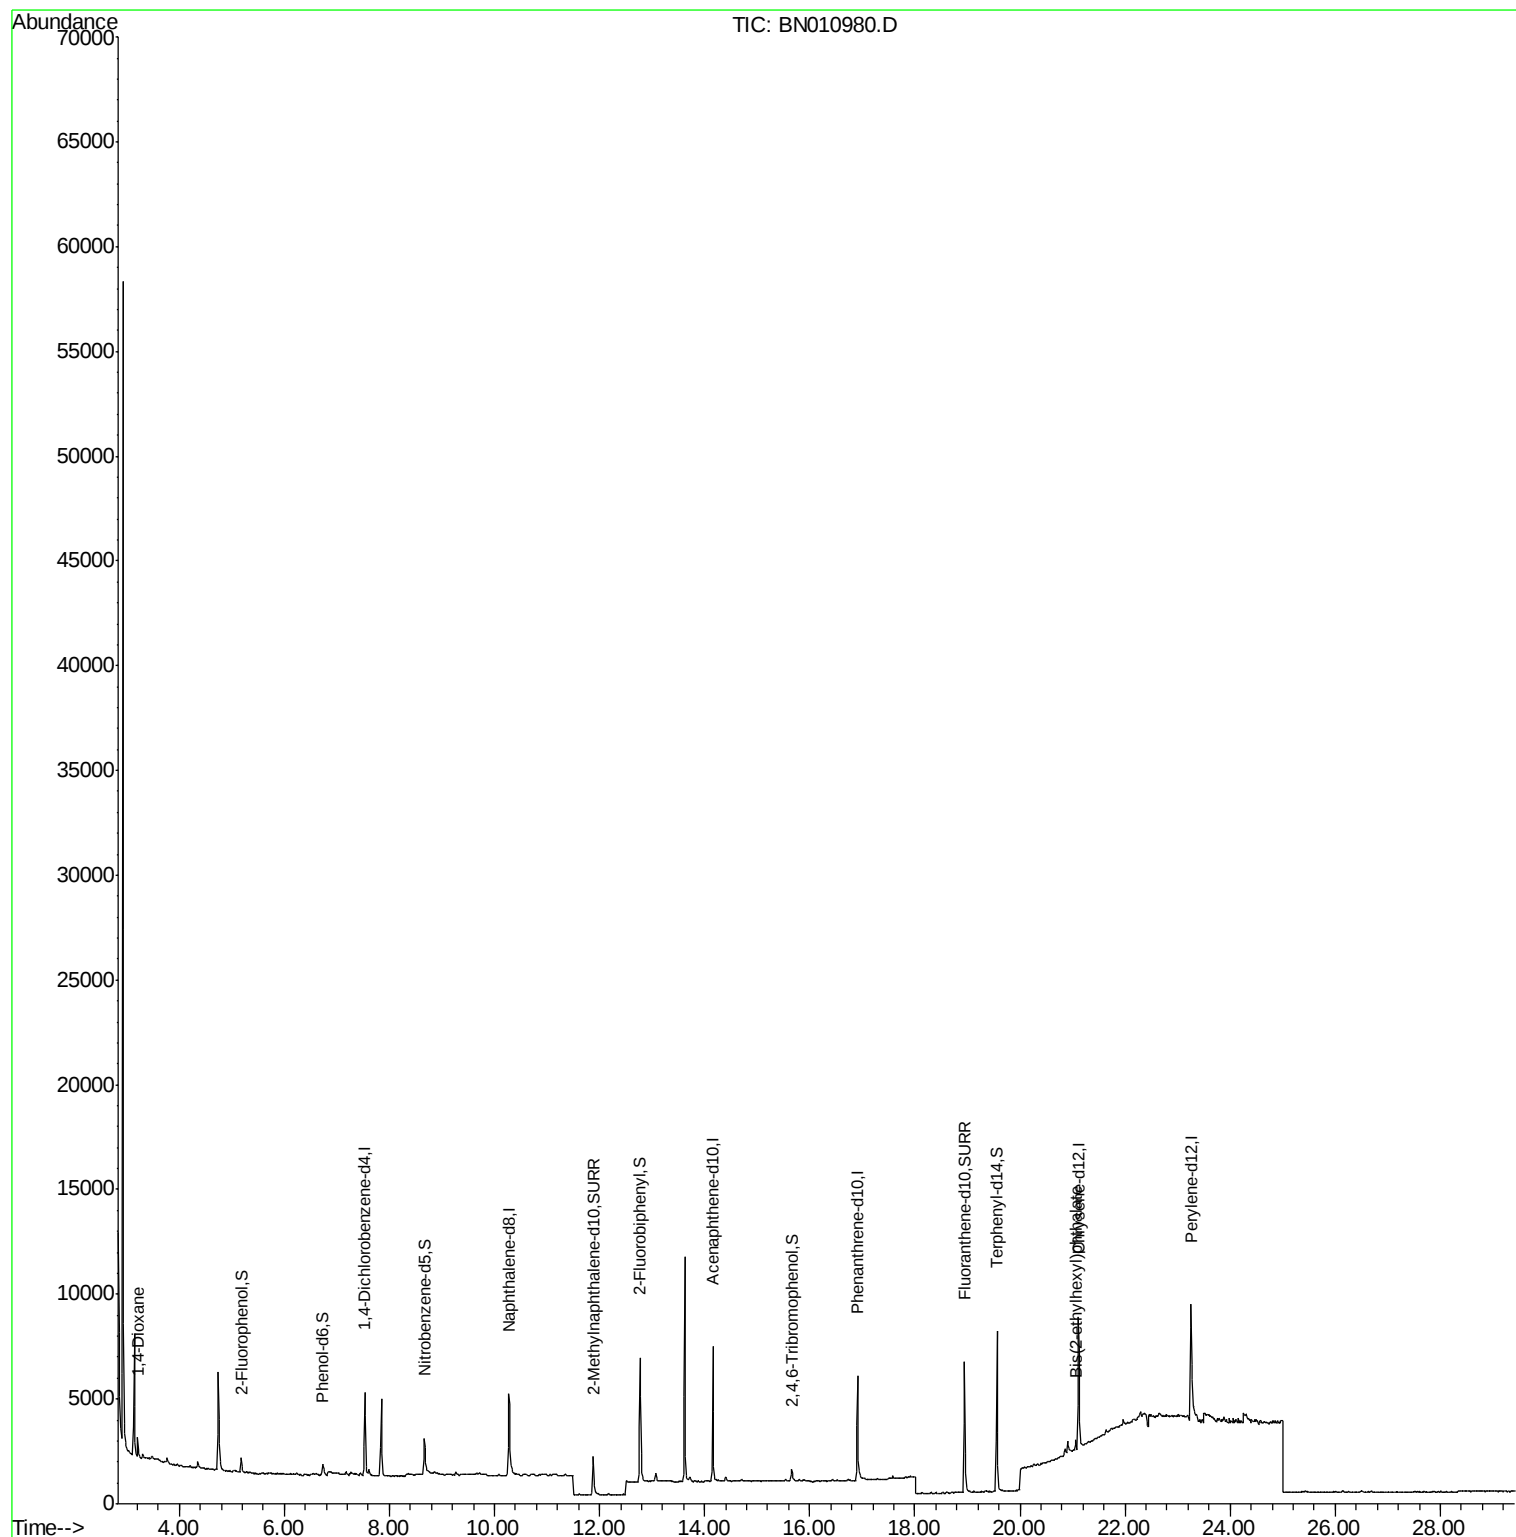

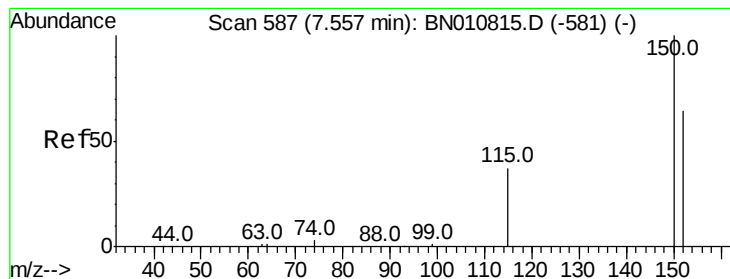

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.53 min Scan# 584

Delta R.T. 0.00 min

Lab File: BN010980.D

Acq: 19 Jun 2020 21:10

Instrument :

BNA_N

ClientSampleId :

MW202D1-20200613


Tot Ion:152 Resp: 2126

Ion Ratio Lower Upper

152 100

150 148.8 123.8 185.6




115 57.6 49.2 73.8

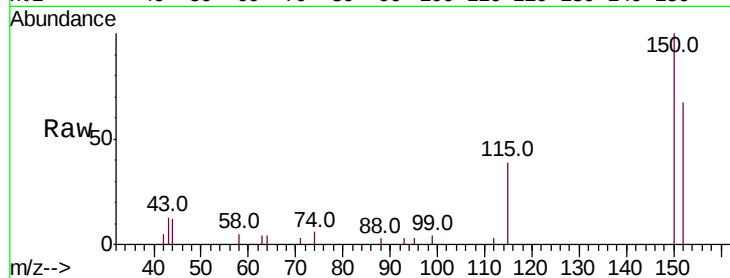

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

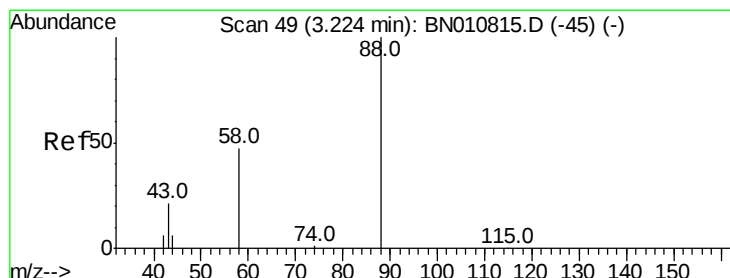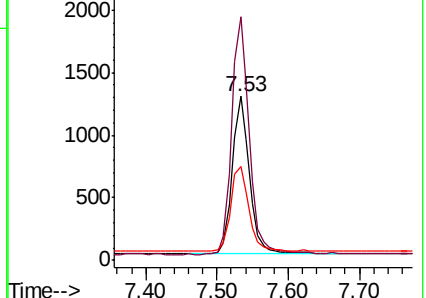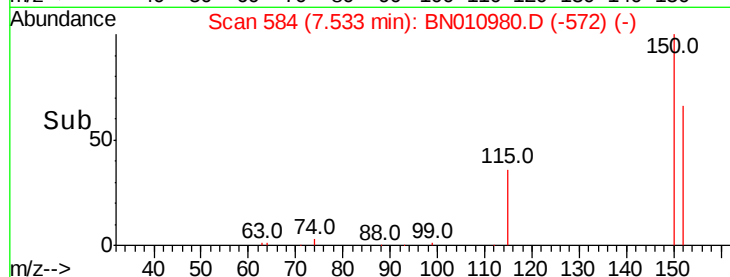

#2

1,4-Dioxane

Concen: 0.357 ng

RT: 3.21 min Scan# 47

Delta R.T. -0.01 min

Lab File: BN010980.D

Acq: 19 Jun 2020 21:10


Tgt Ion: 88 Resp: 743

Ion Ratio Lower Upper

88 100

58 49.8 38.2 57.4



43 39.7 15.1 22.7#

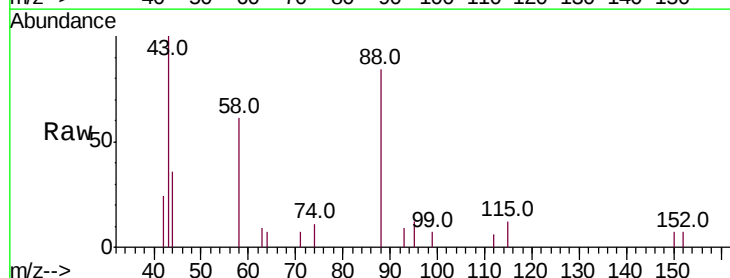


Abundance Ion 88.00 (87.70 to 88.70): BNC

Ion 58.00 (57.70 to 58.70): BNC

Ion 43.00 (42.70 to 43.70): BNC

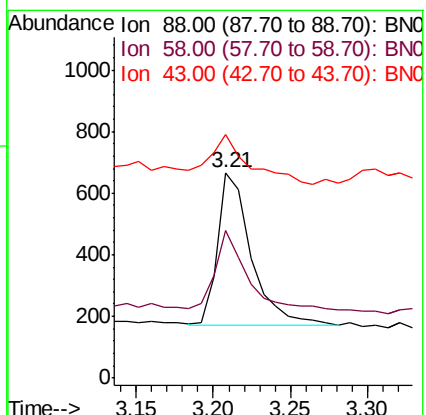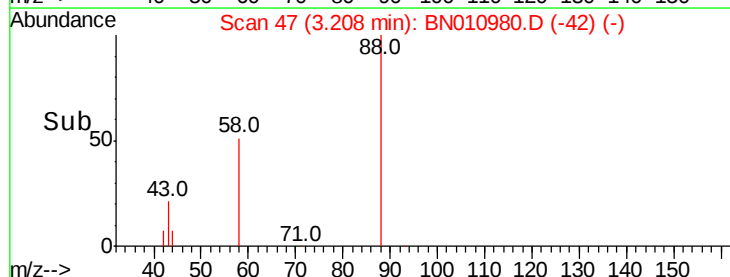



#4

2-Fluorophenol

Concen: 0.169 ng

RT: 5.18 min Scan# 292

Delta R.T. 0.00 min

Lab File: BN010980.D

Acq: 19 Jun 2020 21:10

Instrument :

BNA_N

ClientSampleId :

MW202D1-20200613


Tot Ion:112 Resp: 695

Ion Ratio Lower Upper

112 100

64 46.0 37.4 56.0


63 25.6 22.2 33.4

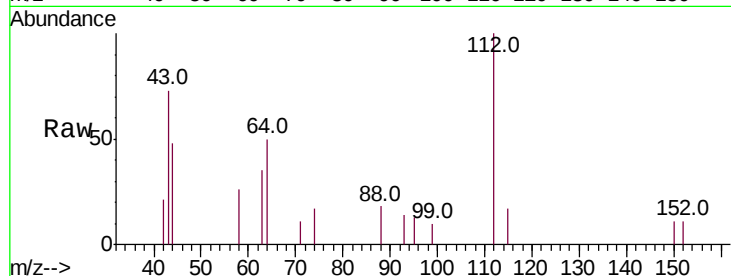



Abundance Ion 112.00 (111.70 to 112.70): BNC

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

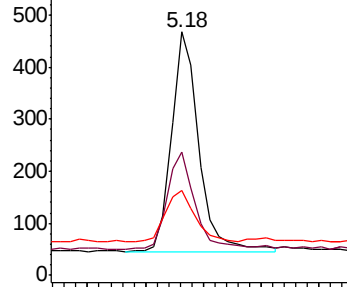

Time-->



#5

Phenol-d6

Concen: 0.097 ng

RT: 6.73 min Scan# 484

Delta R.T. 0.00 min

Lab File: BN010980.D

Acq: 19 Jun 2020 21:10


Tgt Ion: 99 Resp: 468

Ion Ratio Lower Upper

99 100

42 17.5 11.1 16.7#


71 42.7 31.4 47.2




Abundance Ion 99.00 (98.70 to 99.70): BNC


Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

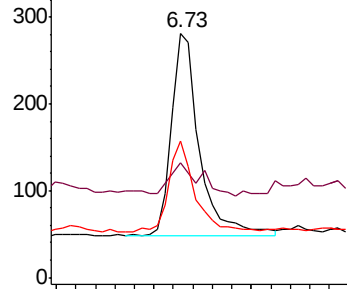

Time-->





#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.28 min Scan# 836

Delta R.T. 0.00 min

Lab File: BN010980.D

Acq: 19 Jun 2020 21:10

Instrument :

BNA_N

ClientSampleId :

MW202D1-20200613

Tot Ion:136 Resp: 6670



Ion Ratio Lower Upper

136 100

137 12.3 9.7 14.5

54 6.4 4.9 7.3

68 6.9 4.7 7.1


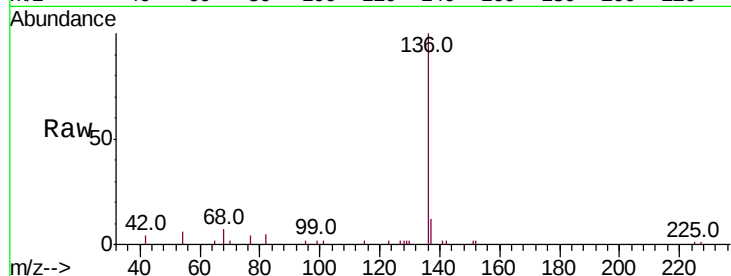


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

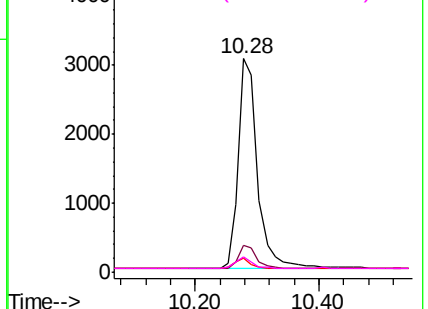

#8

Nitrobenzene-d5

Concen: 0.440 ng

RT: 8.67 min Scan# 709

Delta R.T. 0.00 min

Lab File: BN010980.D

Acq: 19 Jun 2020 21:10



Tgt Ion: 82 Resp: 2174

Ion Ratio Lower Upper

82 100

128 42.6 35.4 53.0


54 35.7 28.2 42.4




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC




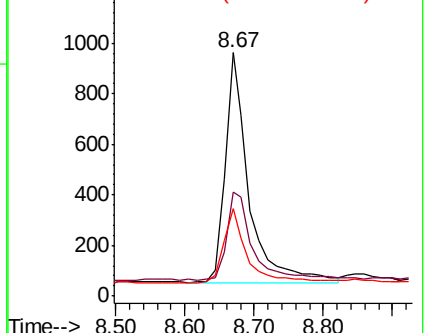




#11
2-Methylnaphthalene-d10
Concen: 0.291 ng
RT: 11.88 min Scan# 1017
Delta R.T. 0.00 min
Lab File: BN010980.D
Acq: 19 Jun 2020 21:10




Instrument :
BNA_N
ClientSampleId :
MW202D1-20200613


Tot Ion:152 Resp: 3012
Ion Ratio Lower Upper
152 100
151 19.2 15.3 22.9

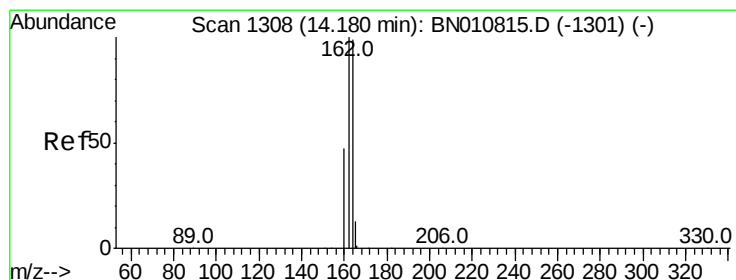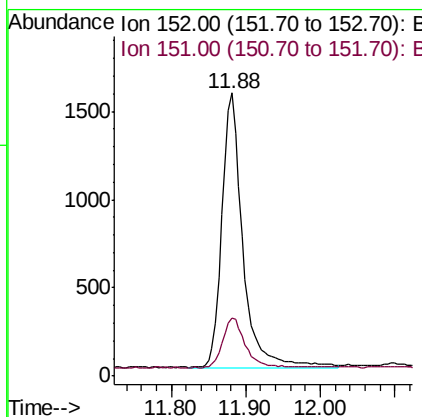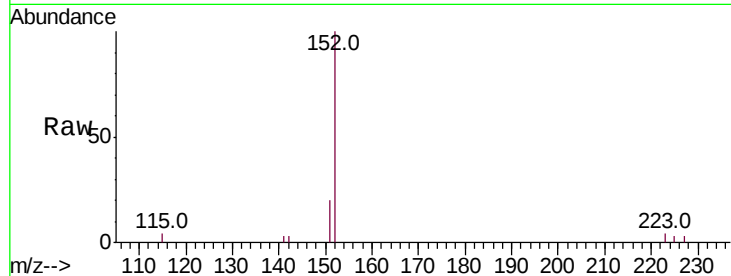

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.15 min Scan# 1305
Delta R.T. -0.00 min
Lab File: BN010980.D
Acq: 19 Jun 2020 21:10

Tgt Ion:164 Resp: 3744
Ion Ratio Lower Upper
164 100
162 102.5 81.0 121.6
160 49.2 38.9 58.3


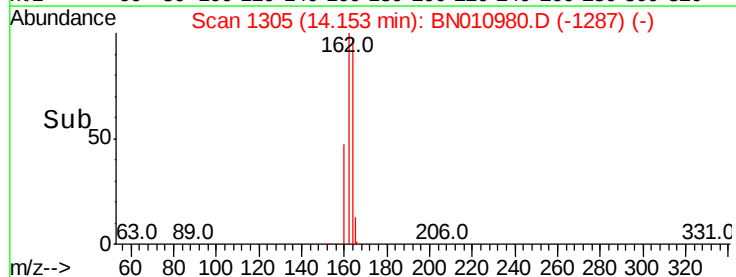
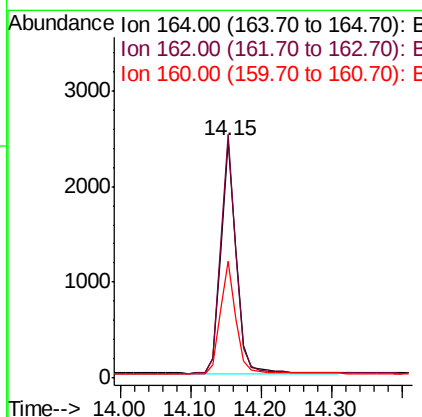
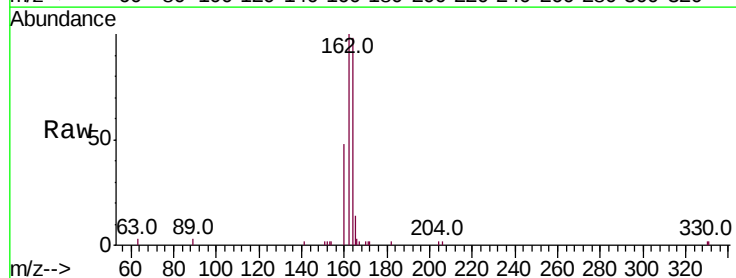


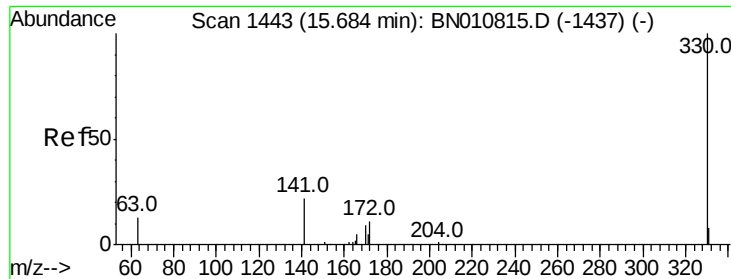

#14
2,4,6-Tribromophenol
Concen: 0.391 ng
RT: 15.66 min Scan# 1440
Delta R.T. 0.01 min
Lab File: BN010980.D
Acq: 19 Jun 2020 21:10




Instrument :
BNA_N
ClientSampleId :
MW202D1-20200613


Tot Ion:330 Resp: 523
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 39.6 33.2 49.8

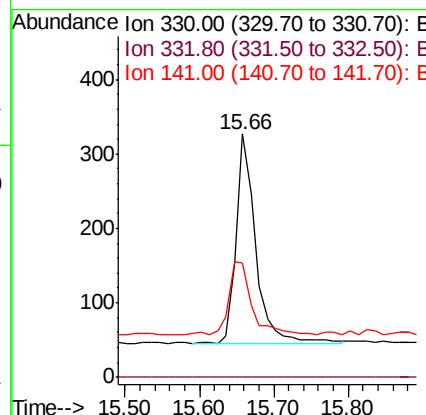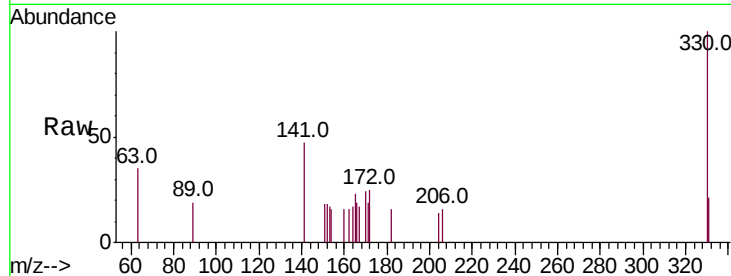

#15
2-Fluorobiphenyl
Concen: 0.395 ng
RT: 12.77 min Scan# 1181
Delta R.T. -0.00 min
Lab File: BN010980.D
Acq: 19 Jun 2020 21:10

Tgt Ion:172 Resp: 5833
Ion Ratio Lower Upper
172 100
171 36.5 28.5 42.7
170 24.6 19.7 29.5

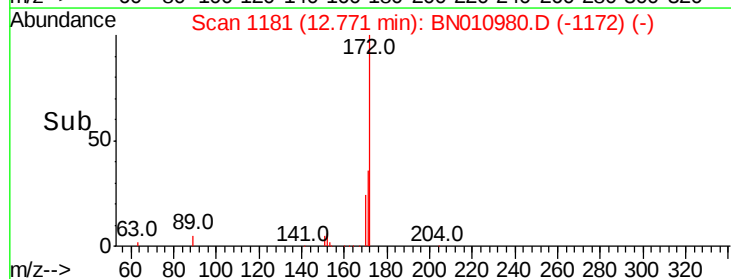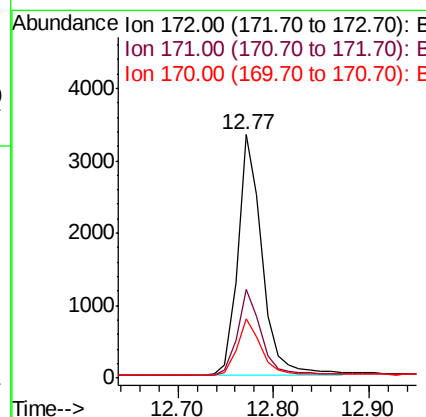



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.91 min Scan# 1556

Delta R.T. 0.01 min

Lab File: BN010980.D

Acq: 19 Jun 2020 21:10

Instrument :

BNA_N

ClientSampleId :

MW202D1-20200613


Tot Ion:188 Resp: 7826

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 8.4 4.5 6.7#

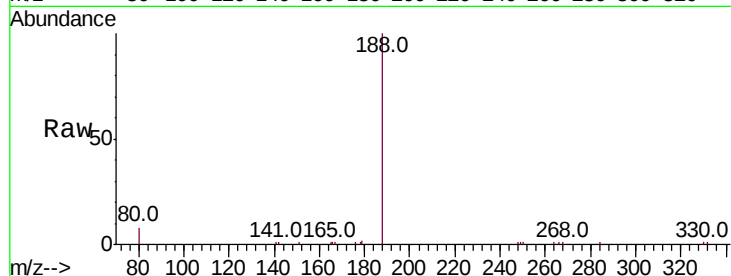

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

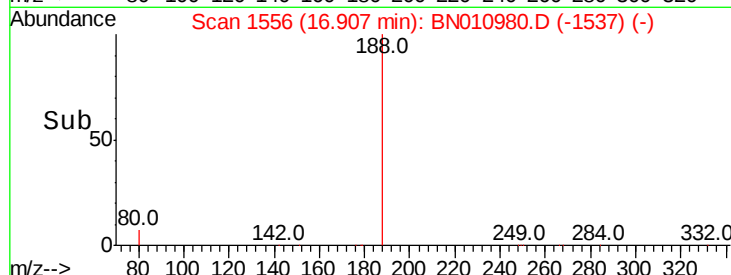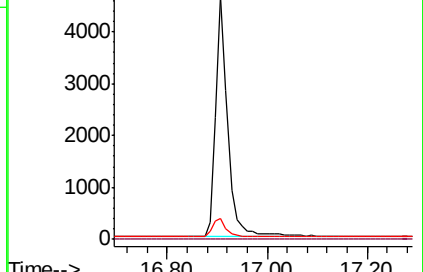

#25

Fluoranthene-d10

Concen: 0.370 ng

RT: 18.95 min Scan# 1848

Delta R.T. 0.00 min

Lab File: BN010980.D

Acq: 19 Jun 2020 21:10


Tgt Ion:212 Resp: 7991

Ion Ratio Lower Upper

212 100

106 9.3 6.6 10.0



104 5.4 4.0 6.0




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

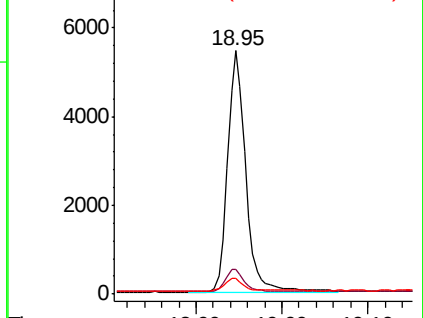



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.11 min Scan# 2166

Delta R.T. -0.01 min

Lab File: BN010980.D

Acq: 19 Jun 2020 21:10

Instrument :

BNA_N

ClientSampleId :

MW202D1-20200613


Tot Ion:240 Resp: 7005

Ion Ratio Lower Upper

240 100

120 12.3 7.5 11.3#




236 28.7 22.3 33.5



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

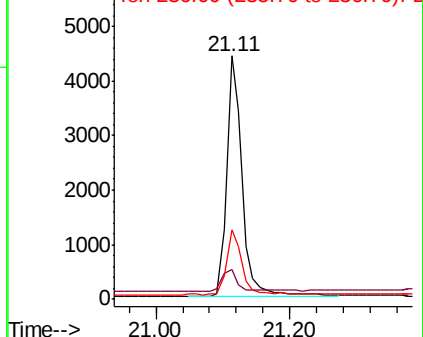

#29

Terphenyl-d14

Concen: 0.534 ng

RT: 19.56 min Scan# 1972

Delta R.T. 0.00 min

Lab File: BN010980.D

Acq: 19 Jun 2020 21:10


Tgt Ion:244 Resp: 8749

Ion Ratio Lower Upper

244 100

212 8.5 7.4 11.2



122 8.8 7.5 11.3




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

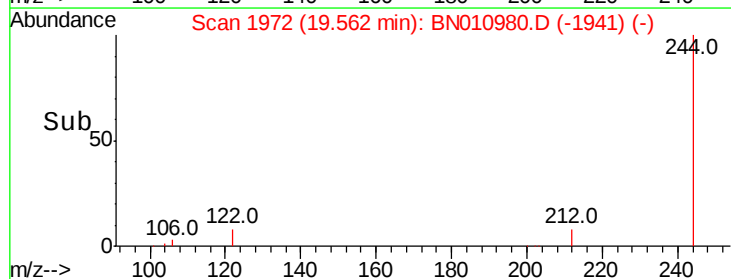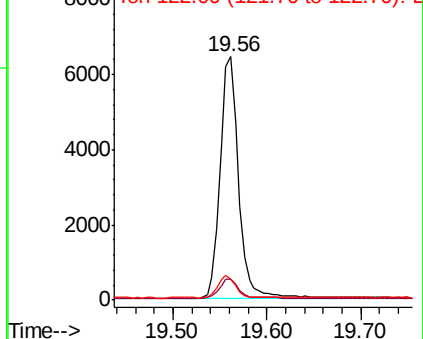






#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.067 ng
 RT: 21.06 min Scan# 2161
 Delta R.T. 0.00 min
 Lab File: BN010980.D
 Acq: 19 Jun 2020 21:10

Instrument :
 BNA_N
 ClientSampleId :
 MW202D1-20200613


Tot Ion:149 Resp: 462
 Ion Ratio Lower Upper
 149 100
 167 25.3 24.1 36.1
 279 7.1 4.6 7.0#

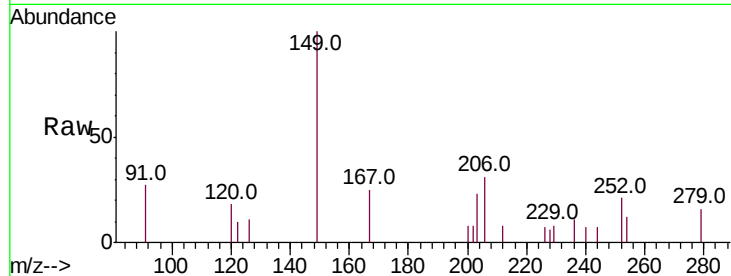

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

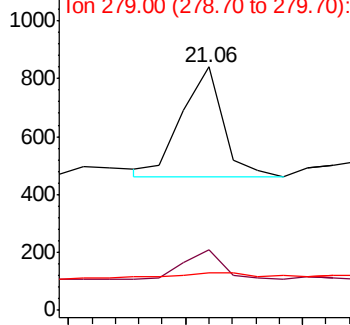


Time--> 21.00 21.05 21.10





#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.26 min Scan# 2537
 Delta R.T. -0.00 min
 Lab File: BN010980.D
 Acq: 19 Jun 2020 21:10

Tgt Ion:264 Resp: 8107
 Ion Ratio Lower Upper
 264 100
 260 24.8 20.4 30.6
 265 84.0 75.0 112.4

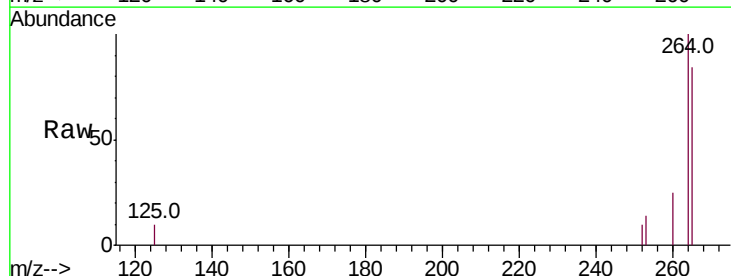

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

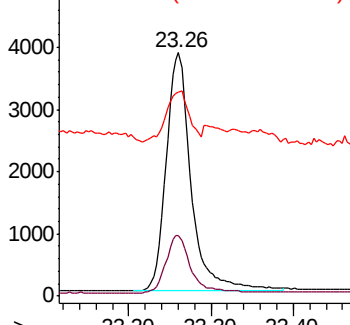

Time--> 23.20 23.30 23.40