

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061920\
 Data File : BN010996.D
 Acq On : 20 Jun 2020 09:11
 Operator : CG/JU
 Sample : L3043-20
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE139D1-20200612

Quant Time: Jun 22 00:30:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 19 12:43:49 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	2173	0.40	ng	0.00
7) Naphthalene-d8	10.28	136	7405	0.40	ng	0.00
13) Acenaphthene-d10	14.15	164	4486	0.40	ng	-0.01
19) Phenanthrene-d10	16.91	188	8909	0.40	ng	0.01
27) Chrysene-d12	21.12	240	8508	0.40	ng	0.00
34) Perylene-d12	23.26	264	9288	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.18	112	826	0.20	ng	0.00
5) Phenol-d6	6.73	99	540	0.11	ng	0.00
8) Nitrobenzene-d5	8.67	82	2448	0.45	ng	0.00
11) 2-Methylnaphthalene-d10	11.88	152	3583	0.31	ng	0.00
14) 2,4,6-Tribromophenol	15.66	330	647	0.40	ng	0.01
15) 2-Fluorobiphenyl	12.78	172	7675	0.43	ng	0.00
25) Fluoranthene-d10	18.94	212	9491	0.39	ng	0.00
29) Terphenyl-d14	19.56	244	11844	0.59	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.21	88	2669	1.254	ng	98
32) Bis(2-ethylhexyl)phthalate	21.06	149	910	0.109	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061920\
Data File : BN010996.D
Acq On : 20 Jun 2020 09:11
Operator : CG/JU
Sample : L3043-20
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE139D1-20200612

Quant Time: Jun 22 00:30:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 19 12:43:49 2020
Response via : Initial Calibration

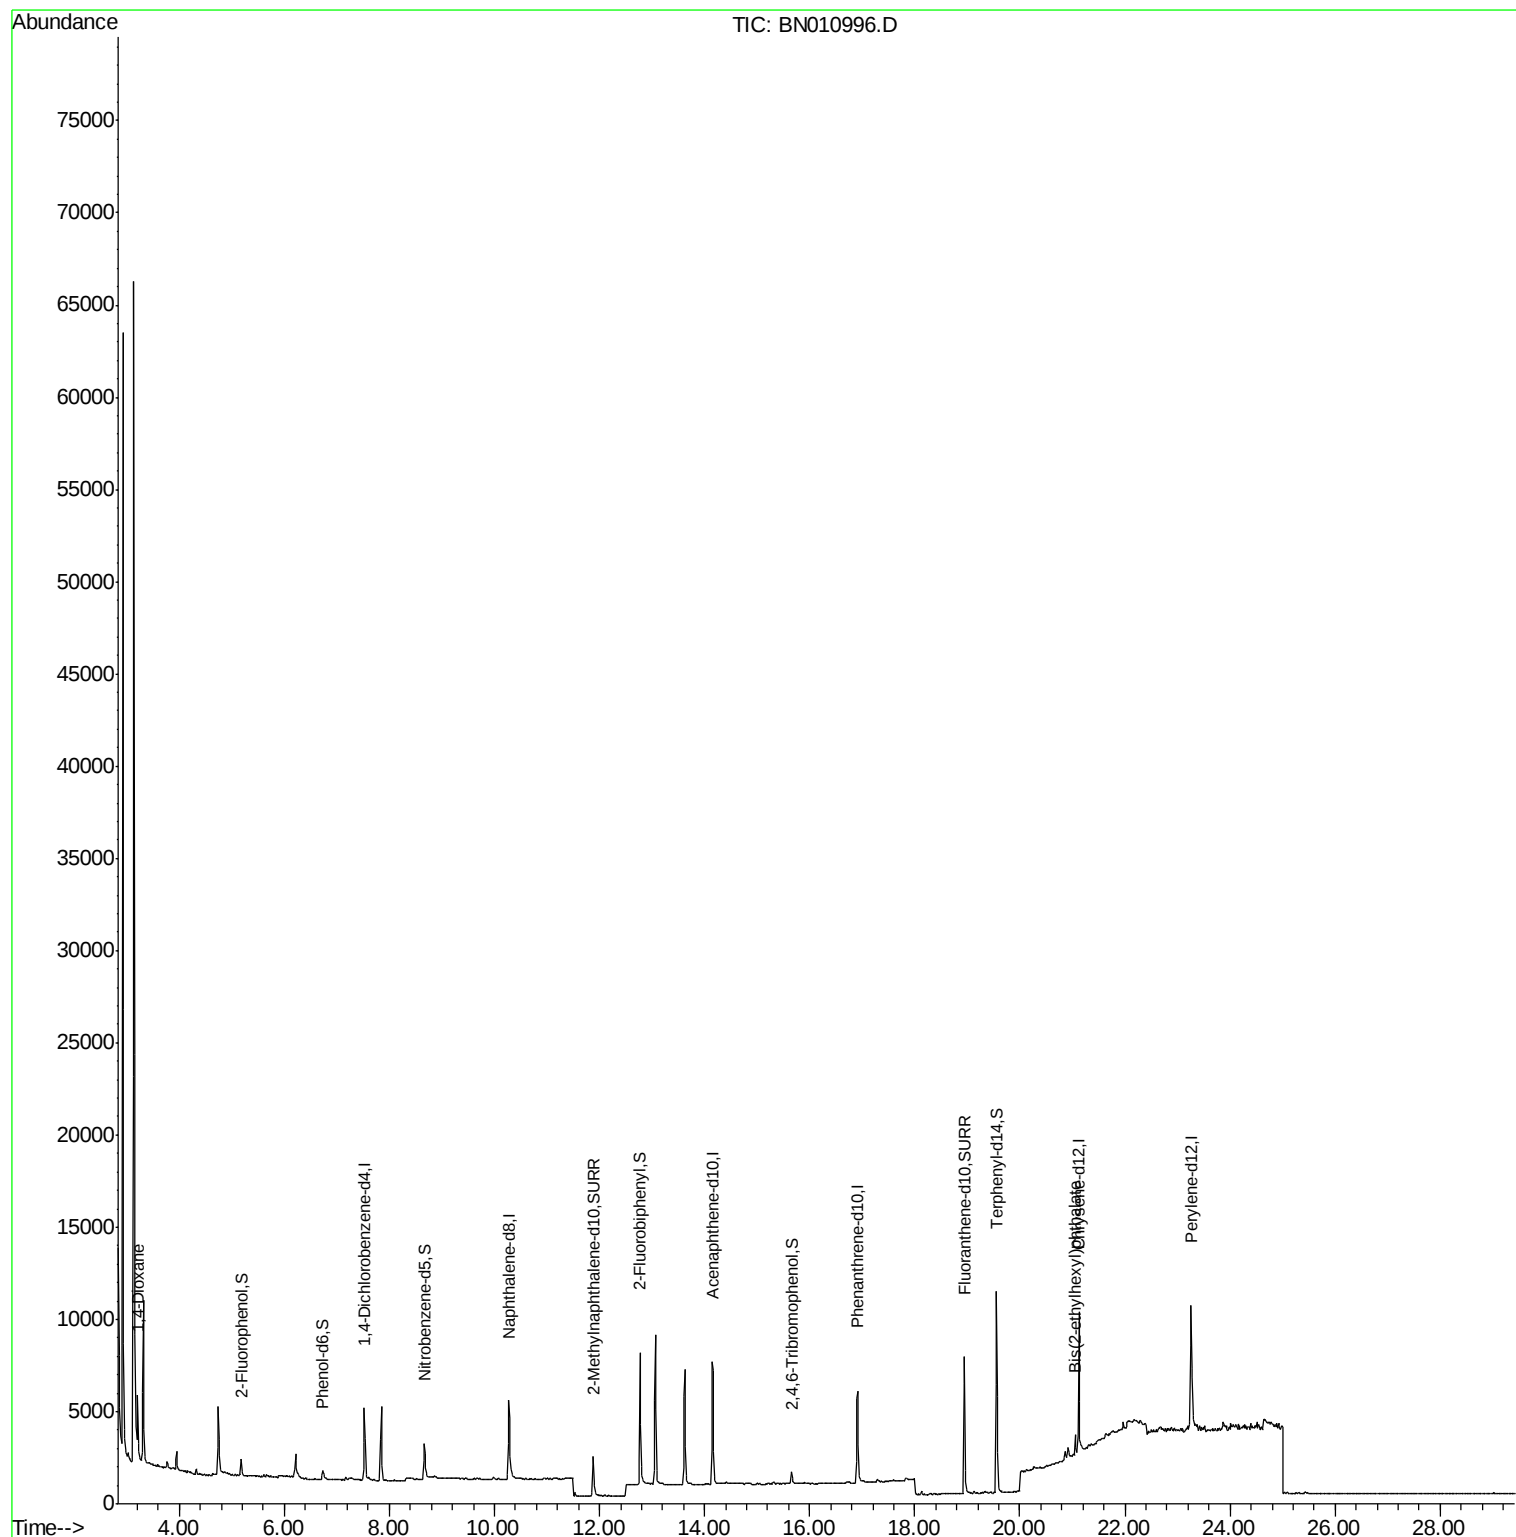

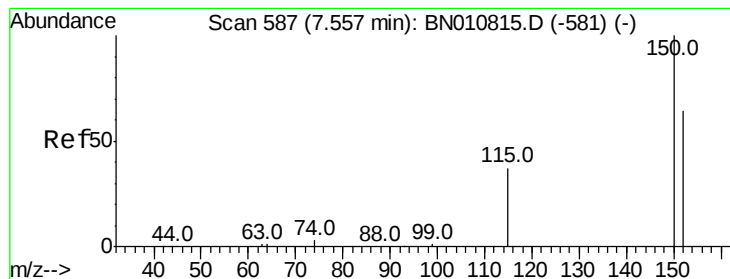


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.53 min Scan# 584
Delta R.T. -0.00 min
Lab File: BN010996.D
Acq: 20 Jun 2020 09:11

Instrument :
BNA_N
ClientSampleId :
RE139D1-20200612

Tot Ion:152 Resp: 2173
Ion Ratio Lower Upper
152 100
150 148.7 123.8 185.6
115 60.3 49.2 73.8

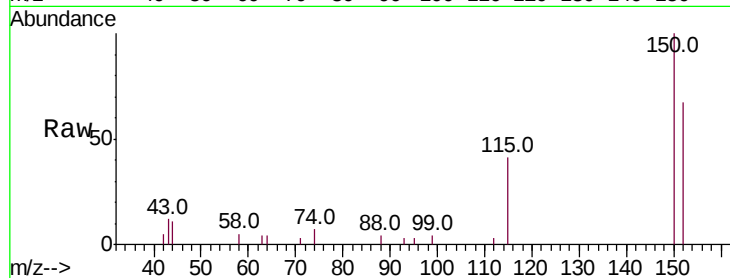


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

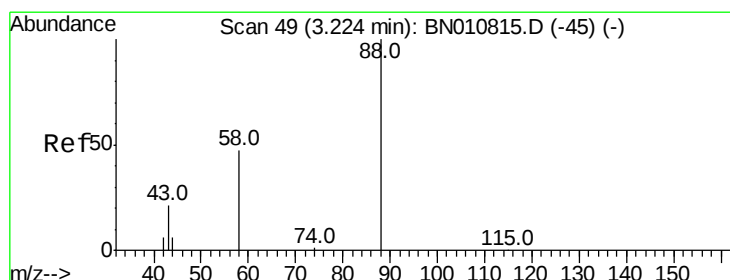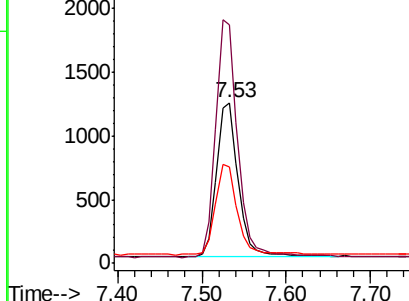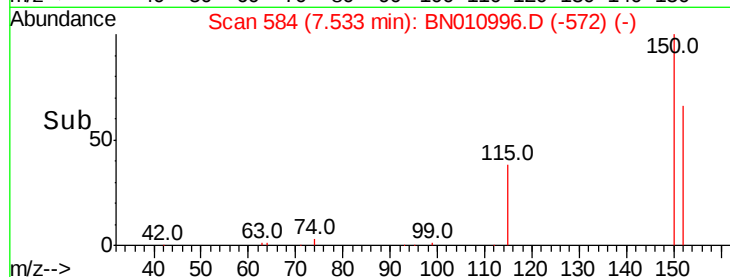



#2


1,4-Dioxane
Concen: 1.254 ng
RT: 3.21 min Scan# 47
Delta R.T. -0.01 min
Lab File: BN010996.D
Acq: 20 Jun 2020 09:11

Tgt Ion: 88 Resp: 2669
Ion Ratio Lower Upper
88 100
58 47.6 38.2 57.4
43 22.4 15.1 22.7

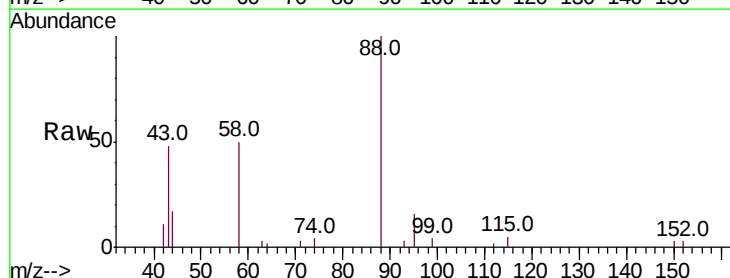

Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC

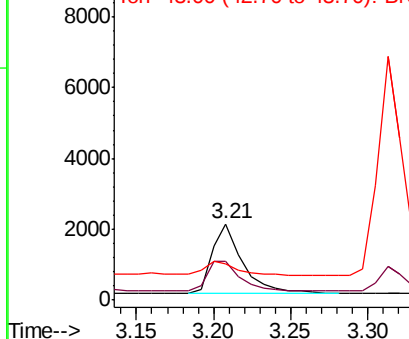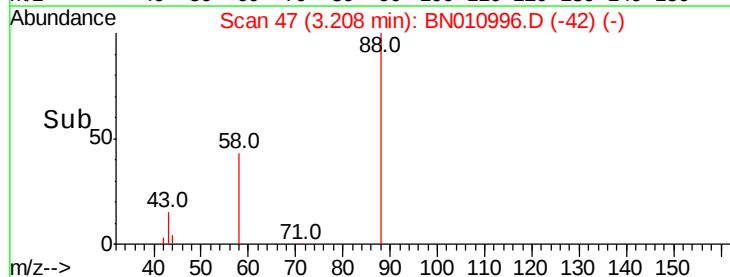

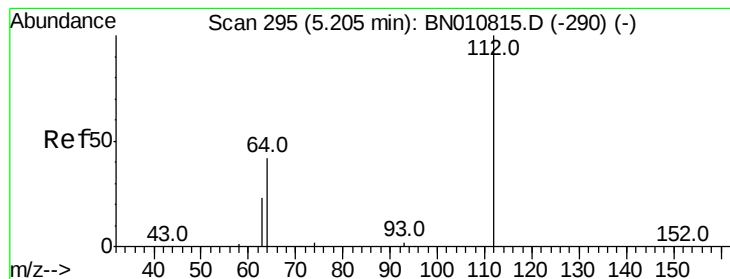

#4

2-Fluorophenol

Concen: 0.197 ng

RT: 5.18 min Scan# 292

Delta R.T. -0.00 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11

Instrument :

BNA_N

ClientSampleId :

RE139D1-20200612


Tot Ion:112 Resp: 826

Ion Ratio Lower Upper

112 100

64 46.7 37.4 56.0




63 26.5 22.2 33.4

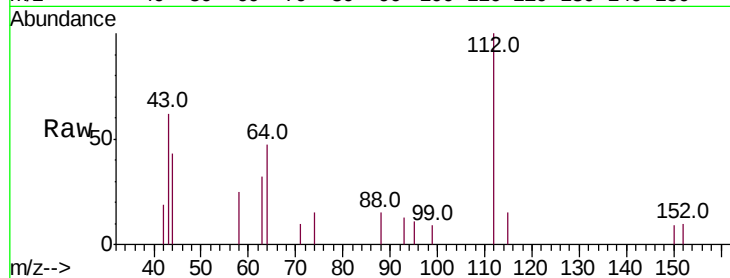

Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): B

Ion 63.00 (62.70 to 63.70): B

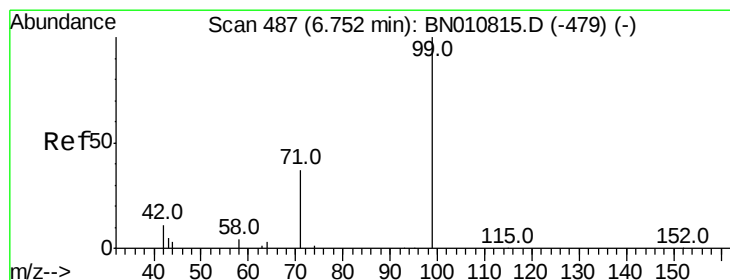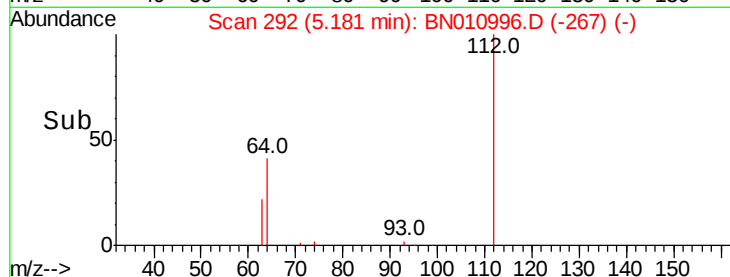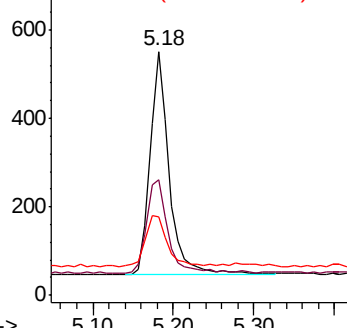

#5

Phenol-d6

Concen: 0.109 ng

RT: 6.73 min Scan# 484

Delta R.T. -0.00 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11


Tgt Ion: 99 Resp: 540

Ion Ratio Lower Upper

99 100

42 17.8 11.1 16.7#



71 37.4 31.4 47.2

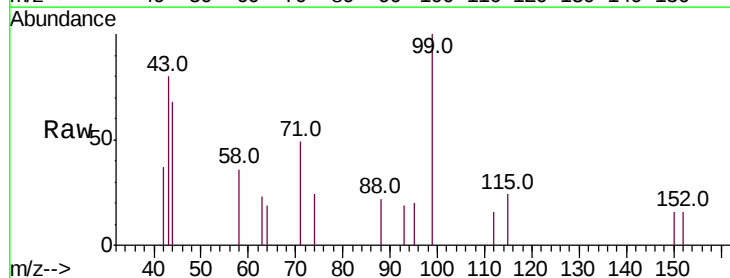


Abundance Ion 99.00 (98.70 to 99.70): B

Ion 42.00 (41.70 to 42.70): B

Ion 71.00 (70.70 to 71.70): B

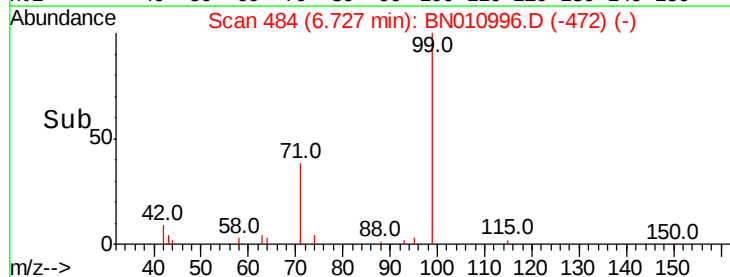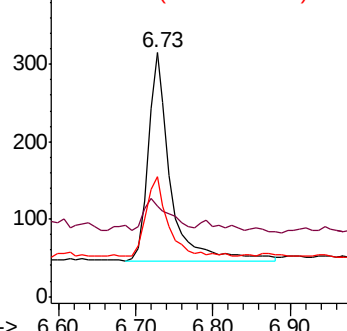



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.28 min Scan# 836

Delta R.T. -0.00 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11

Instrument :

BNA_N

ClientSampleId :

RE139D1-20200612

Tot Ion:136 Resp: 7405


Ion Ratio Lower Upper

136 100

137 12.3 9.7 14.5

54 5.7 4.9 7.3

68 6.3 4.7 7.1



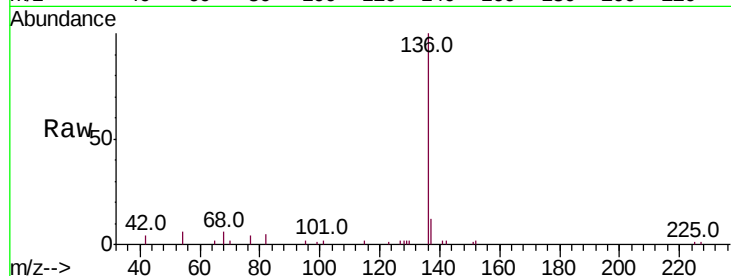


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

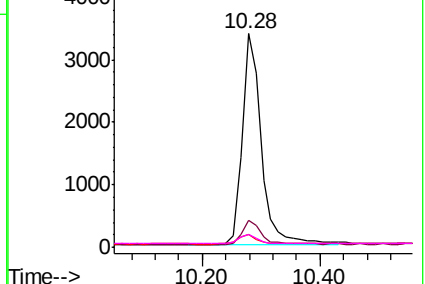

#8

Nitrobenzene-d5

Concen: 0.447 ng

RT: 8.67 min Scan# 709

Delta R.T. -0.00 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11


Tgt Ion: 82 Resp: 2448

Ion Ratio Lower Upper

82 100

128 44.4 35.4 53.0



54 34.8 28.2 42.4




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC

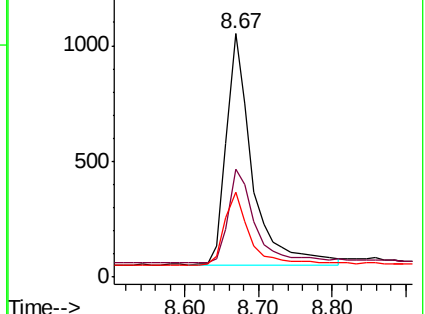



#11

2-Methylnaphthalene-d10

Concen: 0.312 ng

RT: 11.88 min Scan# 1016

Delta R.T. -0.00 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11

Instrument :

BNA_N

ClientSampleId :


RE139D1-20200612

Tot Ion:152 Resp: 3583

Ion Ratio Lower Upper

152 100

151 23.2 15.3 22.9#

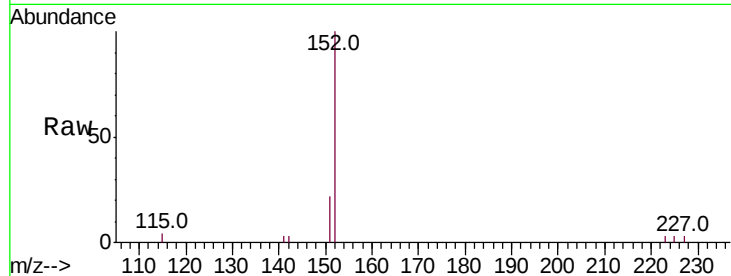

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

11.88

1500



1000

500

0

11.80 11.90 12.00

Time-->

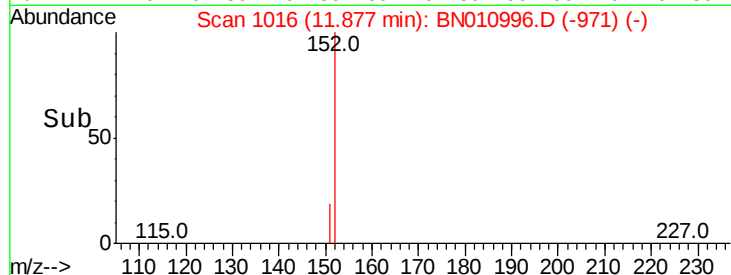

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.15 min Scan# 1305

Delta R.T. -0.01 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11


Tgt Ion:164 Resp: 4486

Ion Ratio Lower Upper

164 100

162 105.6 81.0 121.6

160 50.1 38.9 58.3

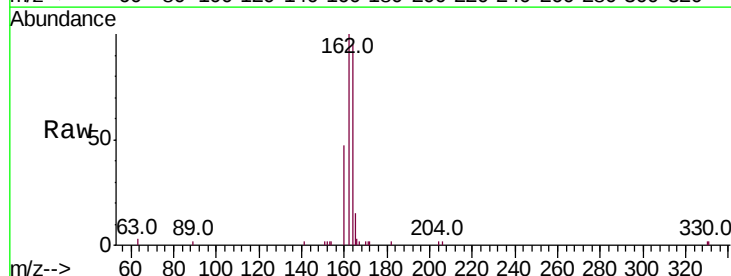

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

14.15

3000


2000


1000

0

14.00 14.20

Time-->









#14
 2,4,6-Tribromophenol
 Concen: 0.403 ng
 RT: 15.66 min Scan# 1441
 Delta R.T. 0.01 min
 Lab File: BN010996.D
 Acq: 20 Jun 2020 09:11




Instrument :
 BNA_N
 ClientSampleId :
 RE139D1-20200612


Tot Ion:330 Resp: 647
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 41.4 33.2 49.8

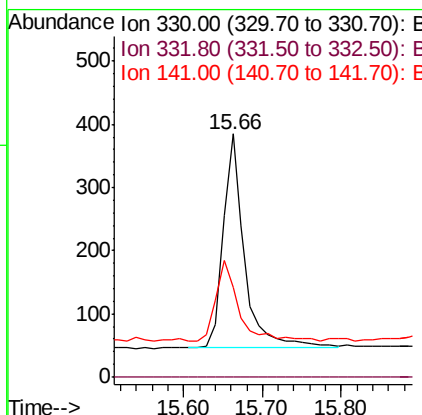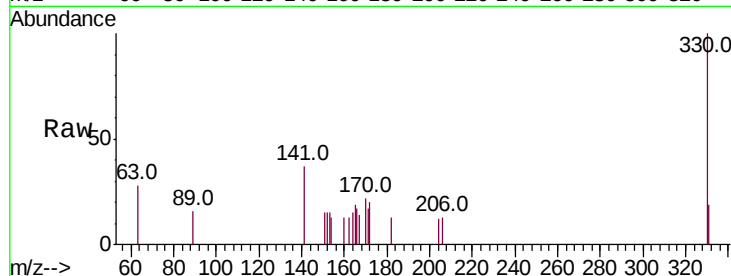

#15
 2-Fluorobiphenyl
 Concen: 0.434 ng
 RT: 12.78 min Scan# 1182
 Delta R.T. -0.00 min
 Lab File: BN010996.D
 Acq: 20 Jun 2020 09:11

Tgt Ion:172 Resp: 7675
 Ion Ratio Lower Upper
 172 100
 171 35.3 28.5 42.7
 170 22.9 19.7 29.5

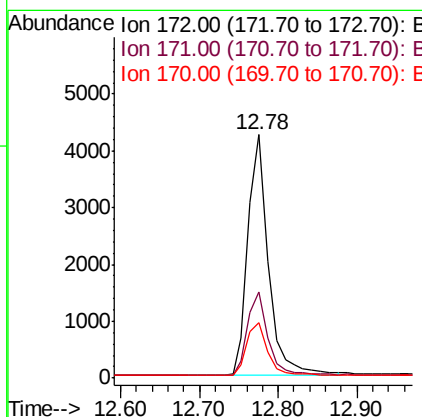

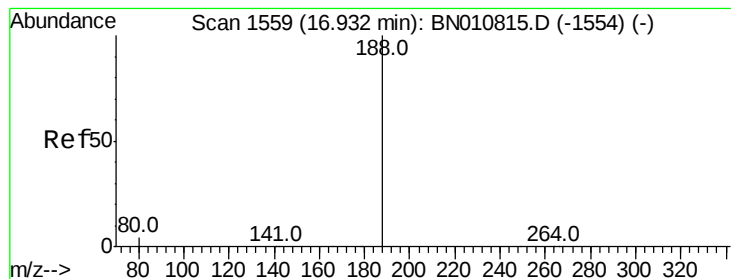

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.91 min Scan# 1557

Delta R.T. 0.01 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11

Instrument :

BNA_N

ClientSampleId :

RE139D1-20200612


Tot Ion:188 Resp: 8909

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 7.2 4.5 6.7#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

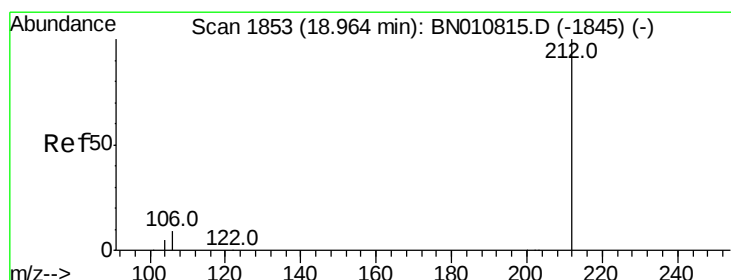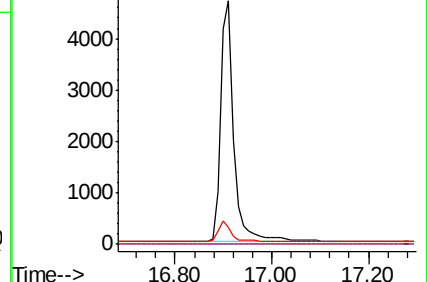

#25

Fluoranthene-d10

Concen: 0.386 ng

RT: 18.94 min Scan# 1849

Delta R.T. -0.00 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11


Tgt Ion:212 Resp: 9491

Ion Ratio Lower Upper

212 100

106 9.6 6.6 10.0



104 5.5 4.0 6.0




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

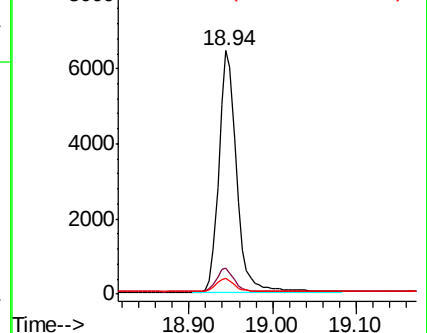



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.12 min Scan# 2168

Delta R.T. -0.00 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11

Instrument :

BNA_N

ClientSampleId :

RE139D1-20200612


Tot Ion:240 Resp: 8508

Ion Ratio Lower Upper

240 100

120 8.1 7.5 11.3




236 27.9 22.3 33.5



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

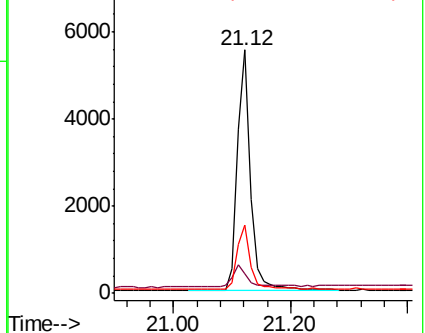

#29

Terphenyl-d14

Concen: 0.595 ng

RT: 19.56 min Scan# 1973

Delta R.T. -0.00 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11


Tgt Ion:244 Resp: 11844

Ion Ratio Lower Upper

244 100

212 8.6 7.4 11.2



122 9.4 7.5 11.3




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

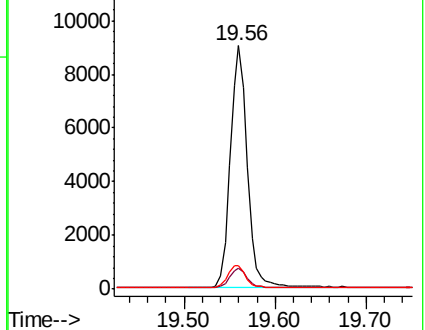



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.109 ng

RT: 21.06 min Scan# 2162

Delta R.T. -0.00 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11

Instrument :

BNA_N

ClientSampleId :

RE139D1-20200612


Tot Ion:149 Resp: 910

Ion Ratio Lower Upper

149 100

167 27.0 24.1 36.1




279 8.0 4.6 7.0#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

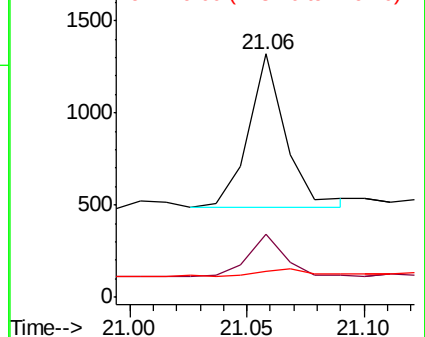

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.26 min Scan# 2539

Delta R.T. -0.00 min

Lab File: BN010996.D

Acq: 20 Jun 2020 09:11


Tgt Ion:264 Resp: 9288

Ion Ratio Lower Upper

264 100

260 24.2 20.4 30.6

265 77.4 75.0 112.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

