


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061920\
 Data File : BN010963.D
 Acq On : 19 Jun 2020 11:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 12:43:49 2020

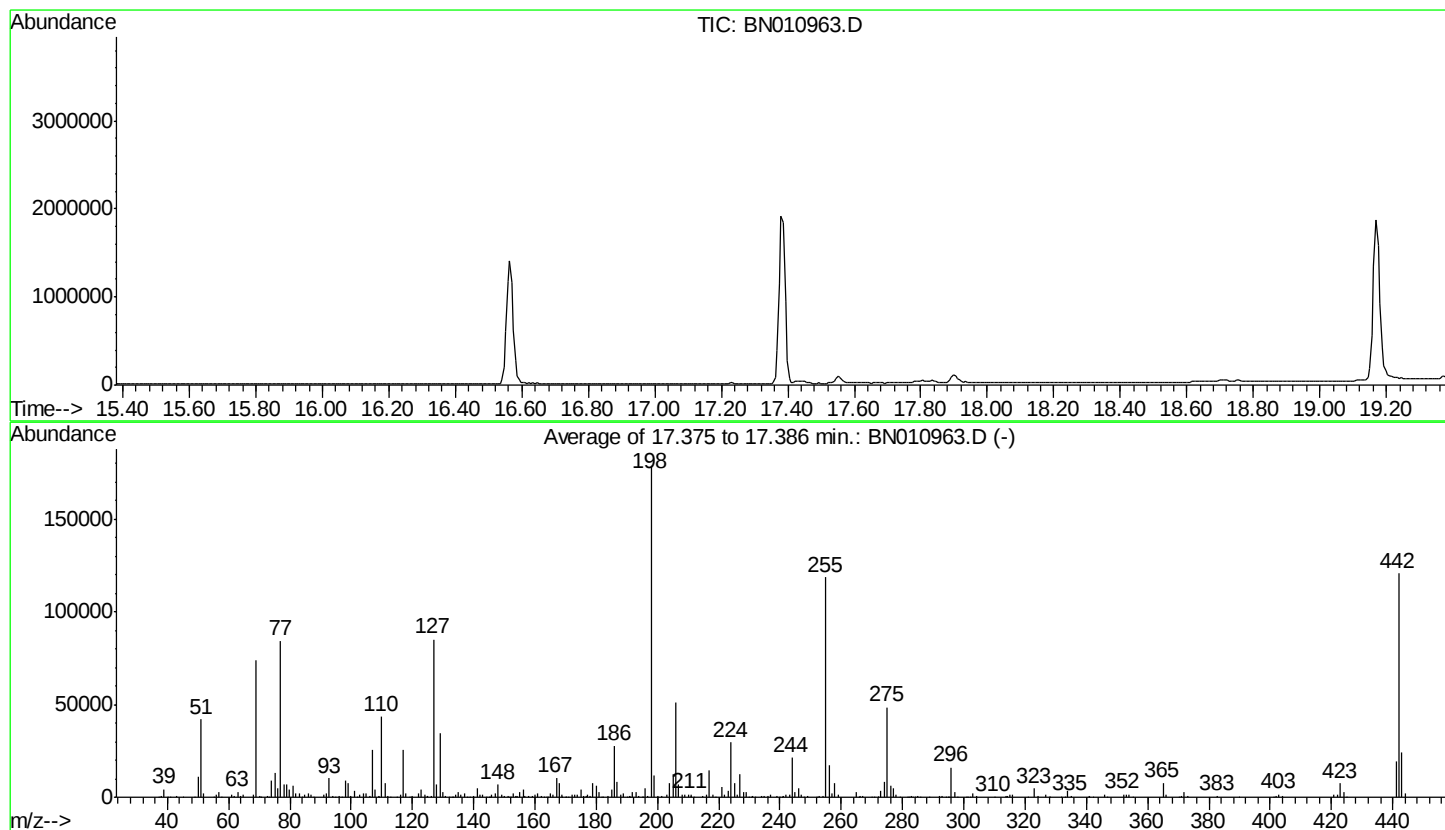

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	41920	PASS
68	69	0.00	2	1.8	1339	PASS
69	198	0.00	100	41.1	73522	PASS
70	69	0.00	2	0.7	546	PASS
127	198	10	80	47.5	84949	PASS
197	198	0.00	2	0.5	836	PASS
198	198	100	100	100.0	178773	PASS
199	198	5	9	6.6	11865	PASS
275	198	10	60	27.0	48338	PASS
365	198	1	100	4.3	7625	PASS
441	198	0.01	100	10.9	19450	PASS
442	198	50	100	67.5	120757	PASS
443	442	15	24	19.8	23876	PASS