
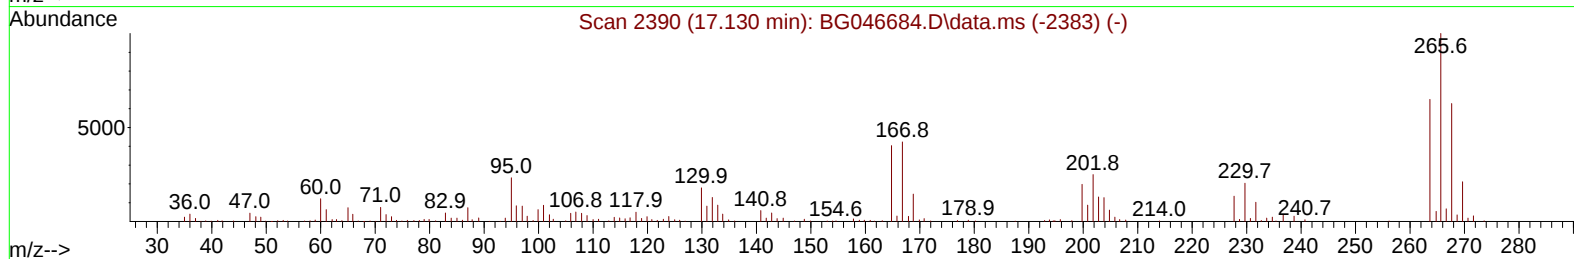
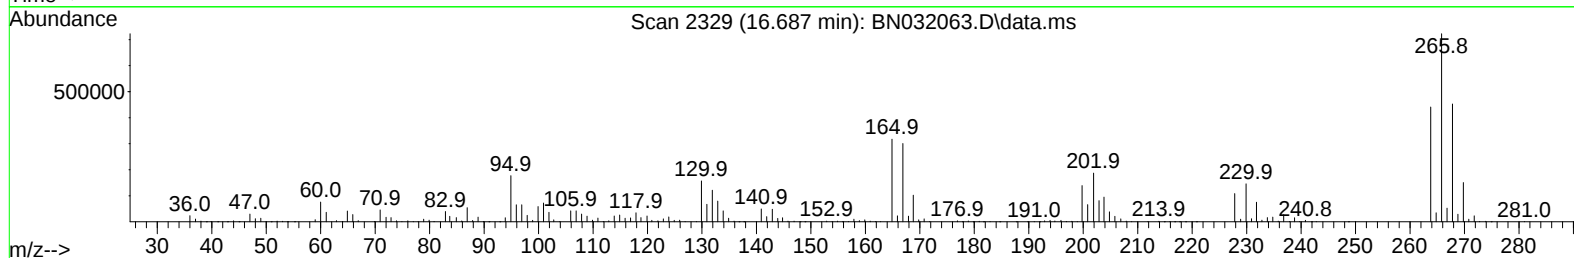


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061924\
Data File : BN032063.D
Acq On : 19 Jun 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 12:06:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

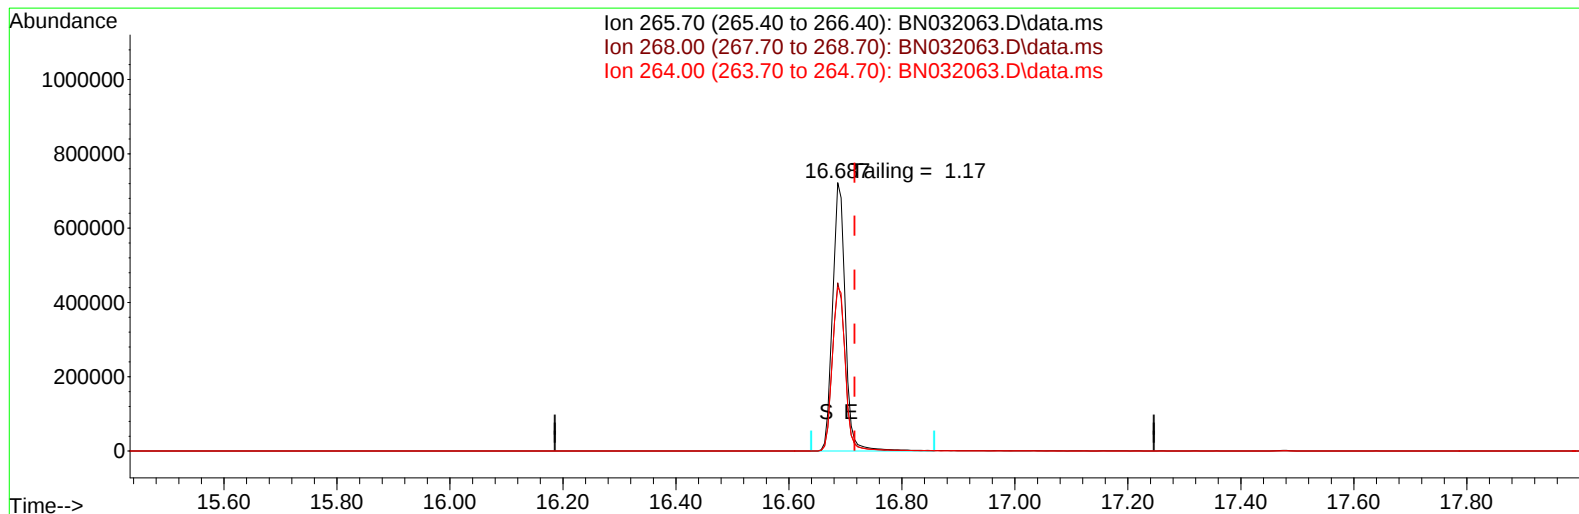

TIC: BN032063.D\data.ms

(70) Pentachlorophenol (C)




16.687min (-0.029) 27688.06 ng

response 1131858

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.67
264.00	61.60	61.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061924\
Data File : BN032063.D
Acq On : 19 Jun 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 12:06:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

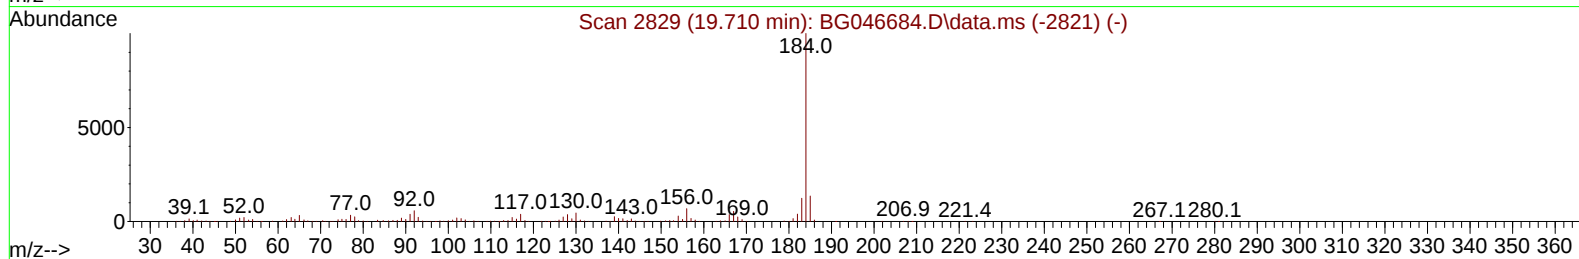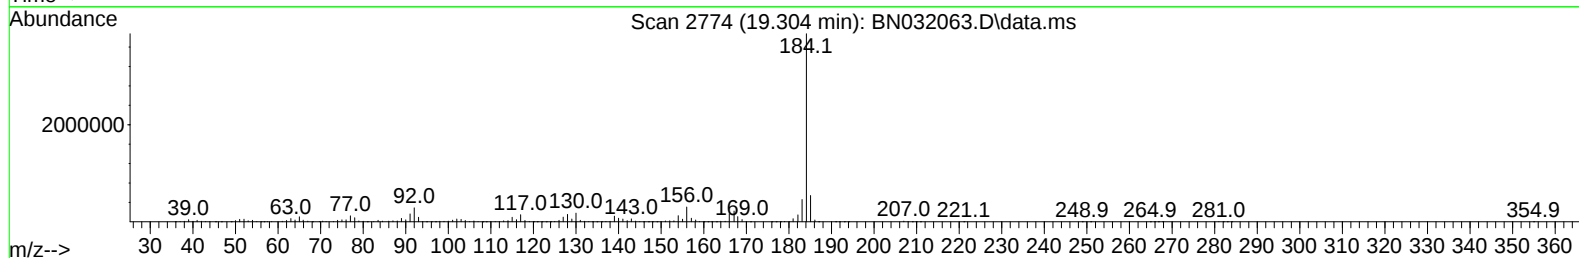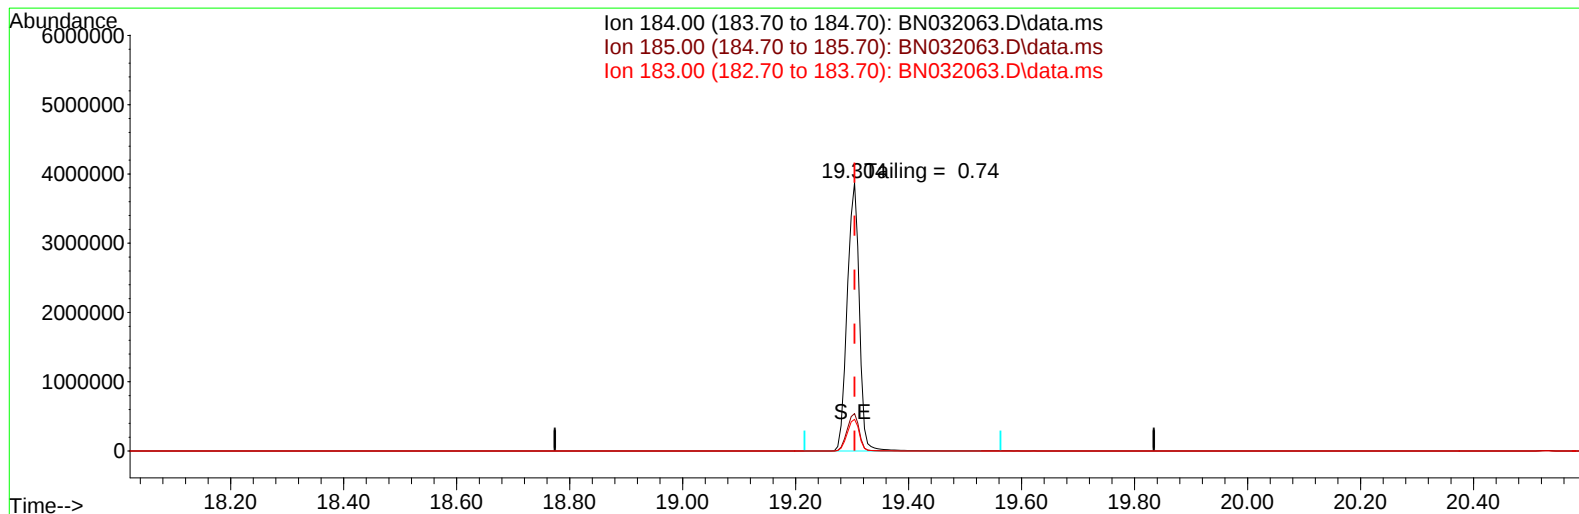

TIC: BN032063.D\data.ms

(77) Benzidine

19.304min (-0.000) 0.00 ng

response 5773859

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.85
0.00	0.00	0.00