
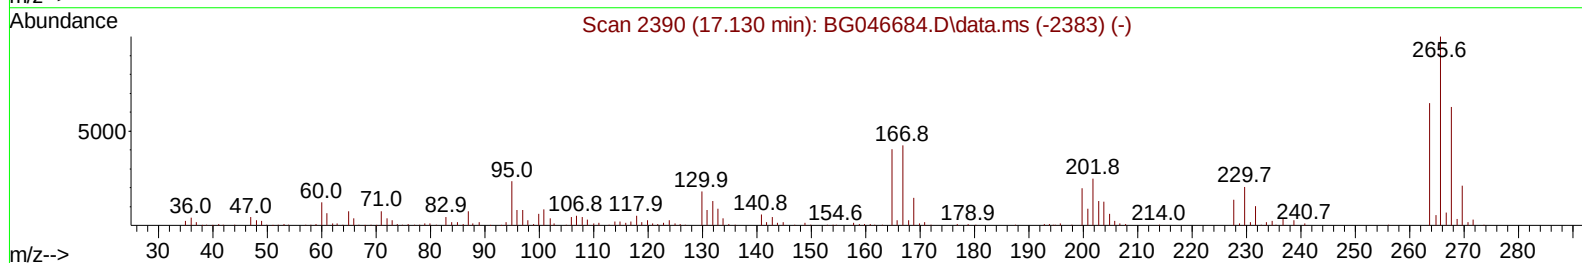
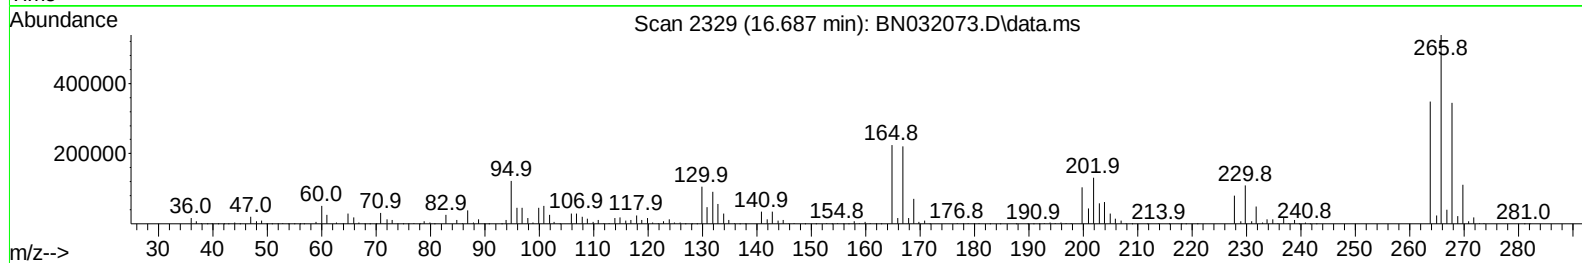


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061924\
Data File : BN032073.D
Acq On : 19 Jun 2024 18:10
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jun 20 01:44:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration



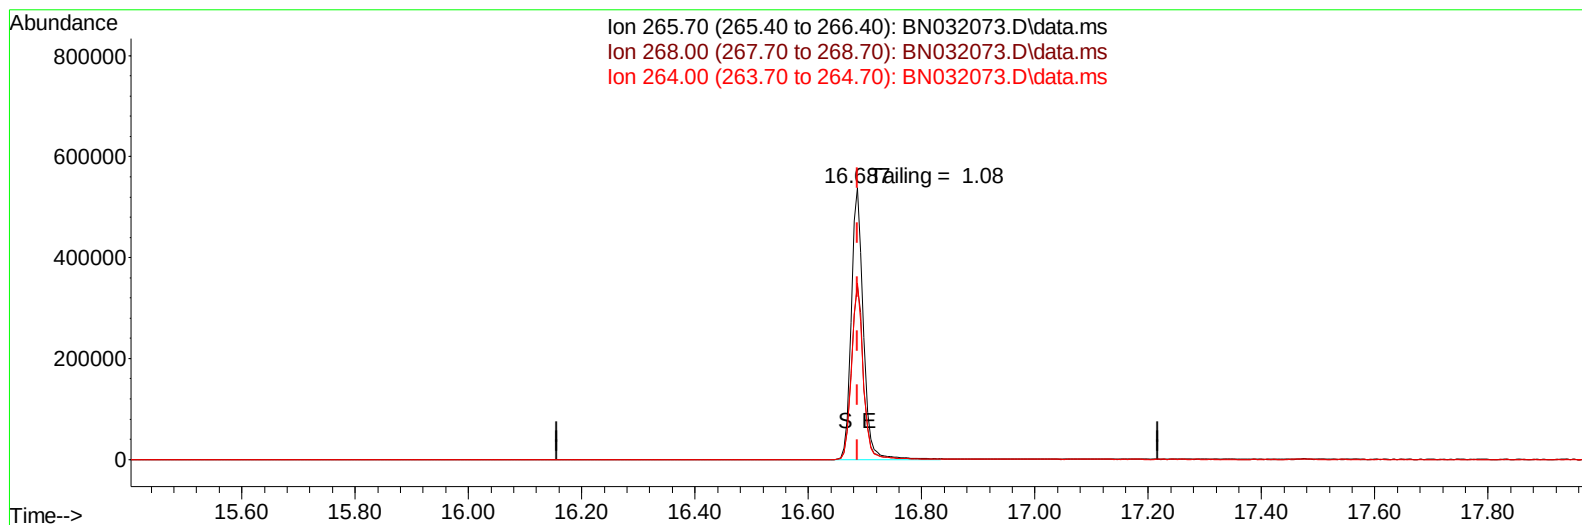


TIC: BN032073.D\data.ms

(70) Pentachlorophenol (C)**16.687min (0.000) 25078.64 ng****response 800233**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.11
264.00	61.60	64.89
0.00	0.00	0.00

Quant Time: Jun 20 01:44:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

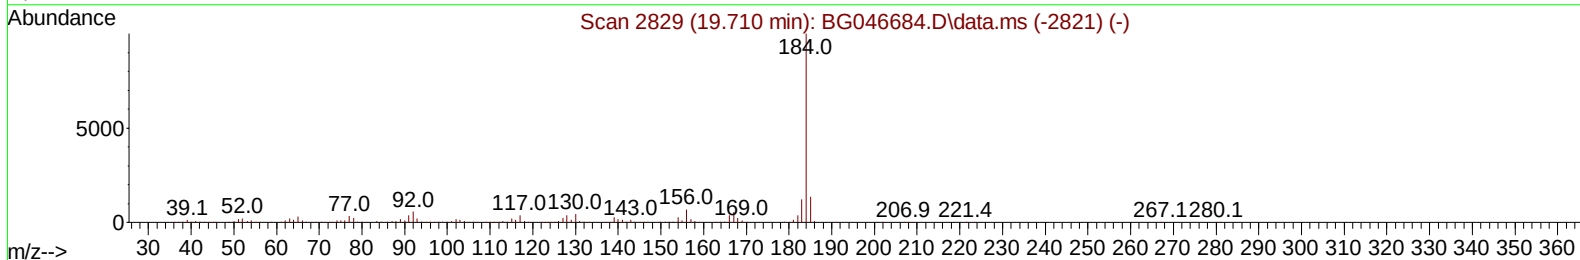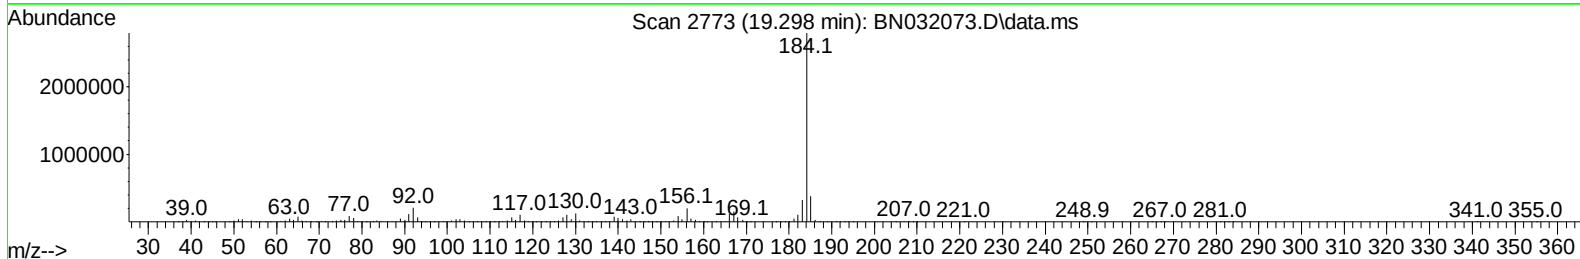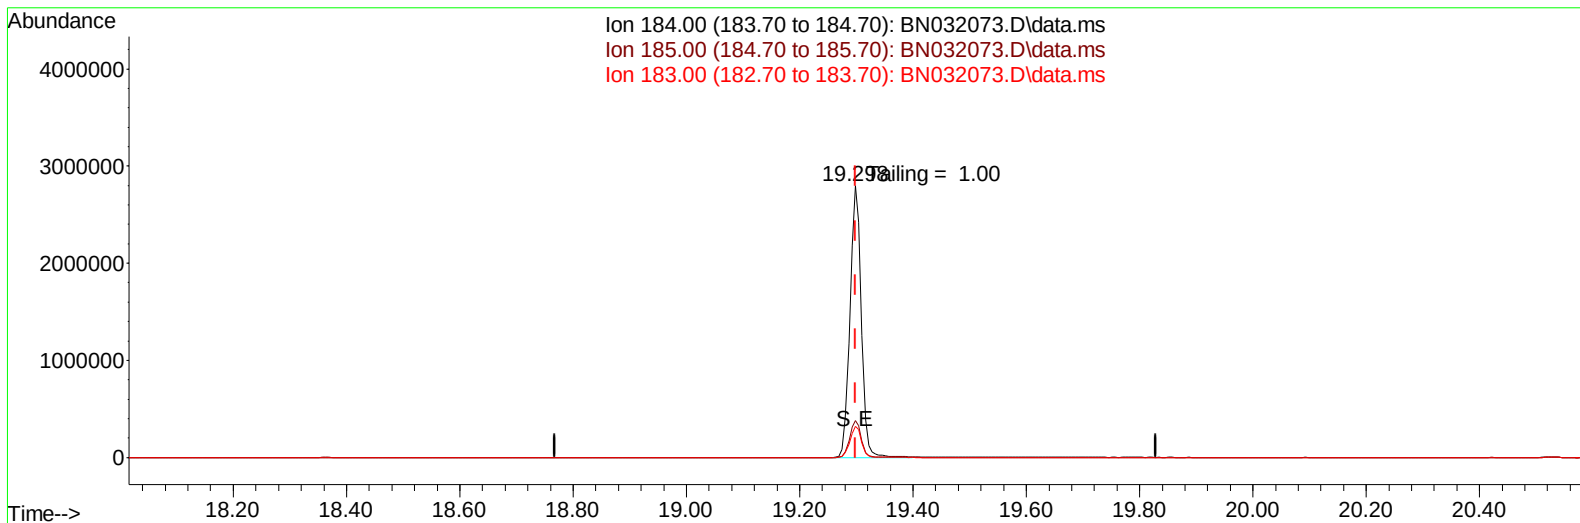

TIC: BN032073.D\data.ms

(77) Benzidine

19.298min (0.000) 0.00 ng

response **3921366**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.48
183.00	13.20	11.49
0.00	0.00	0.00