
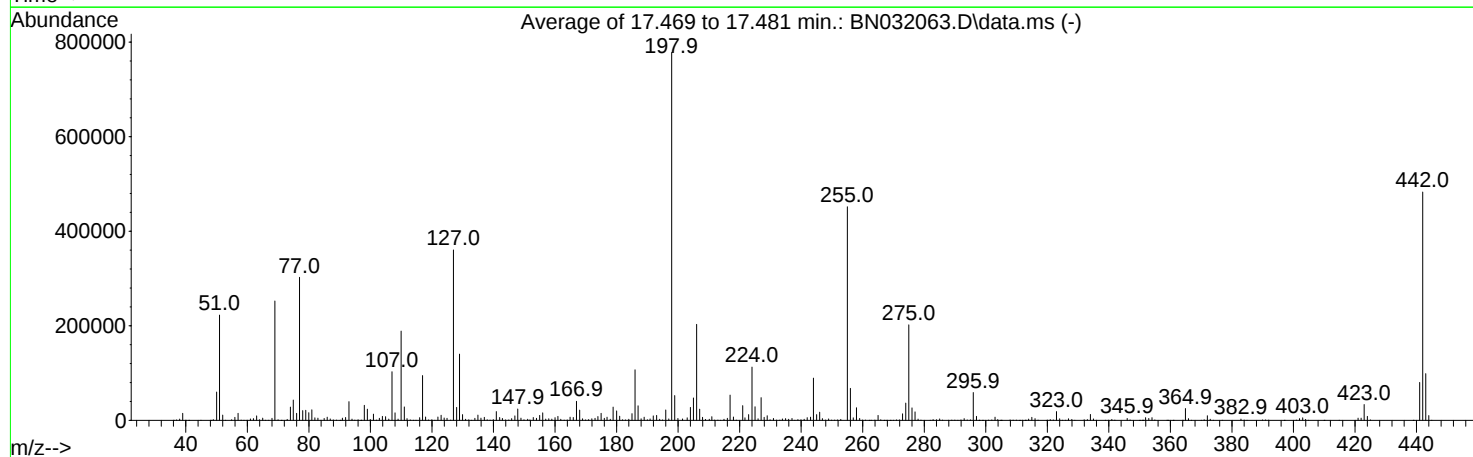


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061924\
Data File : BN032063.D
Acq On : 19 Jun 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 19 11:30:34 2024

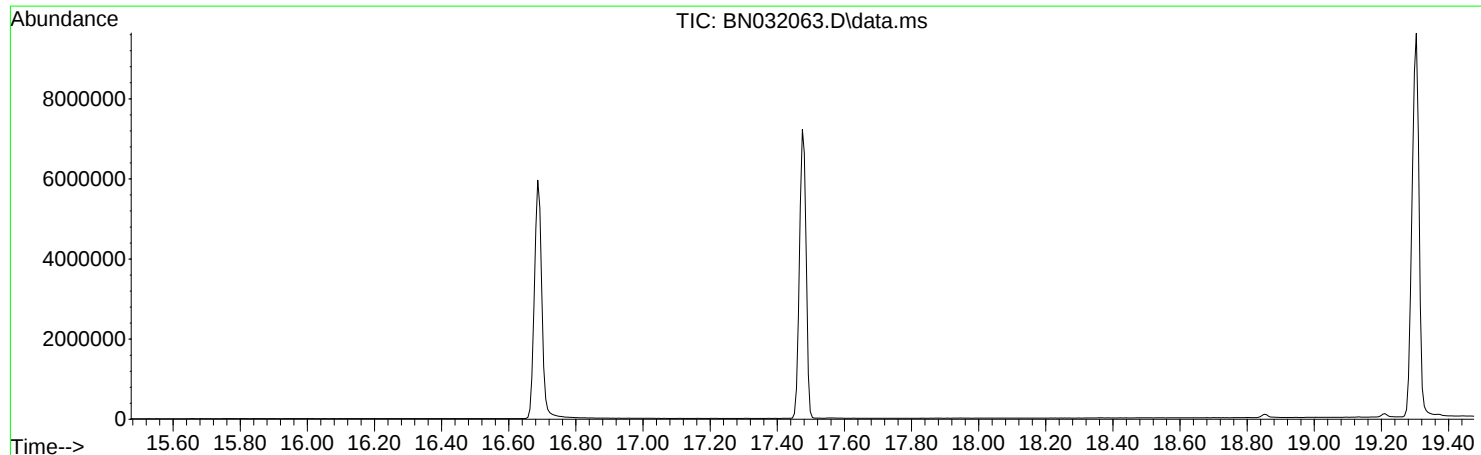

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	222871	PASS
68	69	0.00	2	1.7	4325	PASS
69	198	0.00	100	32.4	252437	PASS
70	69	0.00	2	0.5	1276	PASS
127	198	10	80	46.3	360448	PASS
197	198	0.00	2	0.4	3105	PASS
198	198	100	100	100.0	778048	PASS
199	198	5	9	6.7	52384	PASS
275	198	10	60	26.0	202133	PASS
365	198	1	100	3.2	25176	PASS
441	198	0.01	100	10.3	80240	PASS
442	442	50	100	100.0	483072	PASS
443	442	15	24	20.5	98811	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/19/2024	BNA_N	<u>BN032063.D</u>
Compound Name	Response	Retention Time
DDT	2396038	20.528
DDD	295160	20.086
DDE	3225	19.581
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
298385	2694423	11.07

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061924\
Data File : BN032063.D
Acq On : 19 Jun 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 19 12:06:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

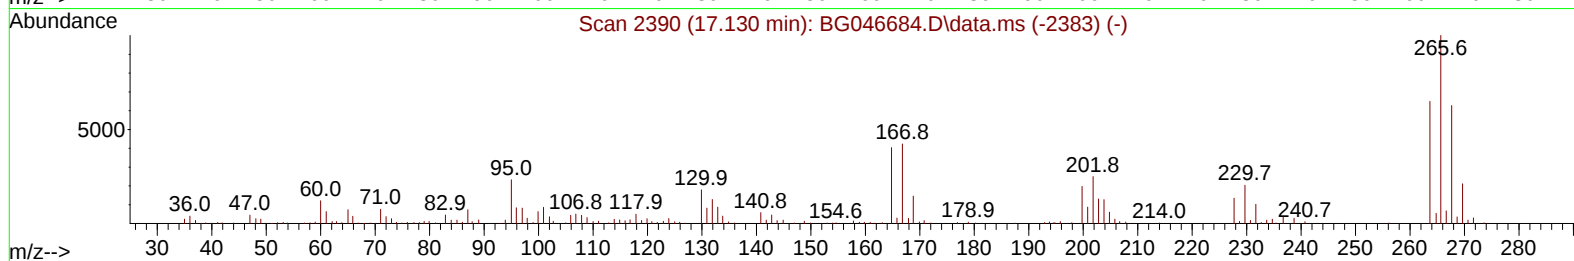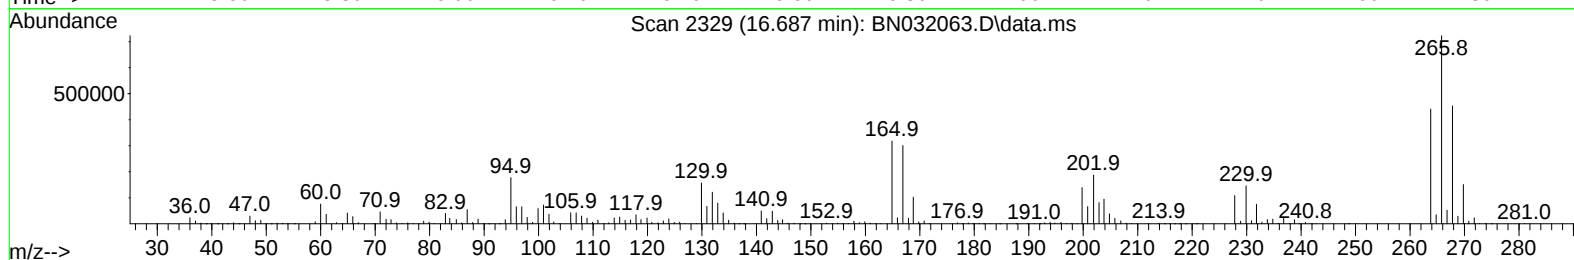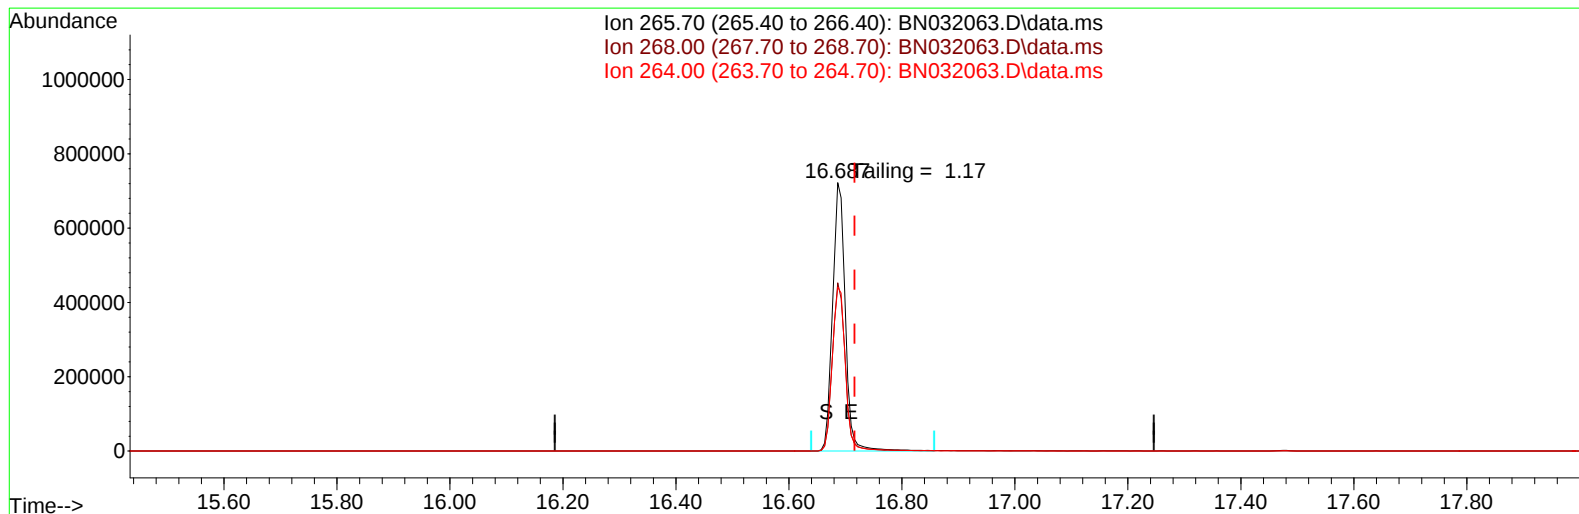

TIC: BN032063.D\data.ms

(70) Pentachlorophenol (C)

16.687min (-0.029) 27688.06 ng




response 1131858

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.67
264.00	61.60	61.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061924\
Data File : BN032063.D
Acq On : 19 Jun 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 19 12:06:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 11 01:48:18 2024
Response via : Initial Calibration

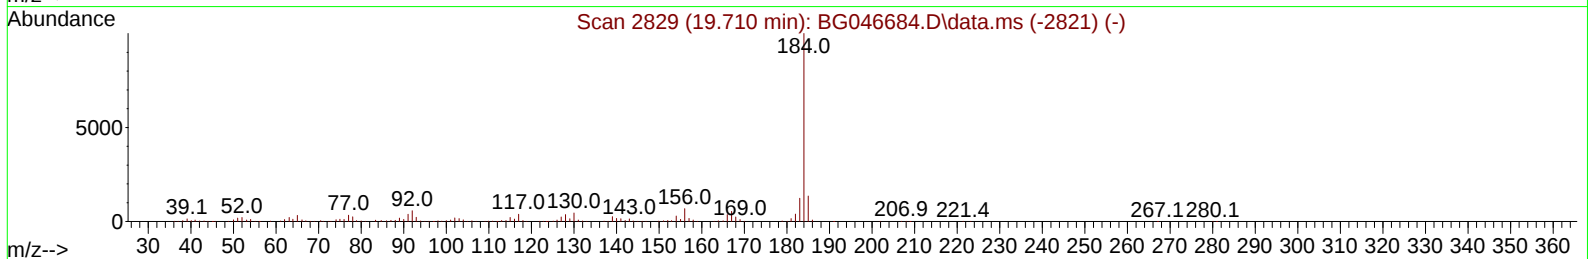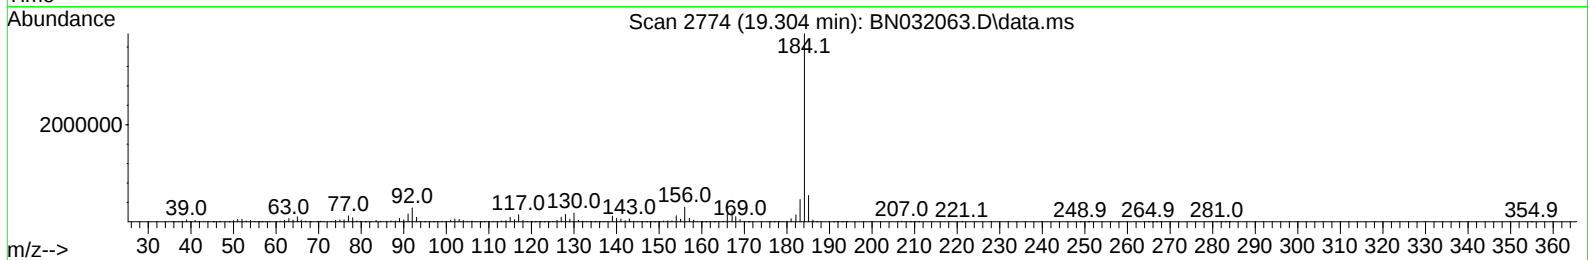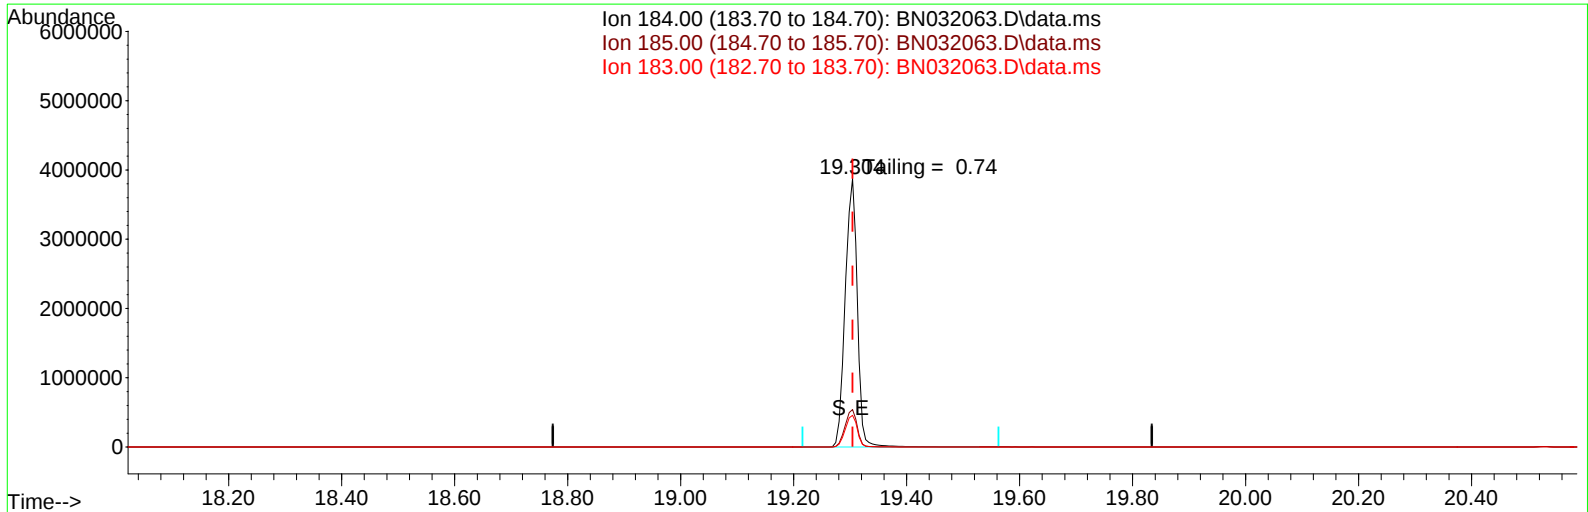

TIC: BN032063.D\data.ms

(77) Benzidine

19.304min (-0.000) 0.00 ng

response 5773859

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.85
0.00	0.00	0.00