
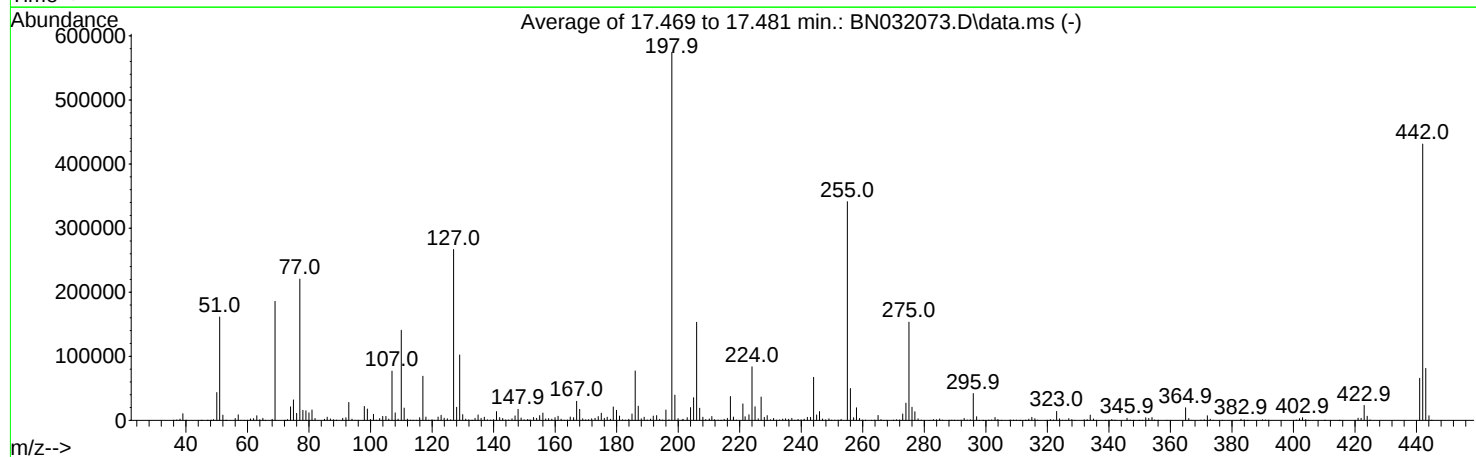


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061924\
Data File : BN032073.D
Acq On : 19 Jun 2024 18:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 19 11:30:34 2024

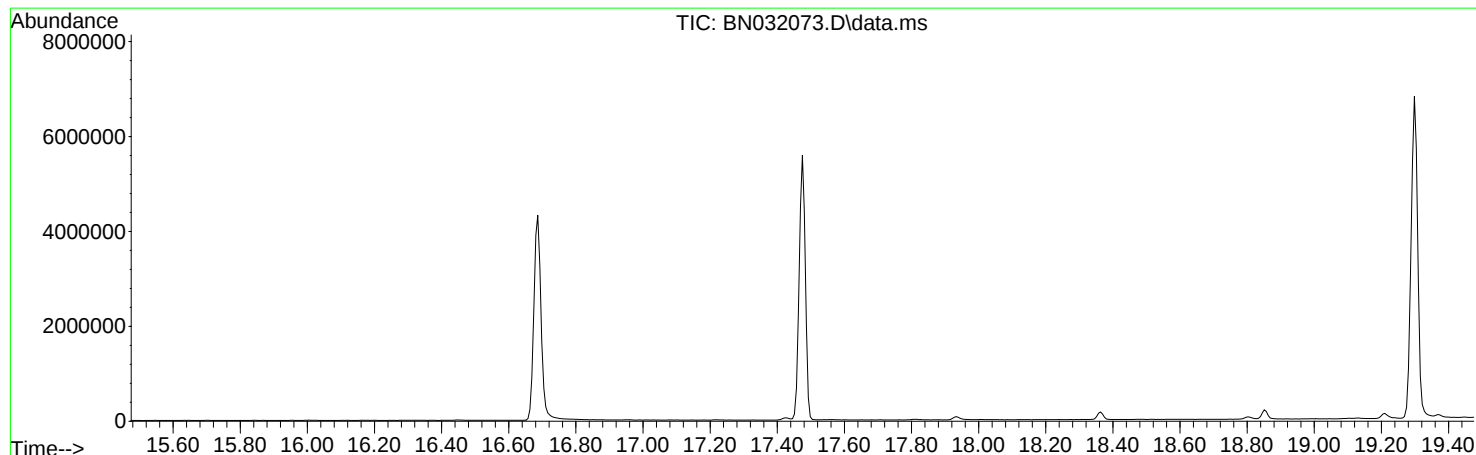

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	161466	PASS
68	69	0.00	2	1.0	1874	PASS
69	198	0.00	100	32.3	185692	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	266773	PASS
197	198	0.00	2	0.2	940	PASS
198	198	100	100	100.0	574101	PASS
199	198	5	9	6.9	39379	PASS
275	198	10	60	26.7	153429	PASS
365	198	1	100	3.5	19868	PASS
441	198	0.01	100	11.4	65669	PASS
442	442	50	100	100.0	431296	PASS
443	442	15	24	18.8	81259	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/19/2024	BNA_N	<u>BN032073.D</u>
Compound Name	Response	Retention Time
DDT	1840382	20.528
DDD	135802	20.086
DDE	1969	19.575
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
137771	1978153	6.96

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061924\
Data File : BN032073.D
Acq On : 19 Jun 2024 18:10
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTTP

Quant Time: Jun 20 01:44:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

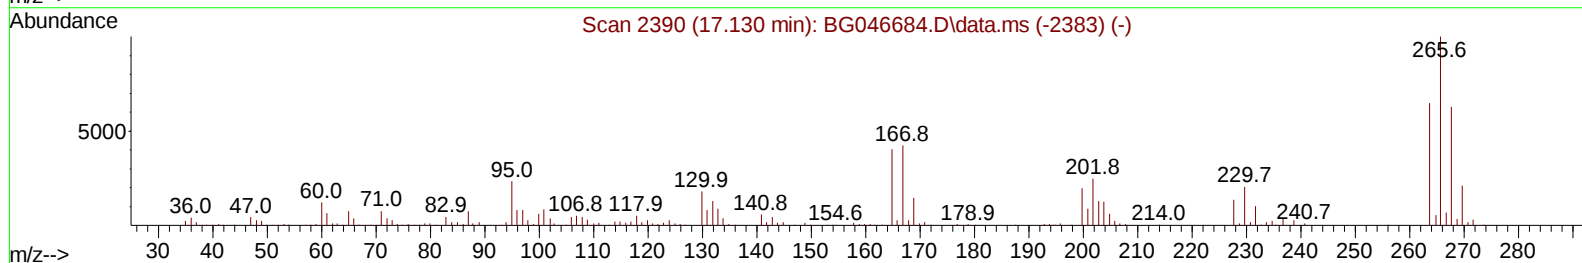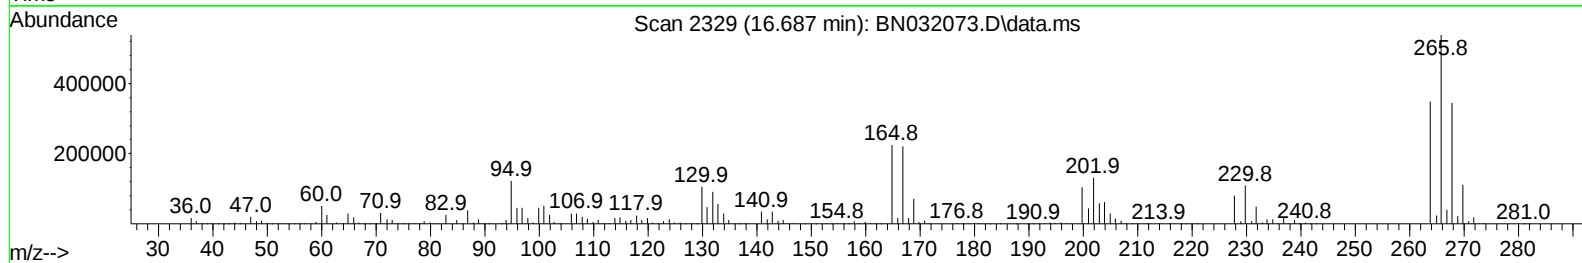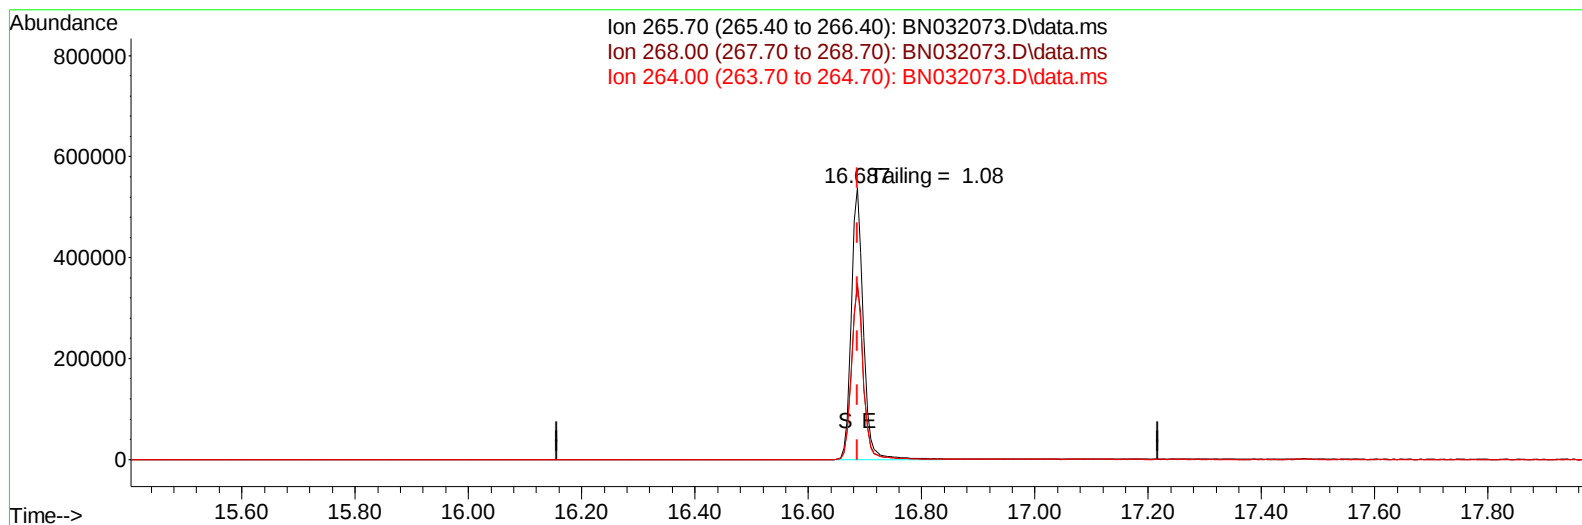

TIC: BN032073.D\data.ms

(70) Pentachlorophenol (C)

16.687min (0.000) 25078.64 ng




response 800233

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.11
264.00	61.60	64.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061924\
Data File : BN032073.D
Acq On : 19 Jun 2024 18:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 20 01:44:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

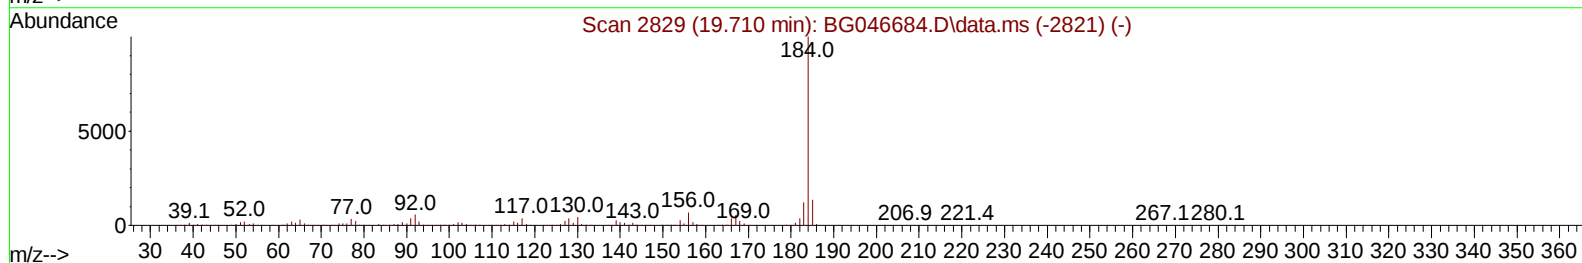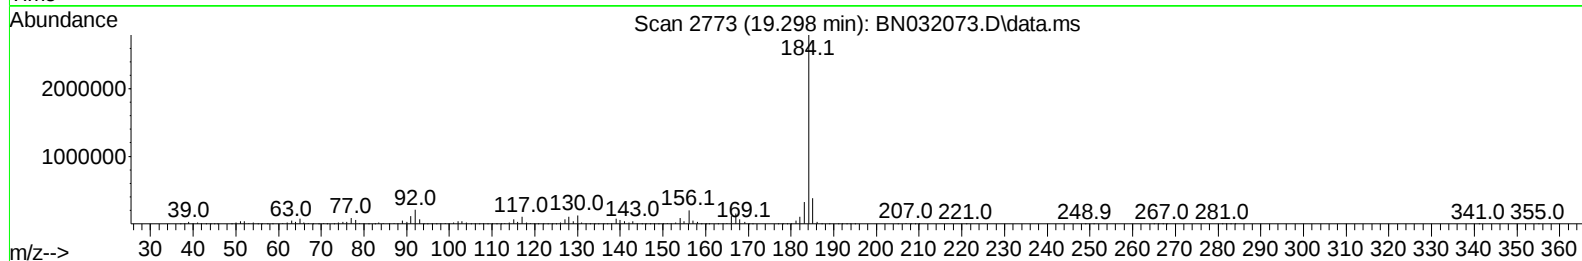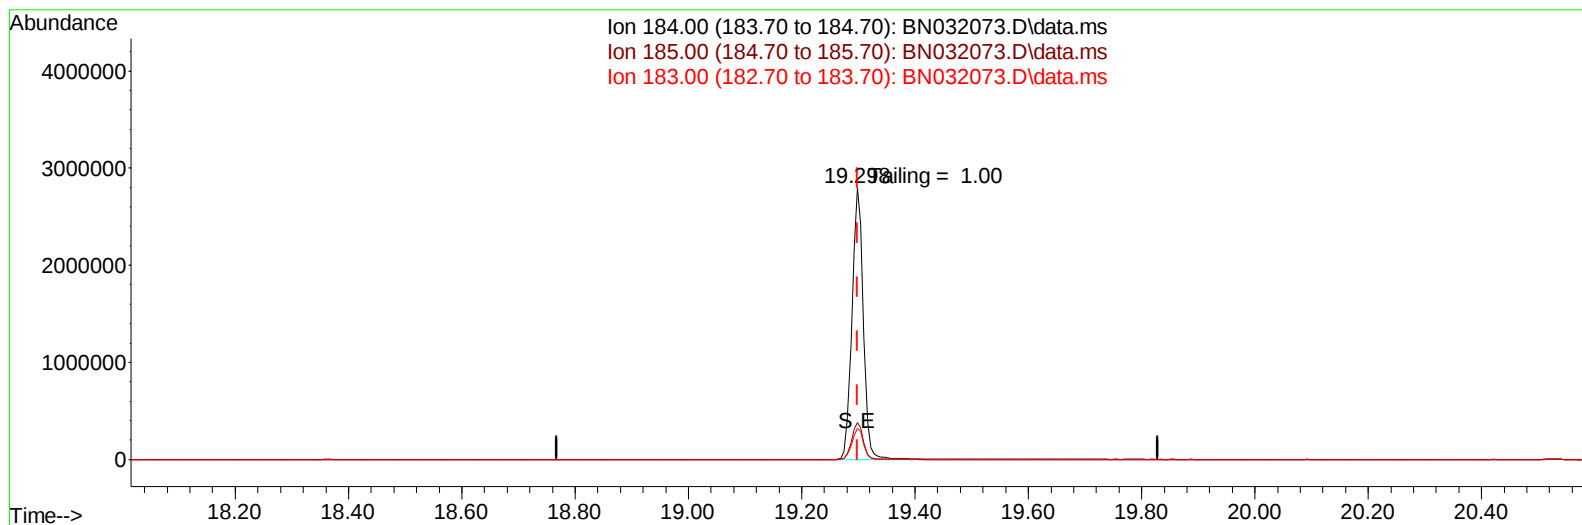

TIC: BN032073.D\data.ms

(77) Benzidine

19.298min (0.000) 0.00 ng

response 3921366

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.48
183.00	13.20	11.49
0.00	0.00	0.00