
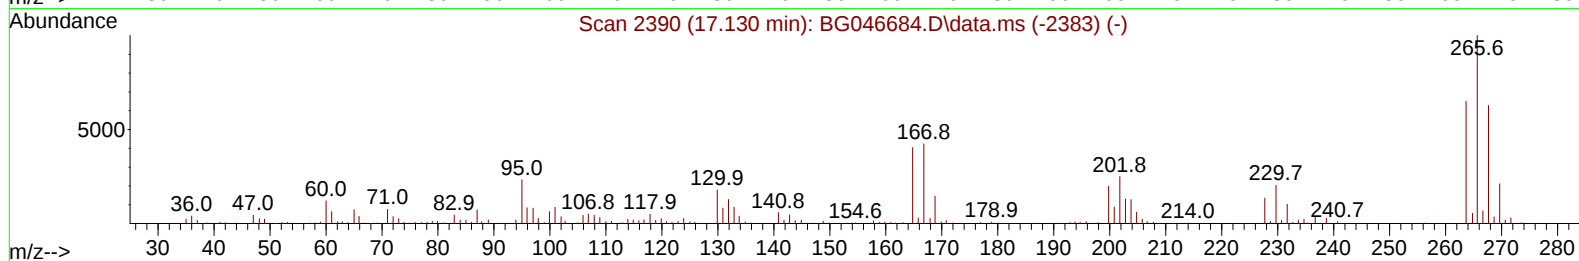
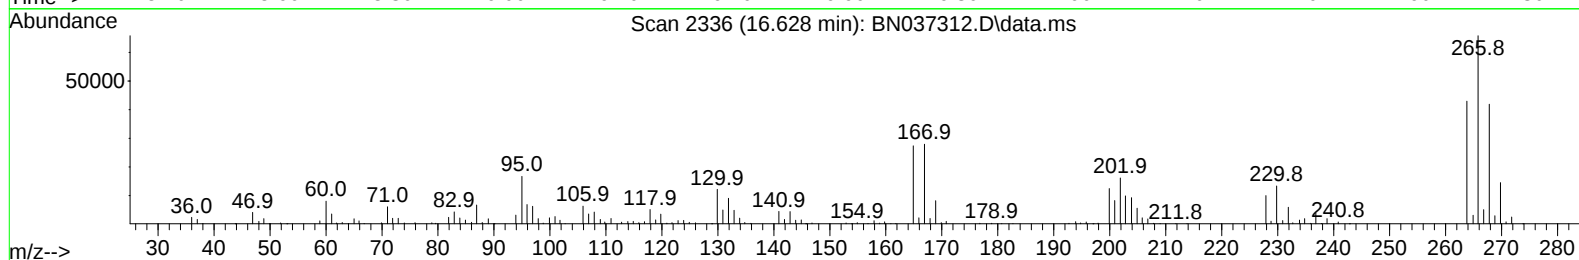


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN061925\  
Data File : BN037312.D  
Acq On : 18 Jun 2025 13:27  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 18:44:53 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 16 03:00:26 2025  
Response via : Initial Calibration

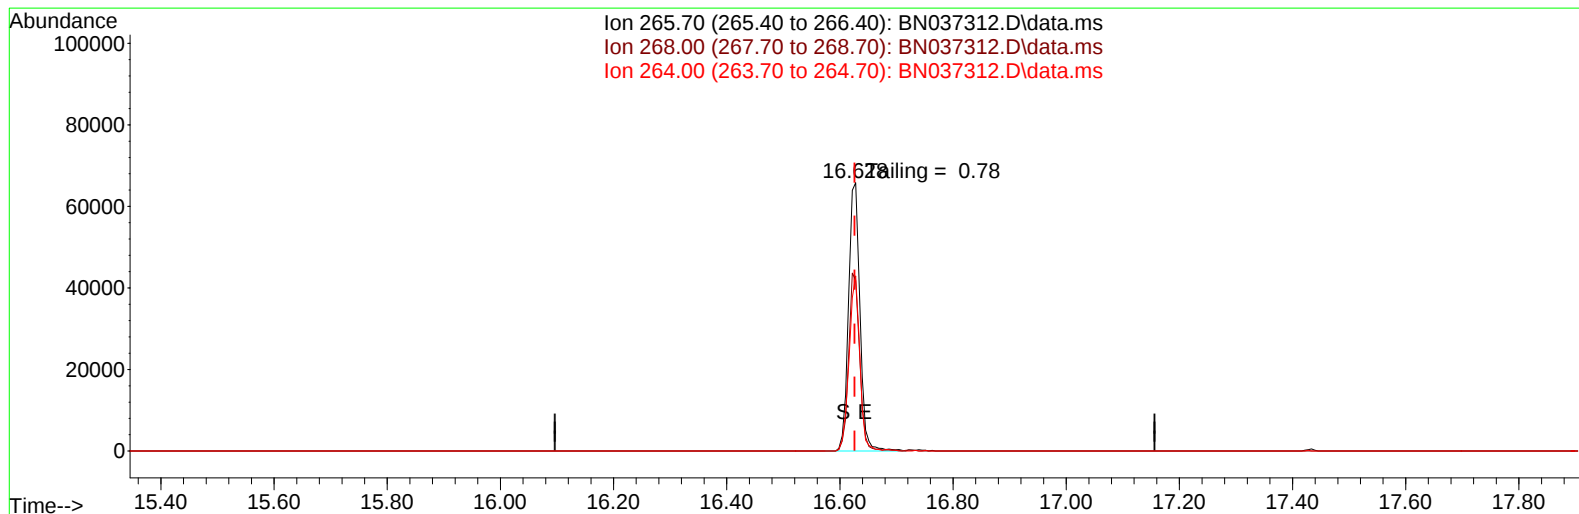

TIC: BN037312.D\data.ms

**(70) Pentachlorophenol (C)**




16.628min (+ 0.002) 17135.53 ng

response 92519

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.64  |
| 264.00 | 61.60  | 65.26  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN061925\  
Data File : BN037312.D  
Acq On : 18 Jun 2025 13:27  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 18:48:49 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 16 03:00:26 2025  
Response via : Initial Calibration

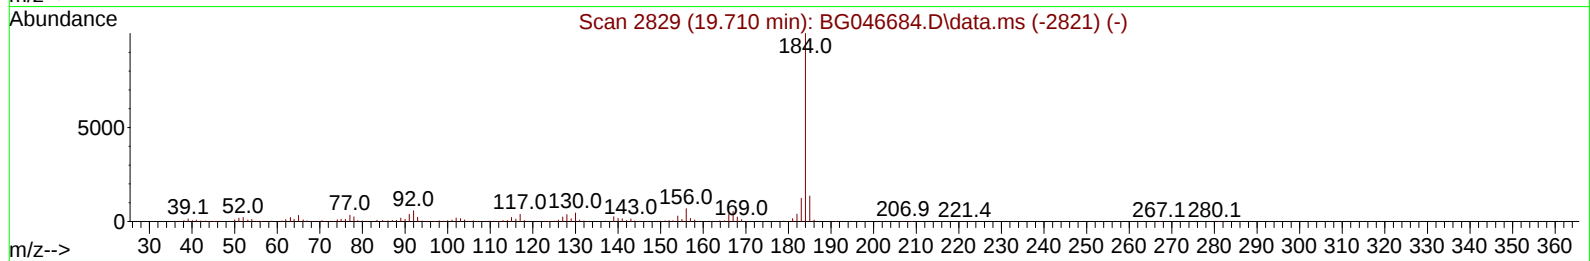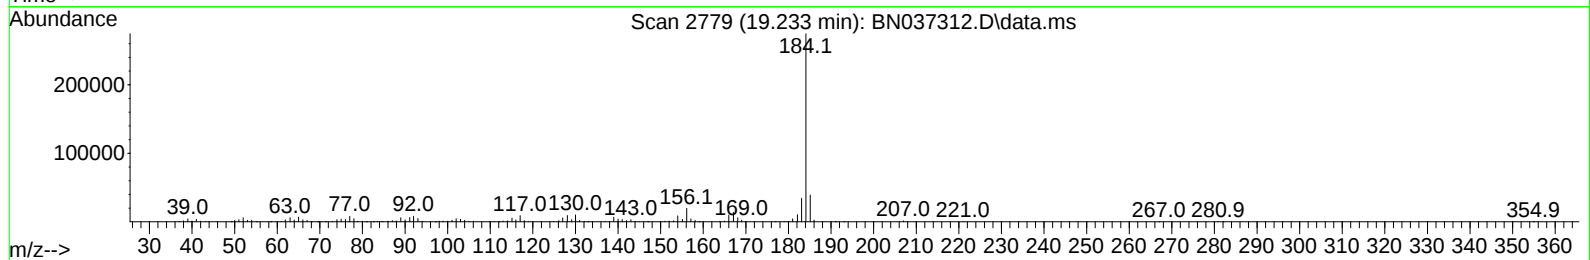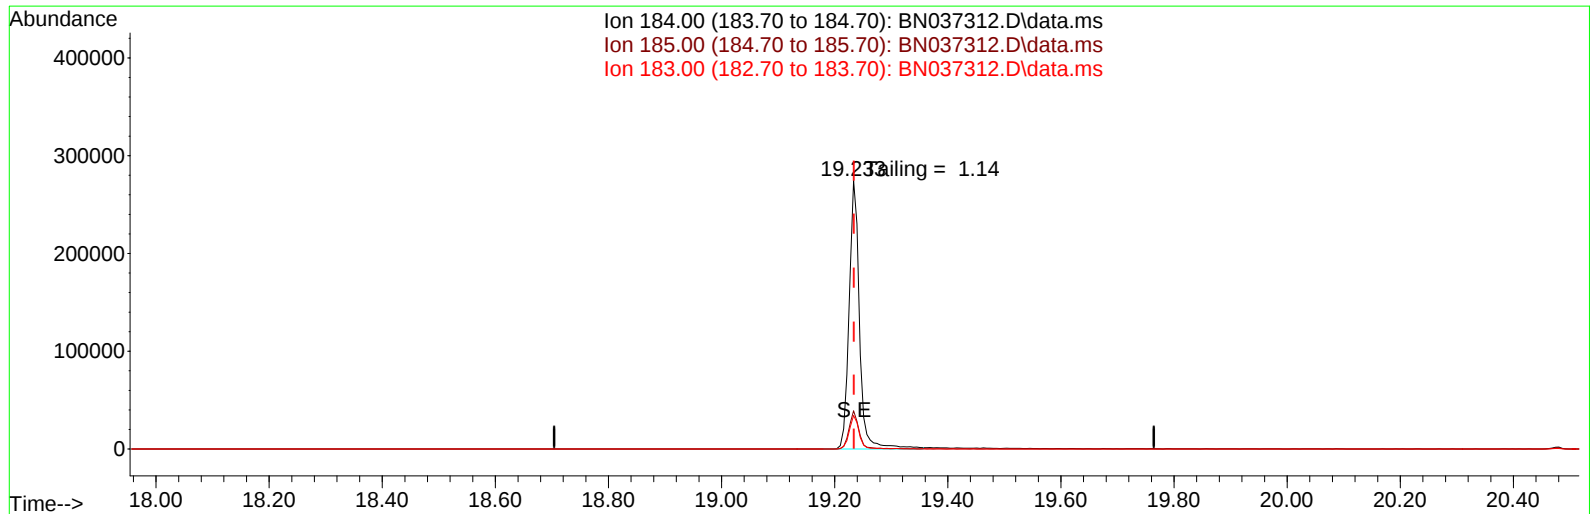

TIC: BN037312.D\data.ms

**(77) Benzidine**

19.233min (-0.001) 0.00 ng

response 354315

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.28  |
| 183.00 | 13.20  | 12.45  |
| 0.00   | 0.00   | 0.00   |