
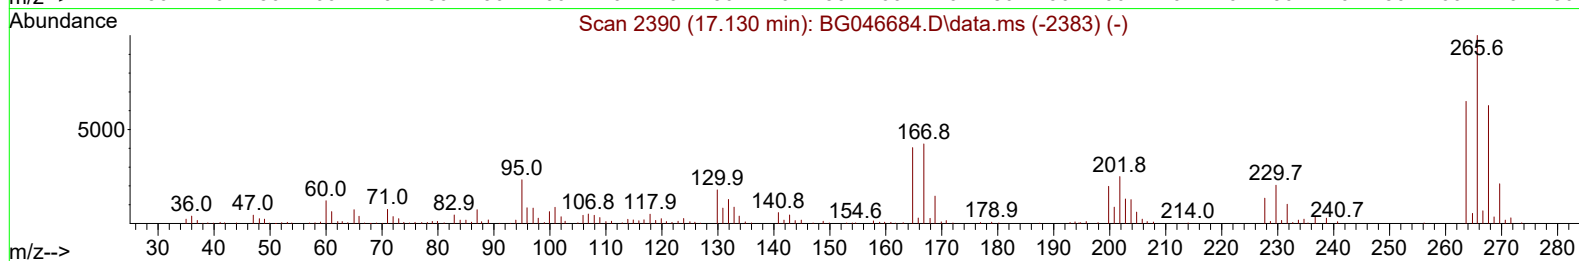
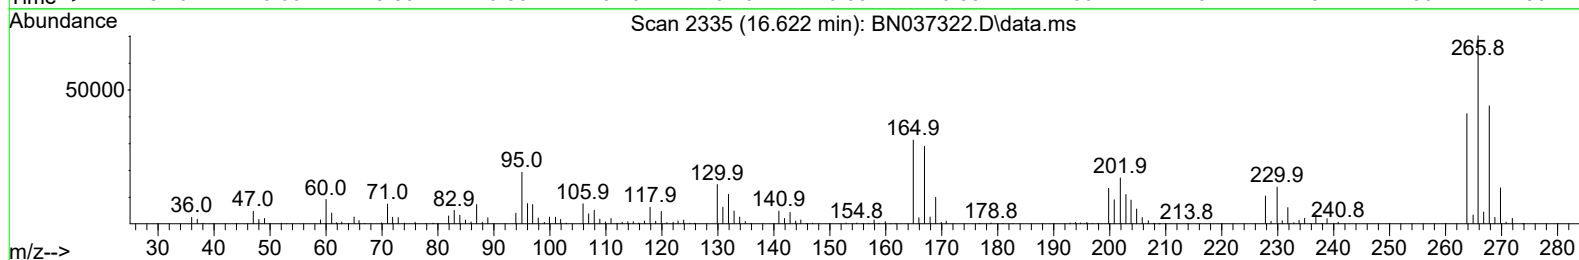


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061925\
Data File : BN037322.D
Acq On : 18 Jun 2025 20:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 02:50:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 19 02:50:12 2025
Response via : Initial Calibration

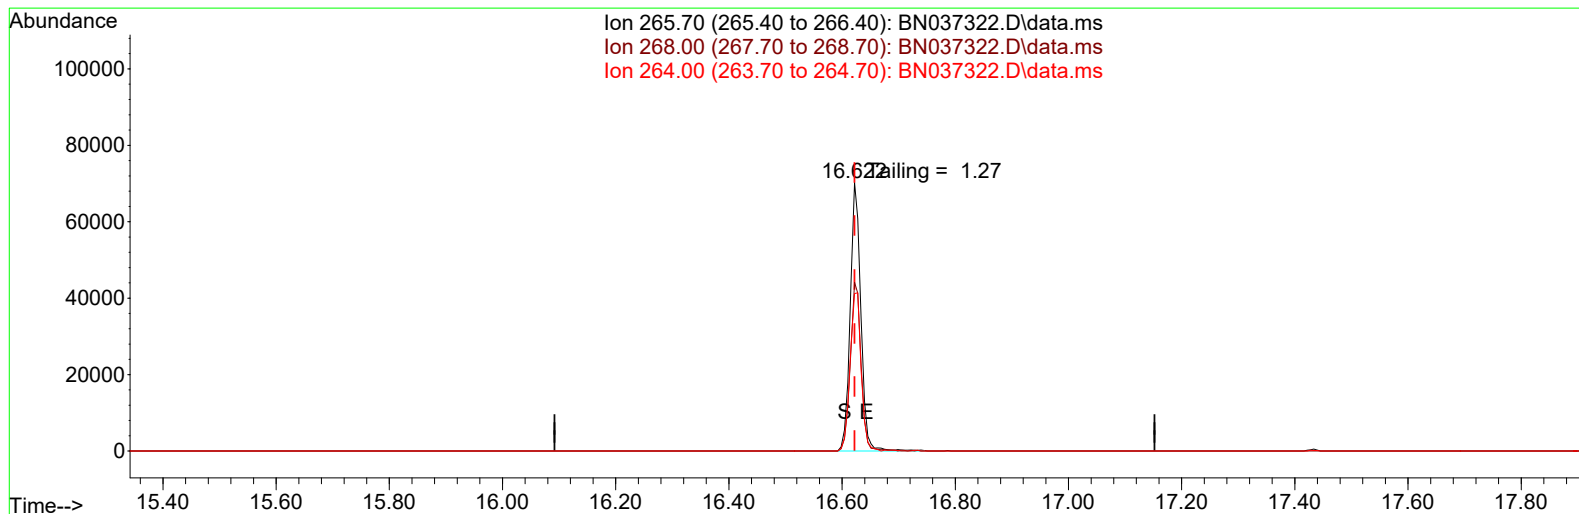

TIC: BN037322.D\data.ms

(70) Pentachlorophenol (C)




16.622min (0.000) 19762.00 ng

response 90726

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.84
264.00	61.60	58.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061925\
Data File : BN037322.D
Acq On : 18 Jun 2025 20:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 02:50:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 19 02:50:12 2025
Response via : Initial Calibration

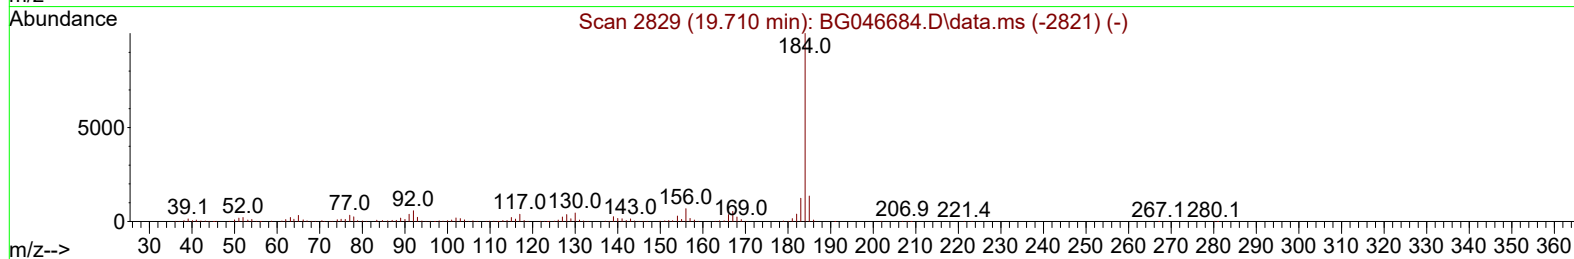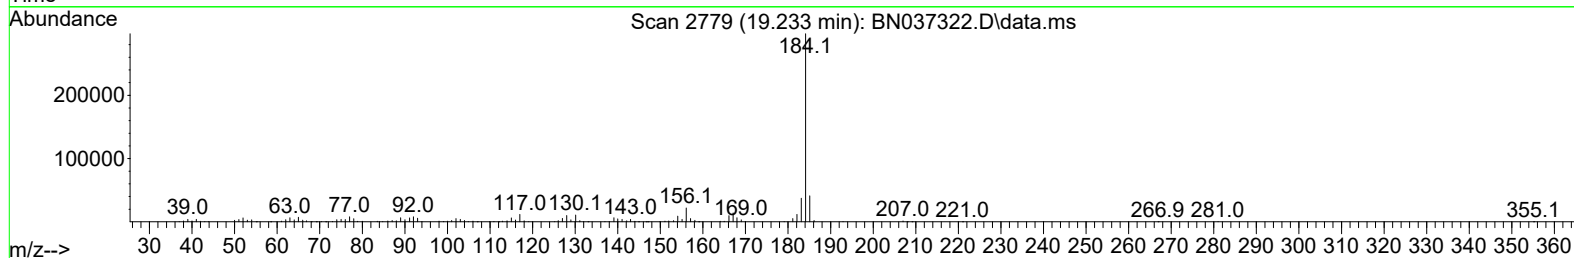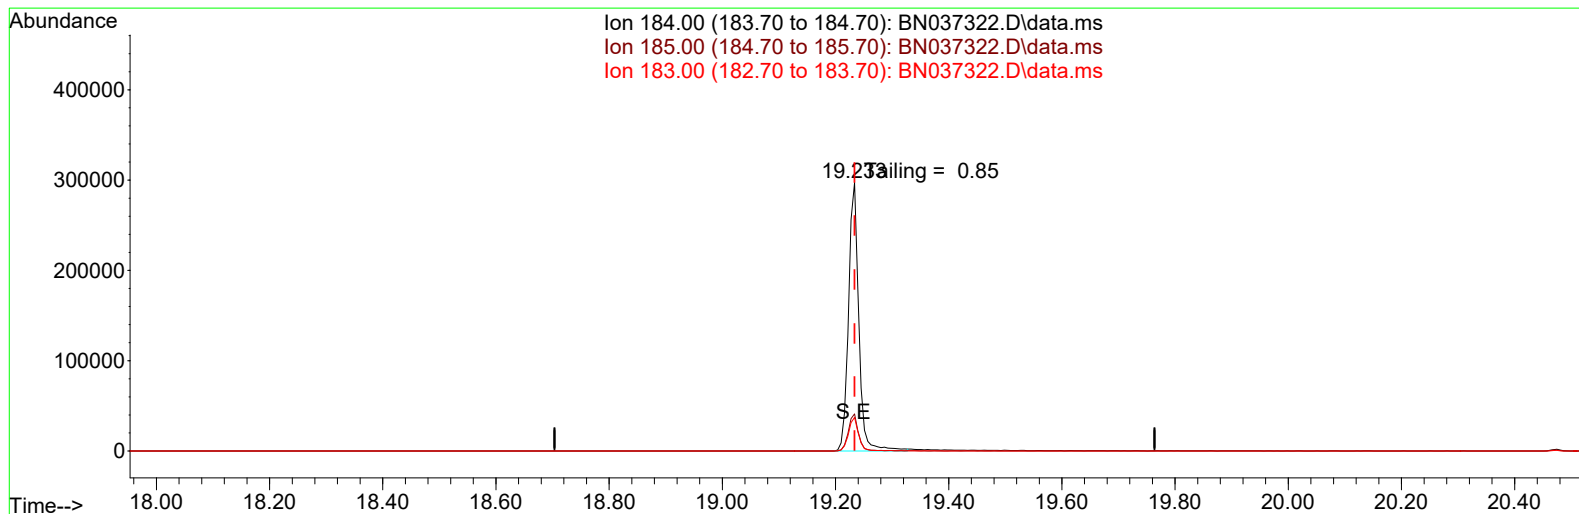

TIC: BN037322.D\data.ms

(77) Benzidine

19.233min (0.000) 0.00 ng

response 373179

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	12.54
0.00	0.00	0.00