


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061925\
Data File : BN037312.D
Acq On : 18 Jun 2025 13:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 19 02:50:12 2025

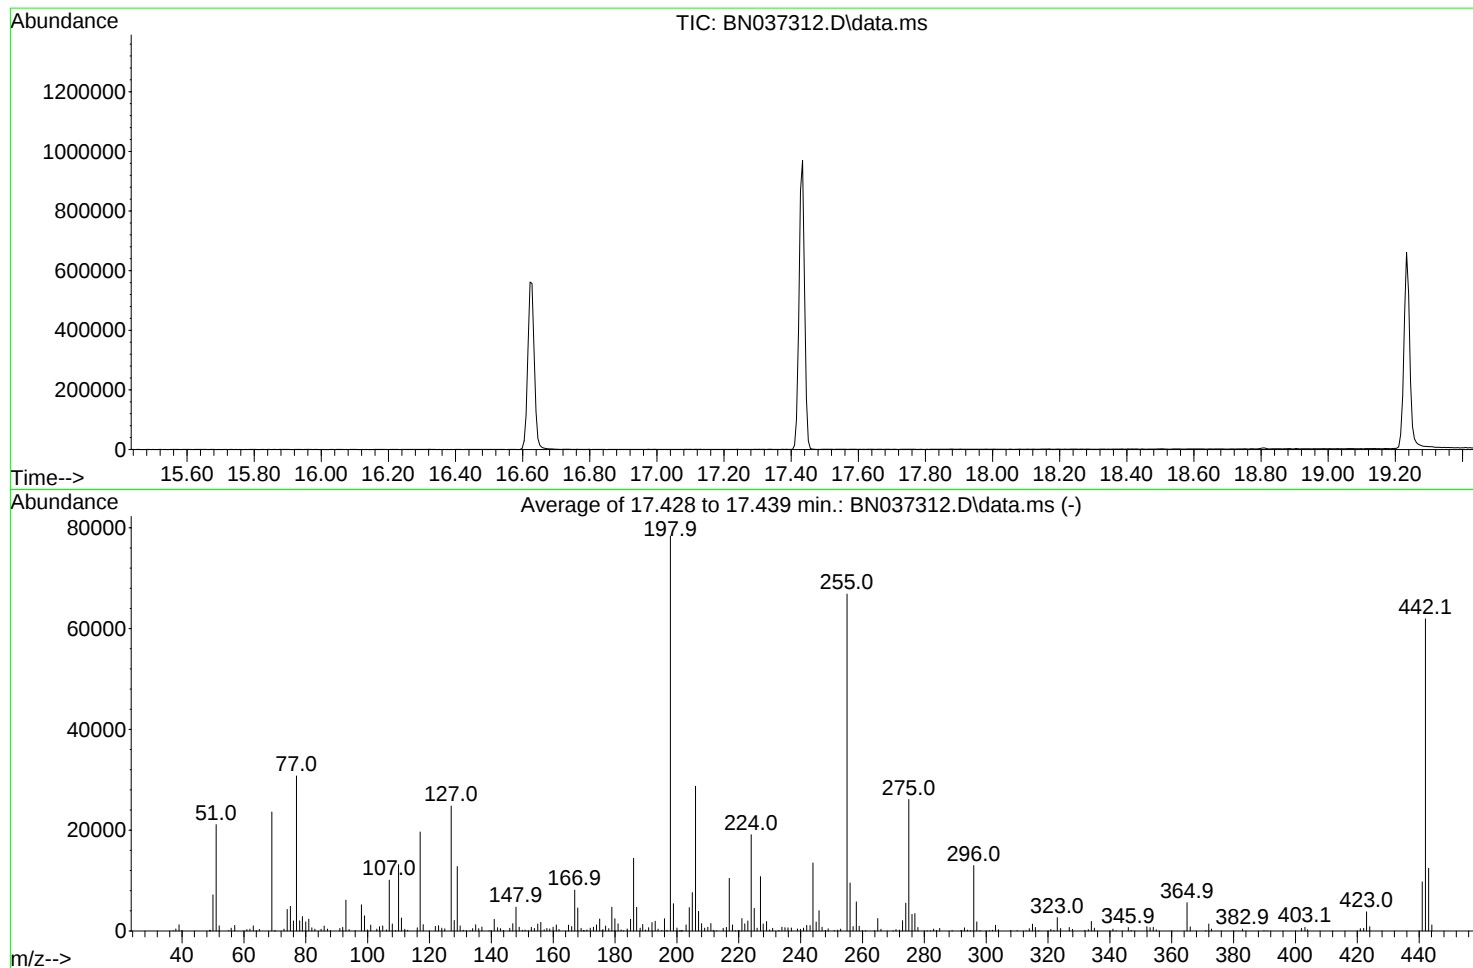




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	23638	PASS
70	69	0.00	2	0.3	60	PASS
197	198	0.00	2	0.2	162	PASS
198	198	100	100	100.0	78347	PASS
199	198	5	9	6.9	5444	PASS
365	198	1	100	7.2	5637	PASS
441	443	0.01	150	78.3	9747	PASS
442	442	100	100	100.0	61936	PASS
443	442	15	24	20.1	12447	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061925\
Data File : BN037312.D
Acq On : 18 Jun 2025 13:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 18 18:44:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 16 03:00:26 2025
Response via : Initial Calibration

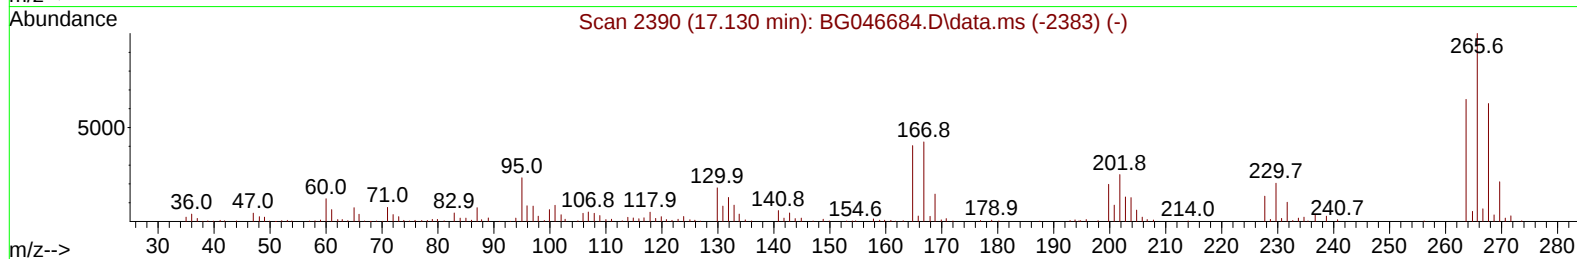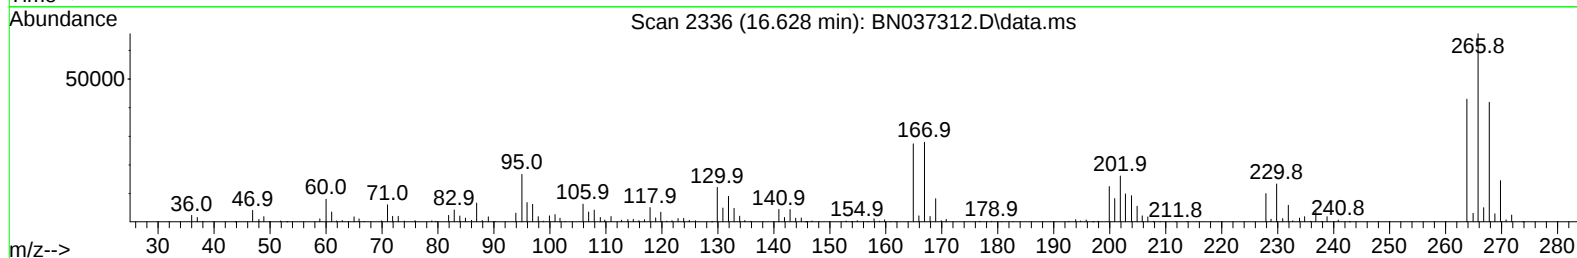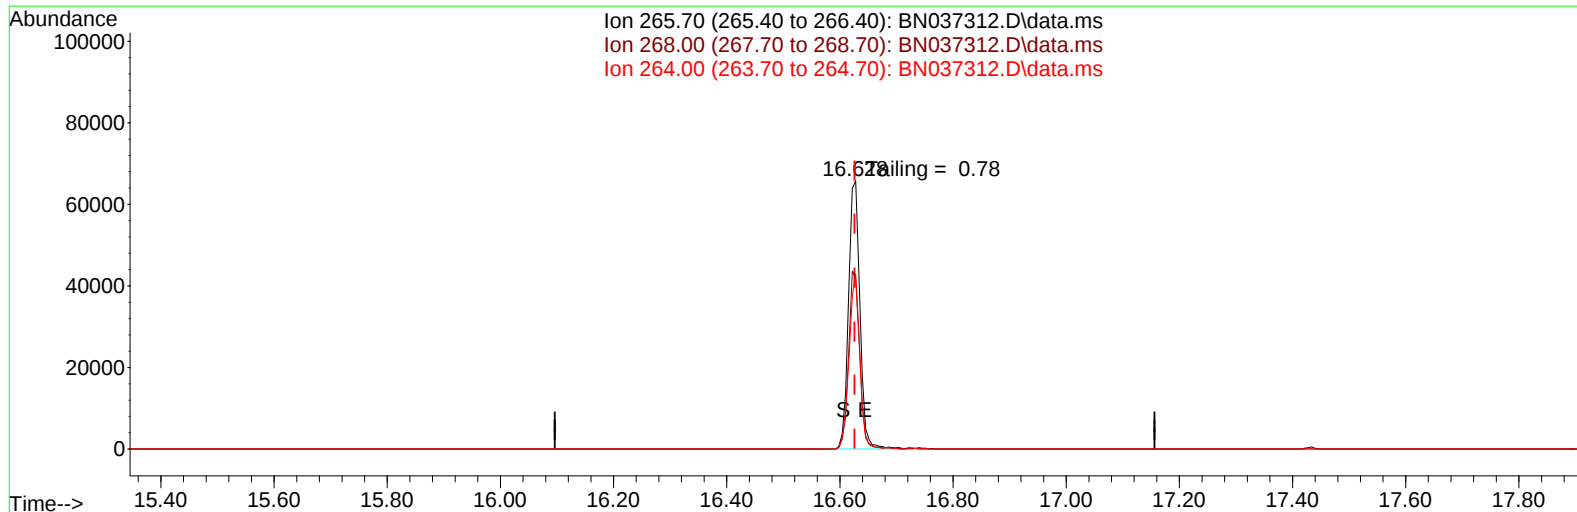

TIC: BN037312.D\data.ms

(70) Pentachlorophenol (C)

16.628min (+ 0.002) 17135.53 ng




response 92519

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.64
264.00	61.60	65.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061925\
Data File : BN037312.D
Acq On : 18 Jun 2025 13:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 18 18:48:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 16 03:00:26 2025
Response via : Initial Calibration

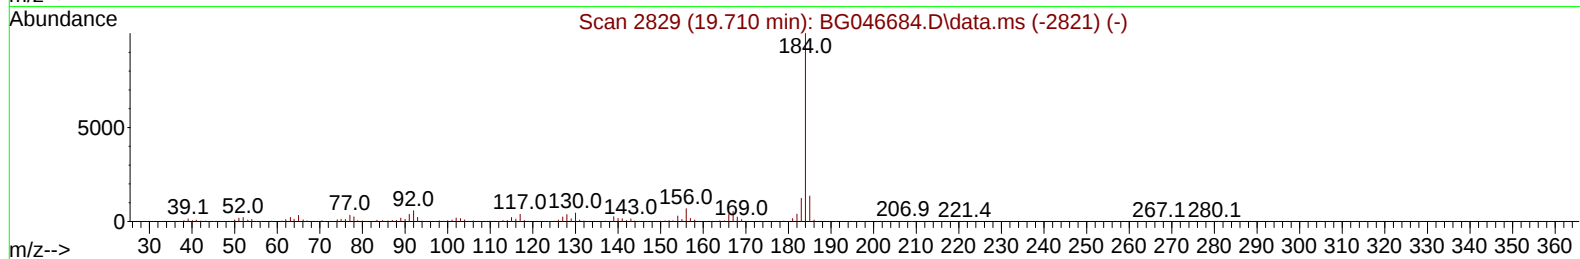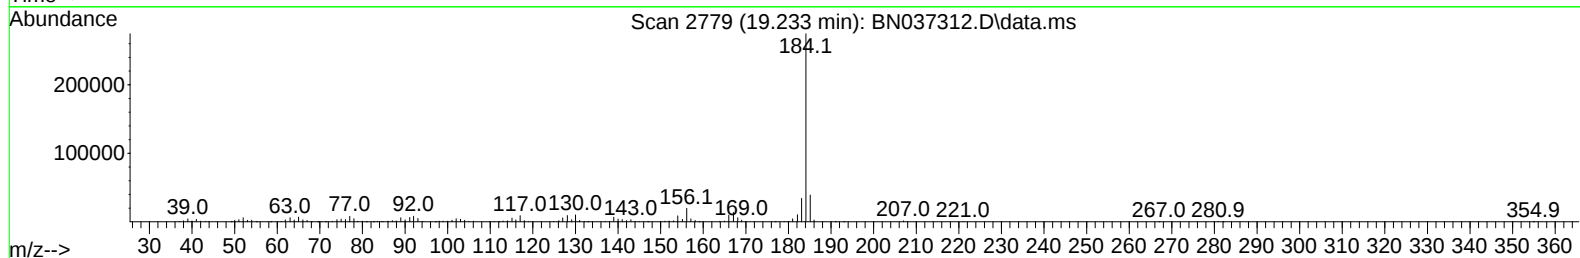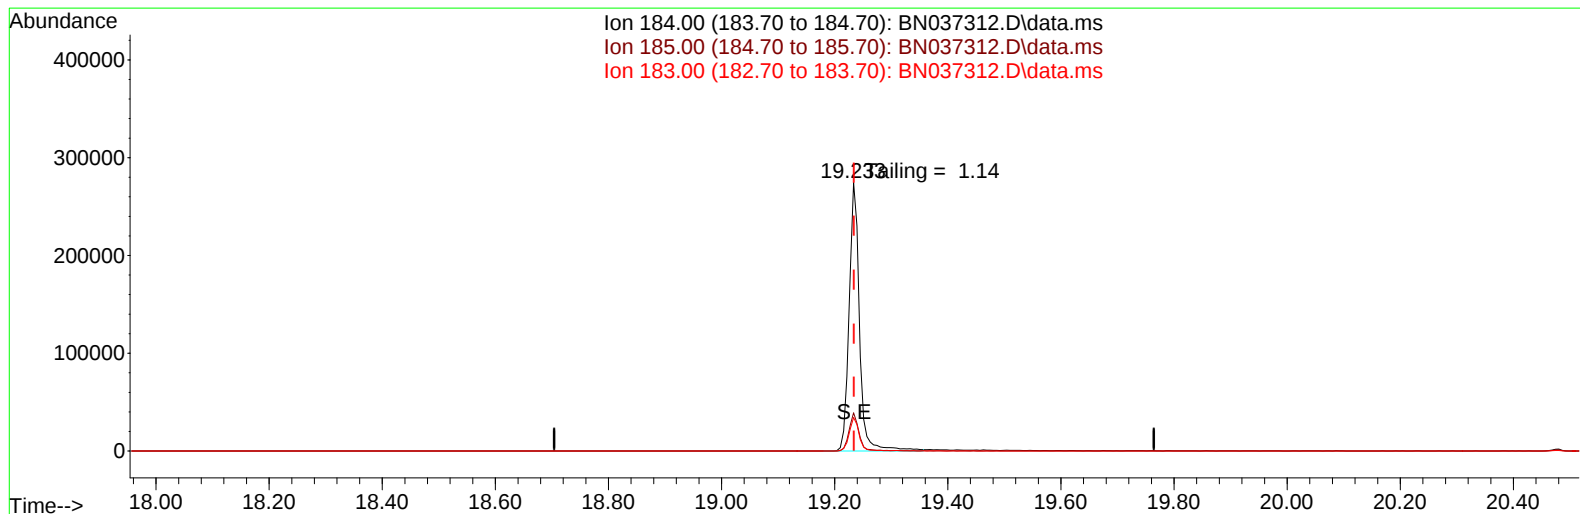

TIC: BN037312.D\data.ms

(77) Benzidine

19.233min (-0.001) 0.00 ng

response 354315

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.28
183.00	13.20	12.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/19/2025	BNA_N	<u>BN037312.D</u>
Compound Name	Response	Retention Time
DDT	261804	20.475
DDD	4079	20.039
DDE	148	19.528
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4227	266031	1.59

Instrument :
BNA_N
ClientSampleId :
DFTPP