

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020272.D
 Acq On : 20 Jun 2022 11:17
 Operator : CG/JU
 Sample : PB145543BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK543

Quant Time: Jun 21 02:37:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	1553	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	5746	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.418	164	4088	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.162	188	9923	0.400	ng/ul	0.00
17) Chrysene-d12	21.356	240	10039	0.400	ng/ul	0.00
23) Perylene-d12	23.662	264	12895	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	7830	4.415	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.179	152	2625	0.276	ng/ul	0.00
18) Fluoranthene-d10	19.192	212	8426	0.407	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.413	166	987	0.051	ng/ul#	18
20) Pyrene	19.555	202	1295	0.029	ng/ul#	1
26) Benzo(a)pyrene	23.513	252	3466	0.059	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020272.D
Acq On : 20 Jun 2022 11:17
Operator : CG/JU
Sample : PB145543BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK543

Quant Time: Jun 21 02:37:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




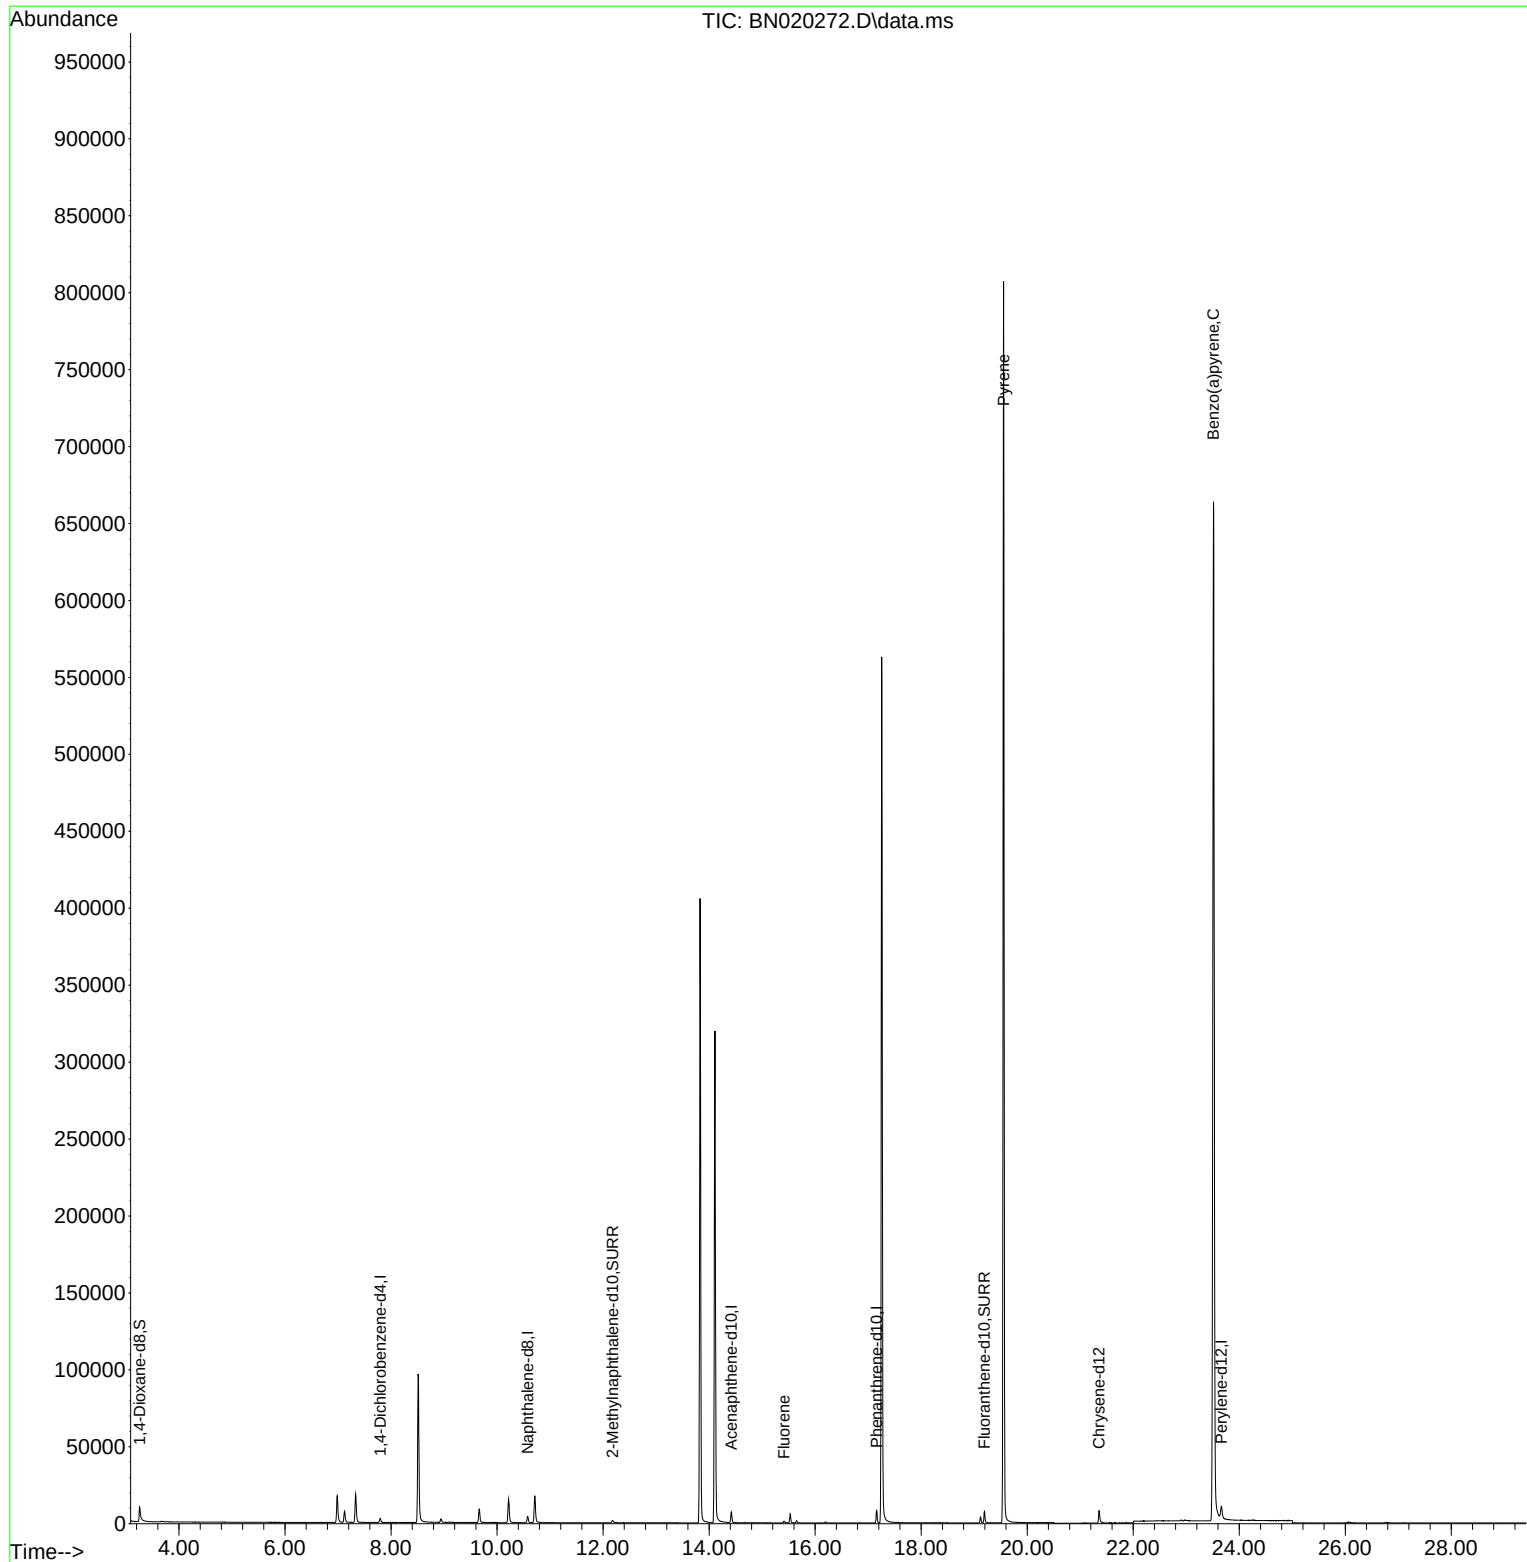


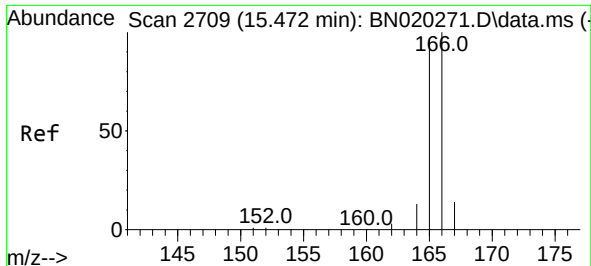

#12
Fluorene
Concen: 0.051 ng/ul
RT: 15.413 min Scan# 2696
Delta R.T. -0.060 min
Lab File: BN020272.D
Acq: 20 Jun 2022 11:17




Instrument :
BNA_N
ClientSampleId :
SBLK543


Tgt Ion:166 Resp: 987
Ion Ratio Lower Upper
166 100
165 12.6 78.2 117.4#
167 38.2 12.1 18.1#

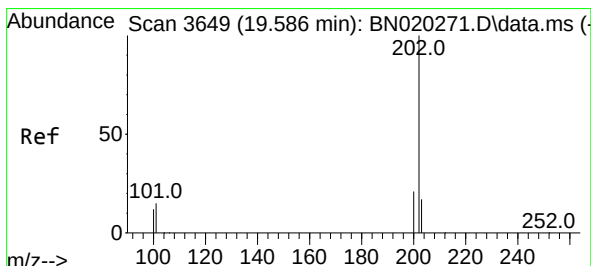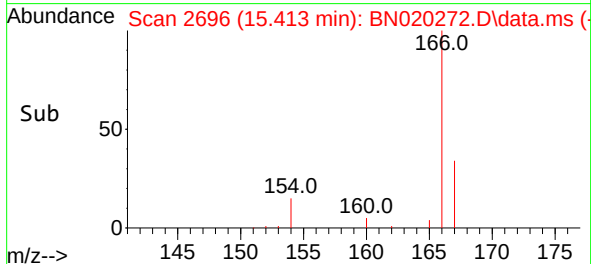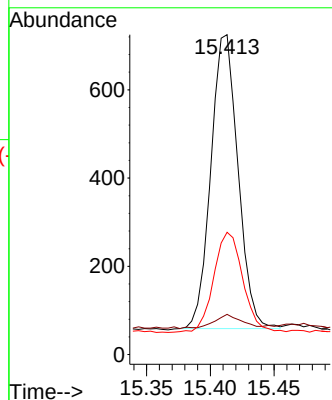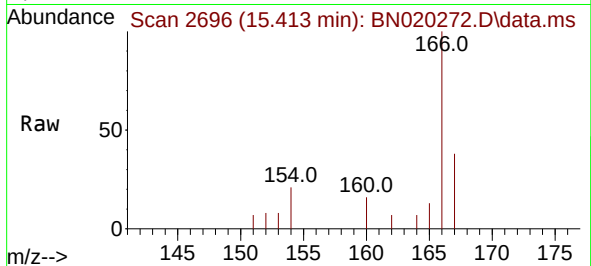

#20
Pyrene
Concen: 0.029 ng/ul
RT: 19.555 min Scan# 3642
Delta R.T. -0.028 min
Lab File: BN020272.D
Acq: 20 Jun 2022 11:17

Tgt Ion:202 Resp: 1295
Ion Ratio Lower Upper
202 100
101 166.2 12.6 19.0#
100 1183.8 10.3 15.5#

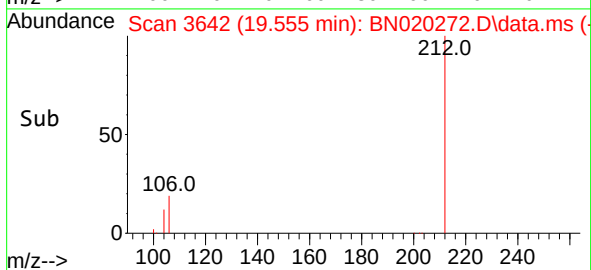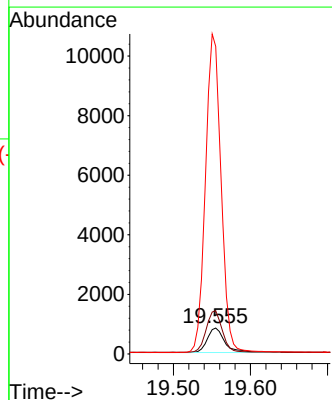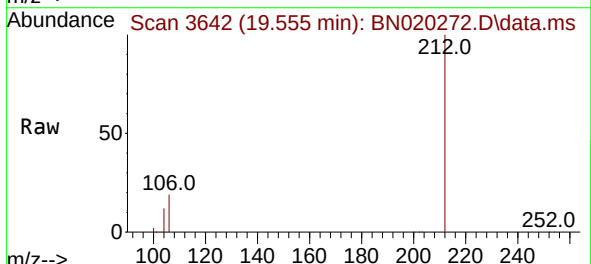

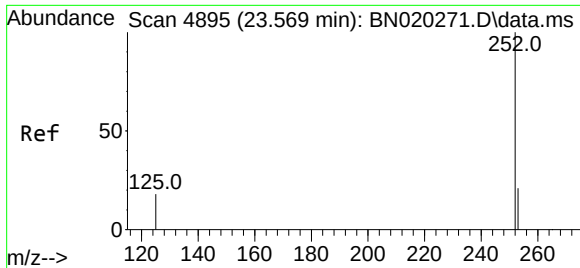

#26

Benzo(a)pyrene

Concen: 0.059 ng/ul

RT: 23.513 min Scan# 4876

Delta R.T. -0.050 min

Lab File: BN020272.D


Acq: 20 Jun 2022 11:17

Instrument :

BNA_N

ClientSampleId :

SBLK543

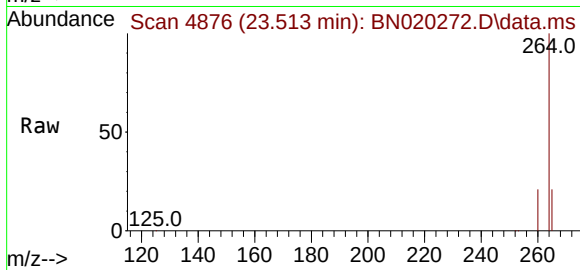

Tgt Ion:252 Resp: 3466

Ion Ratio Lower Upper

252 100

253 43.9 21.7 32.5#

125 36.4 18.6 28.0#

