

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020278.D
 Acq On : 20 Jun 2022 14:52
 Operator : CG/JU
 Sample : N3294-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P7

Quant Time: Jun 21 02:37:56 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	792	0.400	ng/ul	0.00
4) Naphthalene-d8	10.584	136	3182	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.423	164	2900	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.162	188	7196	0.400	ng/ul	0.00
17) Chrysene-d12	21.353	240	8488	0.400	ng/ul	# 0.00
23) Perylene-d12	23.662	264	11164	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	4428	4.896	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.173	152	2097	0.399	ng/ul	0.00
18) Fluoranthene-d10	19.192	212	9933	0.567	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.256	88	94	0.108	ng/ul#	68
20) Pyrene	19.555	202	1527	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.516	252	3750	0.074	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020278.D
Acq On : 20 Jun 2022 14:52
Operator : CG/JU
Sample : N3294-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P7


Quant Time: Jun 21 02:37:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration

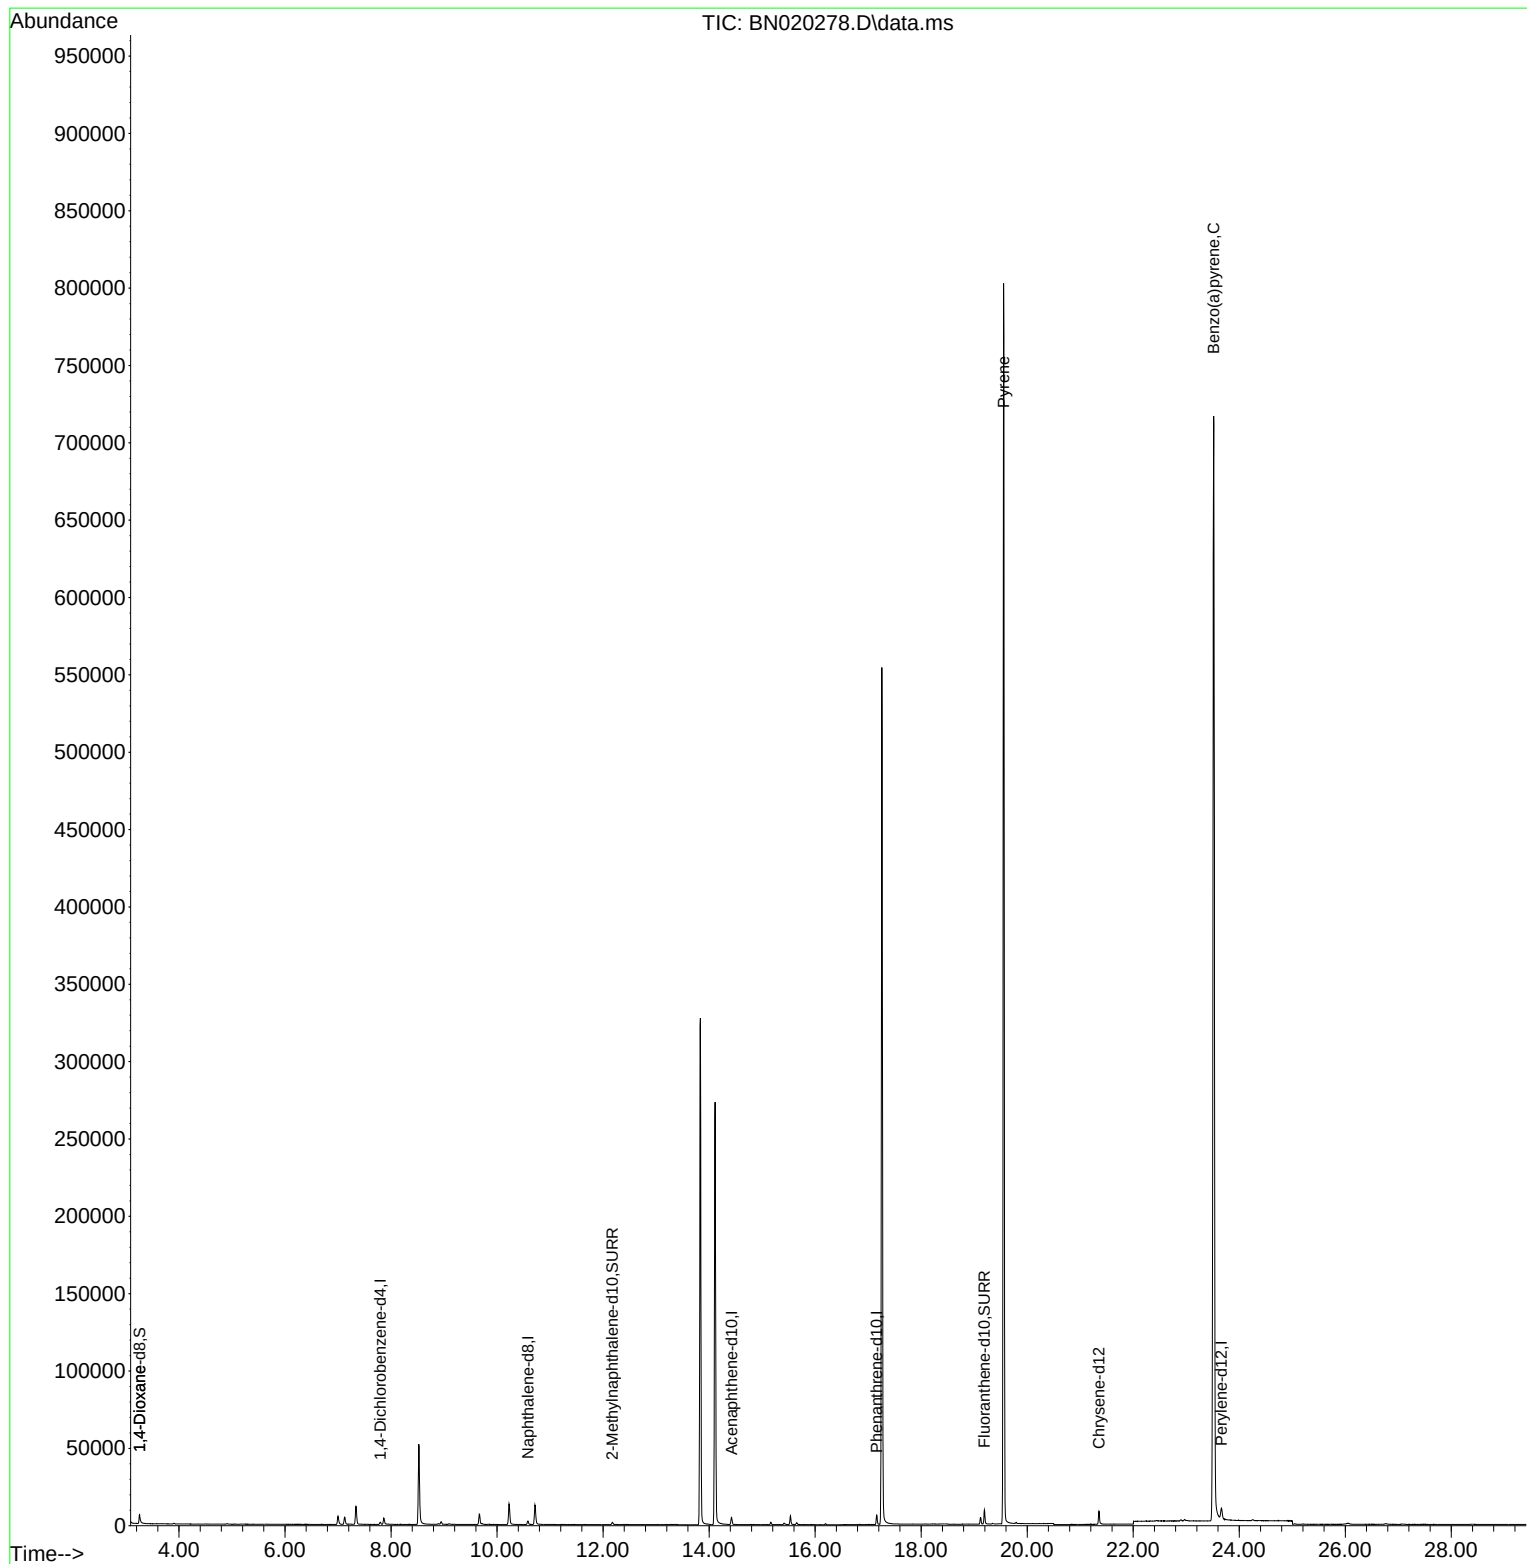



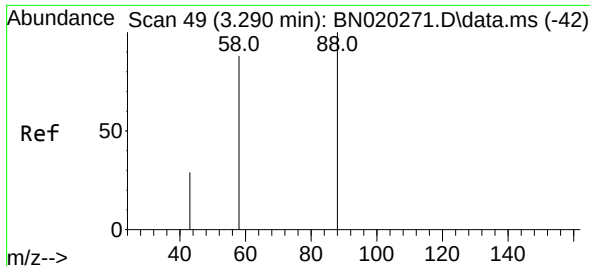


#2
 1,4-Dioxane
 Concen: 0.108 ng/ul
 RT: 3.256 min Scan# 41
 Delta R.T. -0.038 min
 Lab File: BN020278.D
 Acq: 20 Jun 2022 14:52


Instrument :
 BNA_N
 ClientSampleId :
 EW4P7

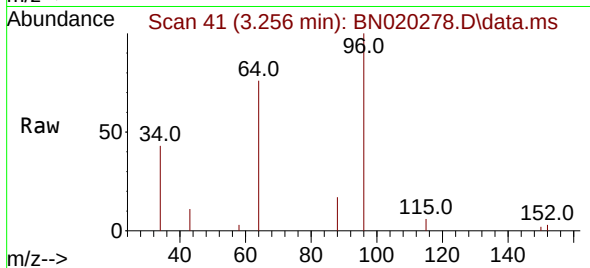



Tgt Ion: 88 Resp: 94
 Ion Ratio Lower Upper
 88 100
 43 66.0 31.6 47.4#
 58 20.0 23.8 35.6#

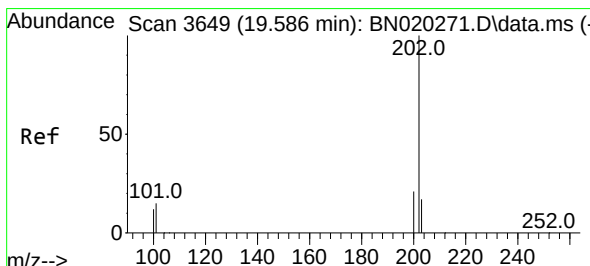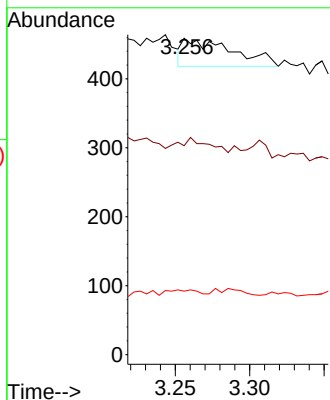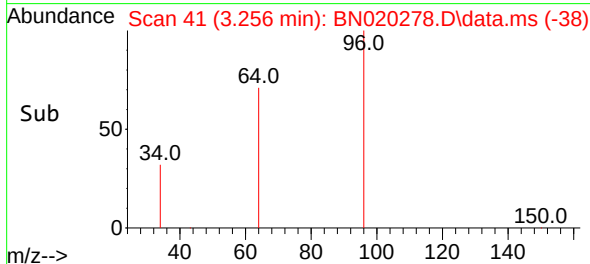


#20
 Pyrene
 Concen: 0.041 ng/ul
 RT: 19.555 min Scan# 3642
 Delta R.T. -0.028 min
 Lab File: BN020278.D
 Acq: 20 Jun 2022 14:52

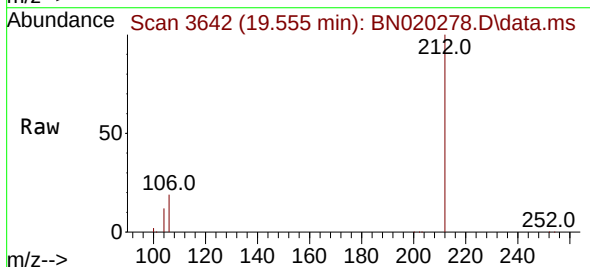


Tgt Ion: 202 Resp: 1527
 Ion Ratio Lower Upper
 202 100
 101 165.5 12.6 19.0#
 100 1180.2 10.3 15.5#

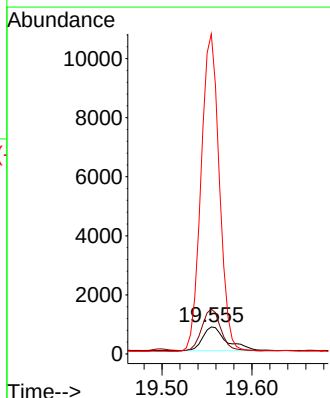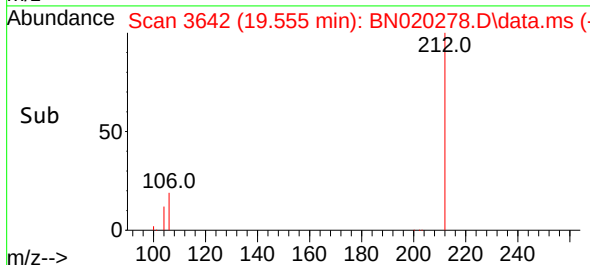

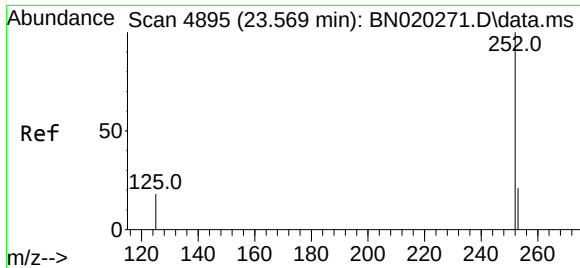

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.516 min Scan# 4877
Delta R.T. -0.047 min
Lab File: BN020278.D
Acq: 20 Jun 2022 14:52

Instrument :
BNA_N
ClientSampleId :
EW4P7

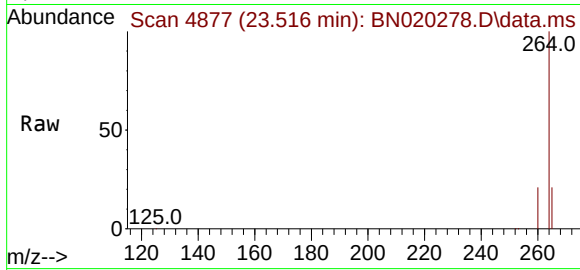

Tgt Ion:252 Resp: 3750
Ion Ratio Lower Upper
252 100
253 52.0 21.7 32.5#
125 43.4 18.6 28.0#

