

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020279.D
 Acq On : 20 Jun 2022 15:28
 Operator : CG/JU
 Sample : N3294-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q0

Quant Time: Jun 21 02:38:01 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	941	0.400	ng/ul	0.00
4) Naphthalene-d8	10.584	136	3872	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.423	164	3150	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.162	188	8261	0.400	ng/ul	0.00
17) Chrysene-d12	21.356	240	10020	0.400	ng/ul	0.00
23) Perylene-d12	23.665	264	13319	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	4704	4.378	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.174	152	2186	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.193	212	9540	0.461	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.265	88	90	0.087	ng/ul#	70
14) Pentachlorophenol	16.833	266	33	0.021	ng/ul#	75
20) Pyrene	19.555	202	1372	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.519	252	3995	0.066	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020279.D
Acq On : 20 Jun 2022 15:28
Operator : CG/JU
Sample : N3294-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q0


Quant Time: Jun 21 02:38:01 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration

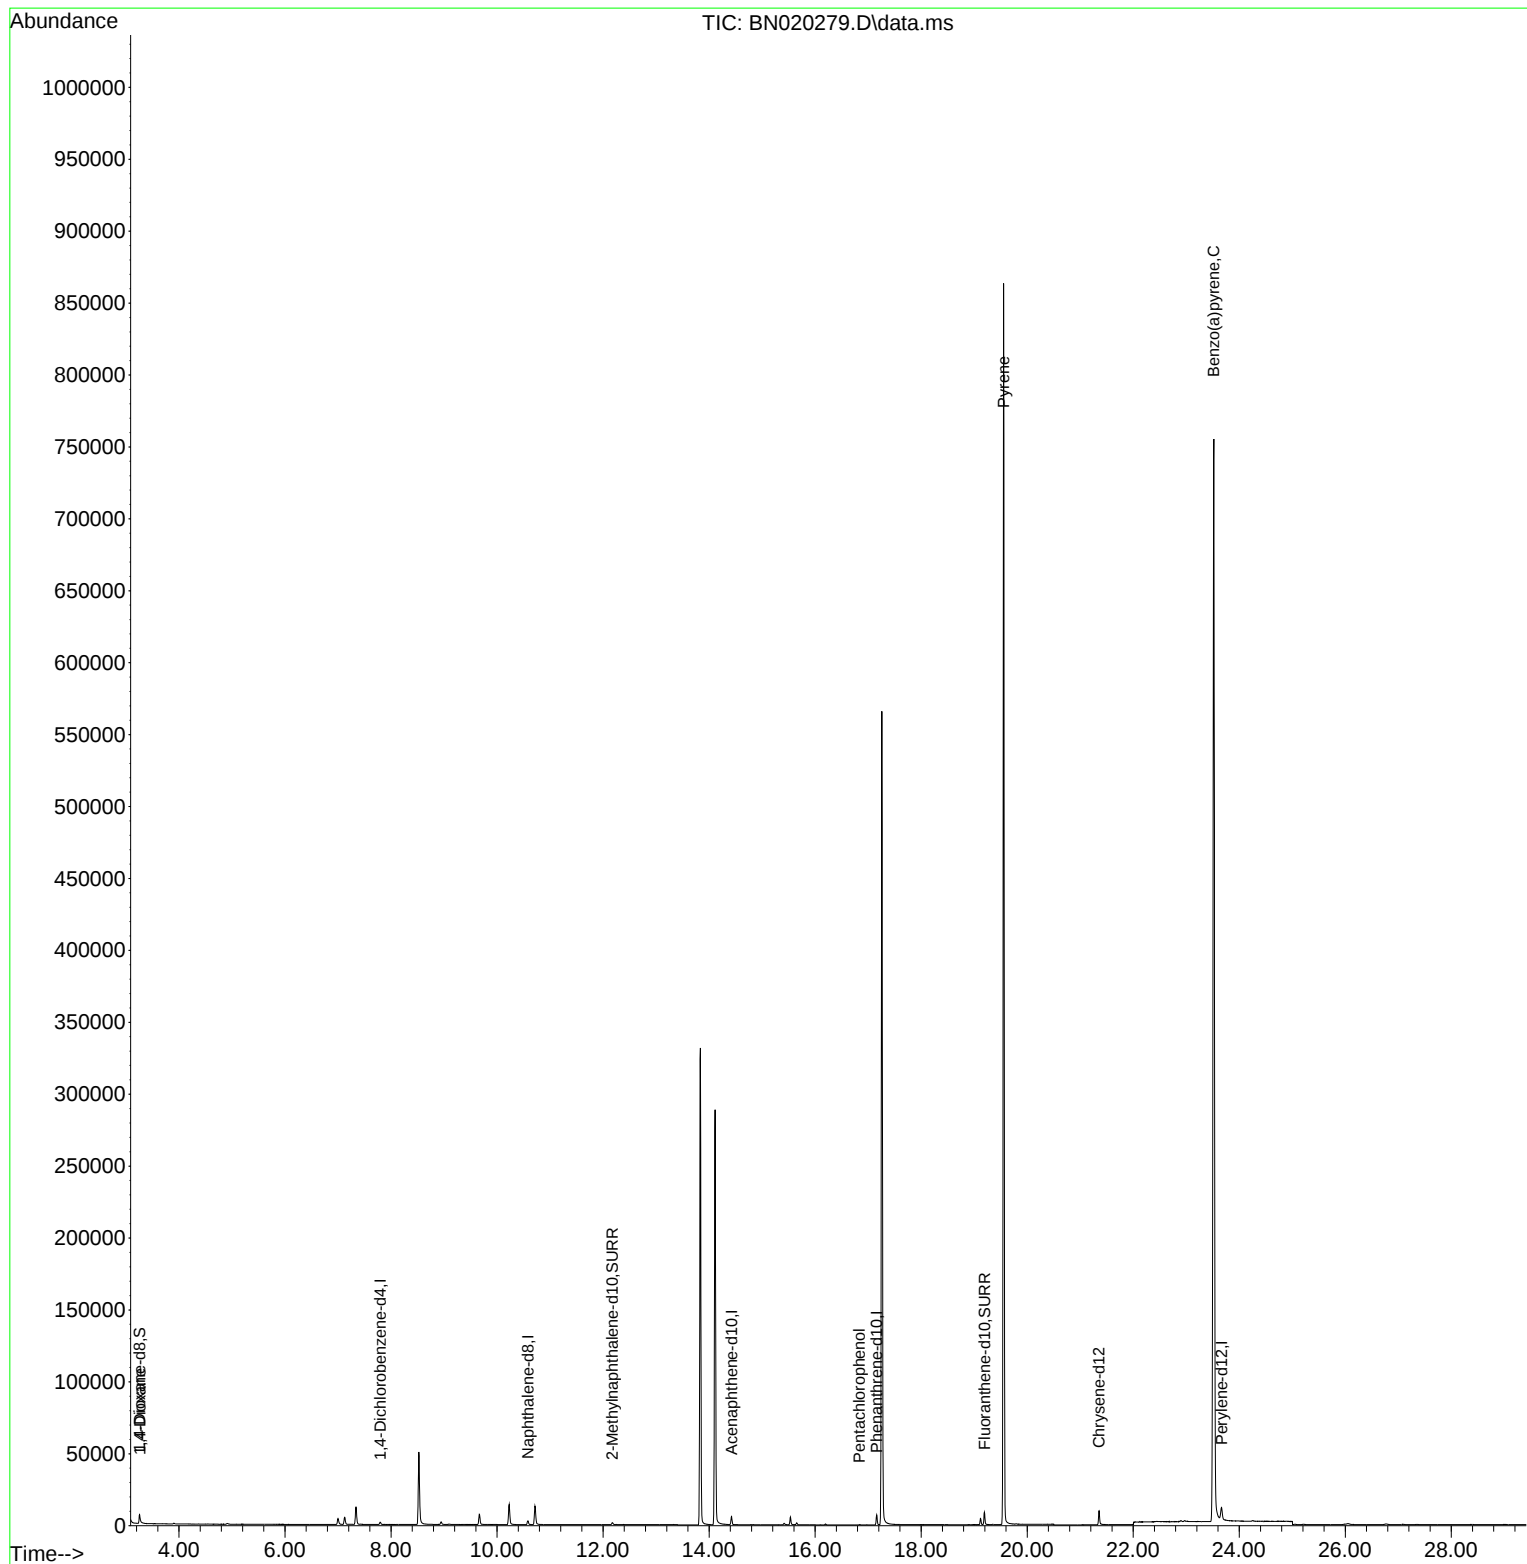



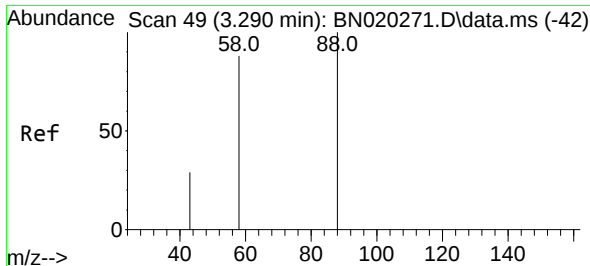


#2
 1,4-Dioxane
 Concen: 0.087 ng/ul
 RT: 3.265 min Scan# 41
 Delta R.T. -0.029 min
 Lab File: BN020279.D
 Acq: 20 Jun 2022 15:28


Instrument :
 BNA_N
 ClientSampleId :
 EW4Q0

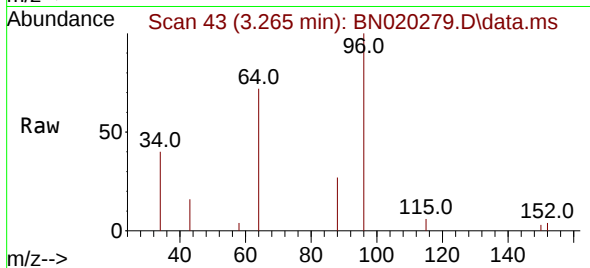



Tgt Ion: 88 Resp: 90
 Ion Ratio Lower Upper
 88 100
 43 59.2 31.6 47.4#
 58 15.2 23.8 35.6#

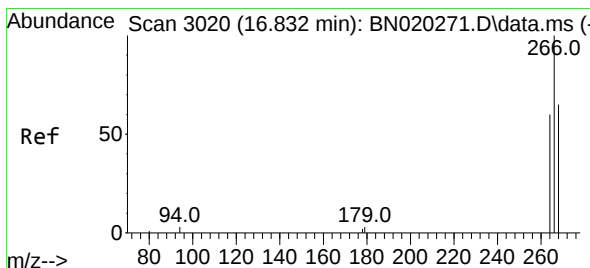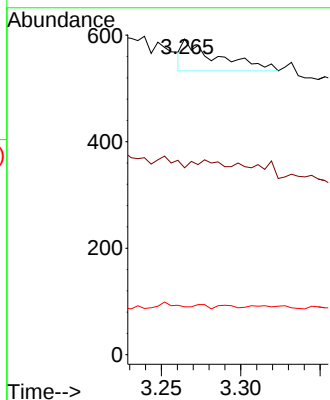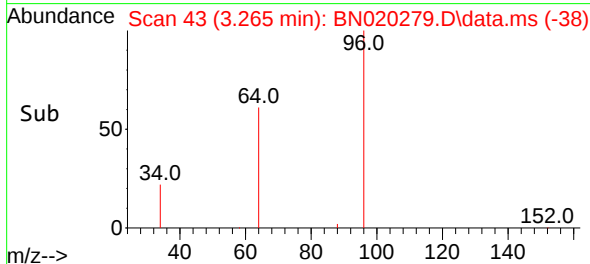


#14
 Pentachlorophenol
 Concen: 0.021 ng/ul
 RT: 16.833 min Scan# 3020
 Delta R.T. -0.004 min
 Lab File: BN020279.D
 Acq: 20 Jun 2022 15:28

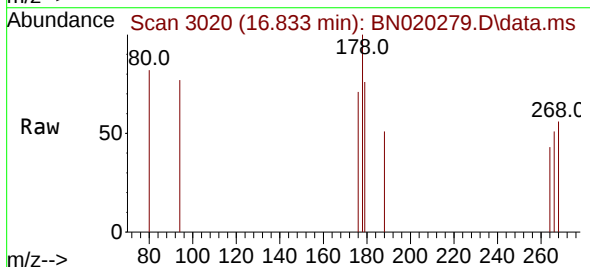

Tgt Ion: 266 Resp: 33
 Ion Ratio Lower Upper
 266 100
 264 45.5 49.8 74.8#
 268 42.4 51.8 77.6#



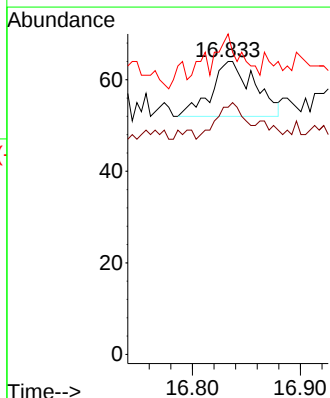
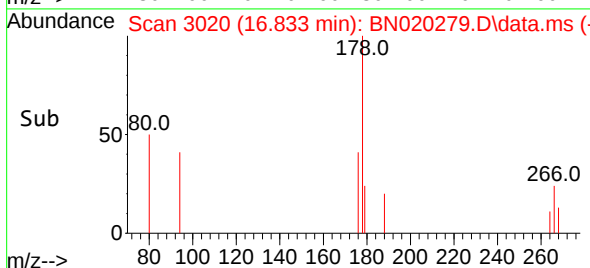


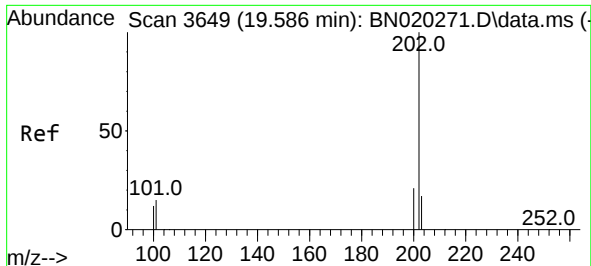

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.555 min Scan# 3642
Delta R.T. -0.028 min
Lab File: BN020279.D
Acq: 20 Jun 2022 15:28

Instrument :
BNA_N
ClientSampleId :
EW4Q0

Tgt Ion:202 Resp: 1372
Ion Ratio Lower Upper
202 100
101 165.0 12.6 19.0#
100 1171.7 10.3 15.5#

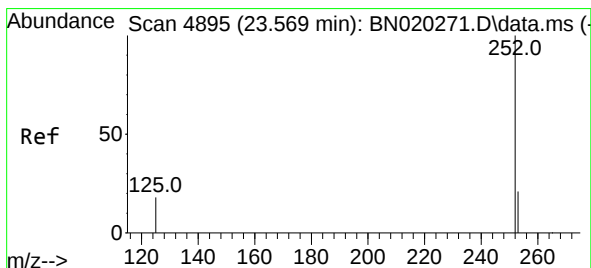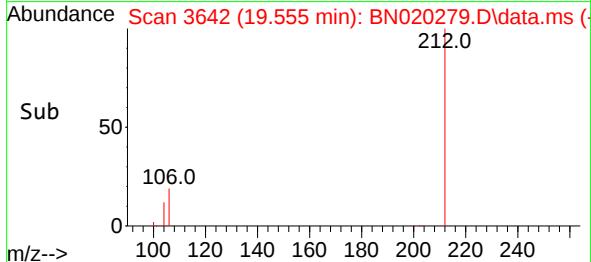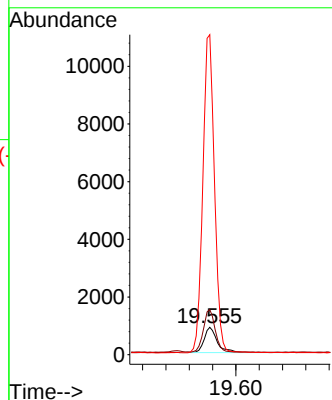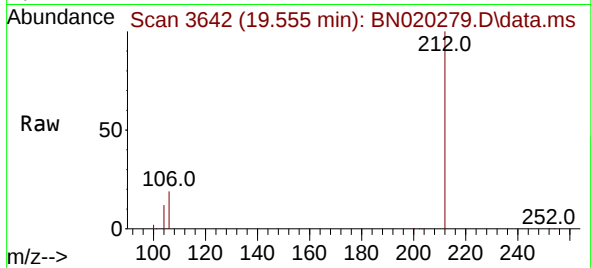

#26
Benzo(a)pyrene
Concen: 0.066 ng/ul
RT: 23.519 min Scan# 4878
Delta R.T. -0.044 min
Lab File: BN020279.D
Acq: 20 Jun 2022 15:28

Tgt Ion:252 Resp: 3995
Ion Ratio Lower Upper
252 100
253 49.2 21.7 32.5#
125 41.1 18.6 28.0#

