

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020280.D
 Acq On : 20 Jun 2022 16:04
 Operator : CG/JU
 Sample : N3294-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q2

Quant Time: Jun 21 02:38:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	939	0.400	ng/ul	0.00
4) Naphthalene-d8	10.584	136	4044	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.423	164	3160	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.162	188	8248	0.400	ng/ul	0.00
17) Chrysene-d12	21.355	240	9842	0.400	ng/ul	0.00
23) Perylene-d12	23.667	264	11785	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	4133	3.855	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.174	152	1892	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.192	212	8914	0.439	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.413	166	815	0.054	ng/ul#	21
20) Pyrene	19.587	202	1172	0.027	ng/ul#	1
26) Benzo(a)pyrene	23.515	252	3138	0.059	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020280.D
Acq On : 20 Jun 2022 16:04
Operator : CG/JU
Sample : N3294-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q2

Quant Time: Jun 21 02:38:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




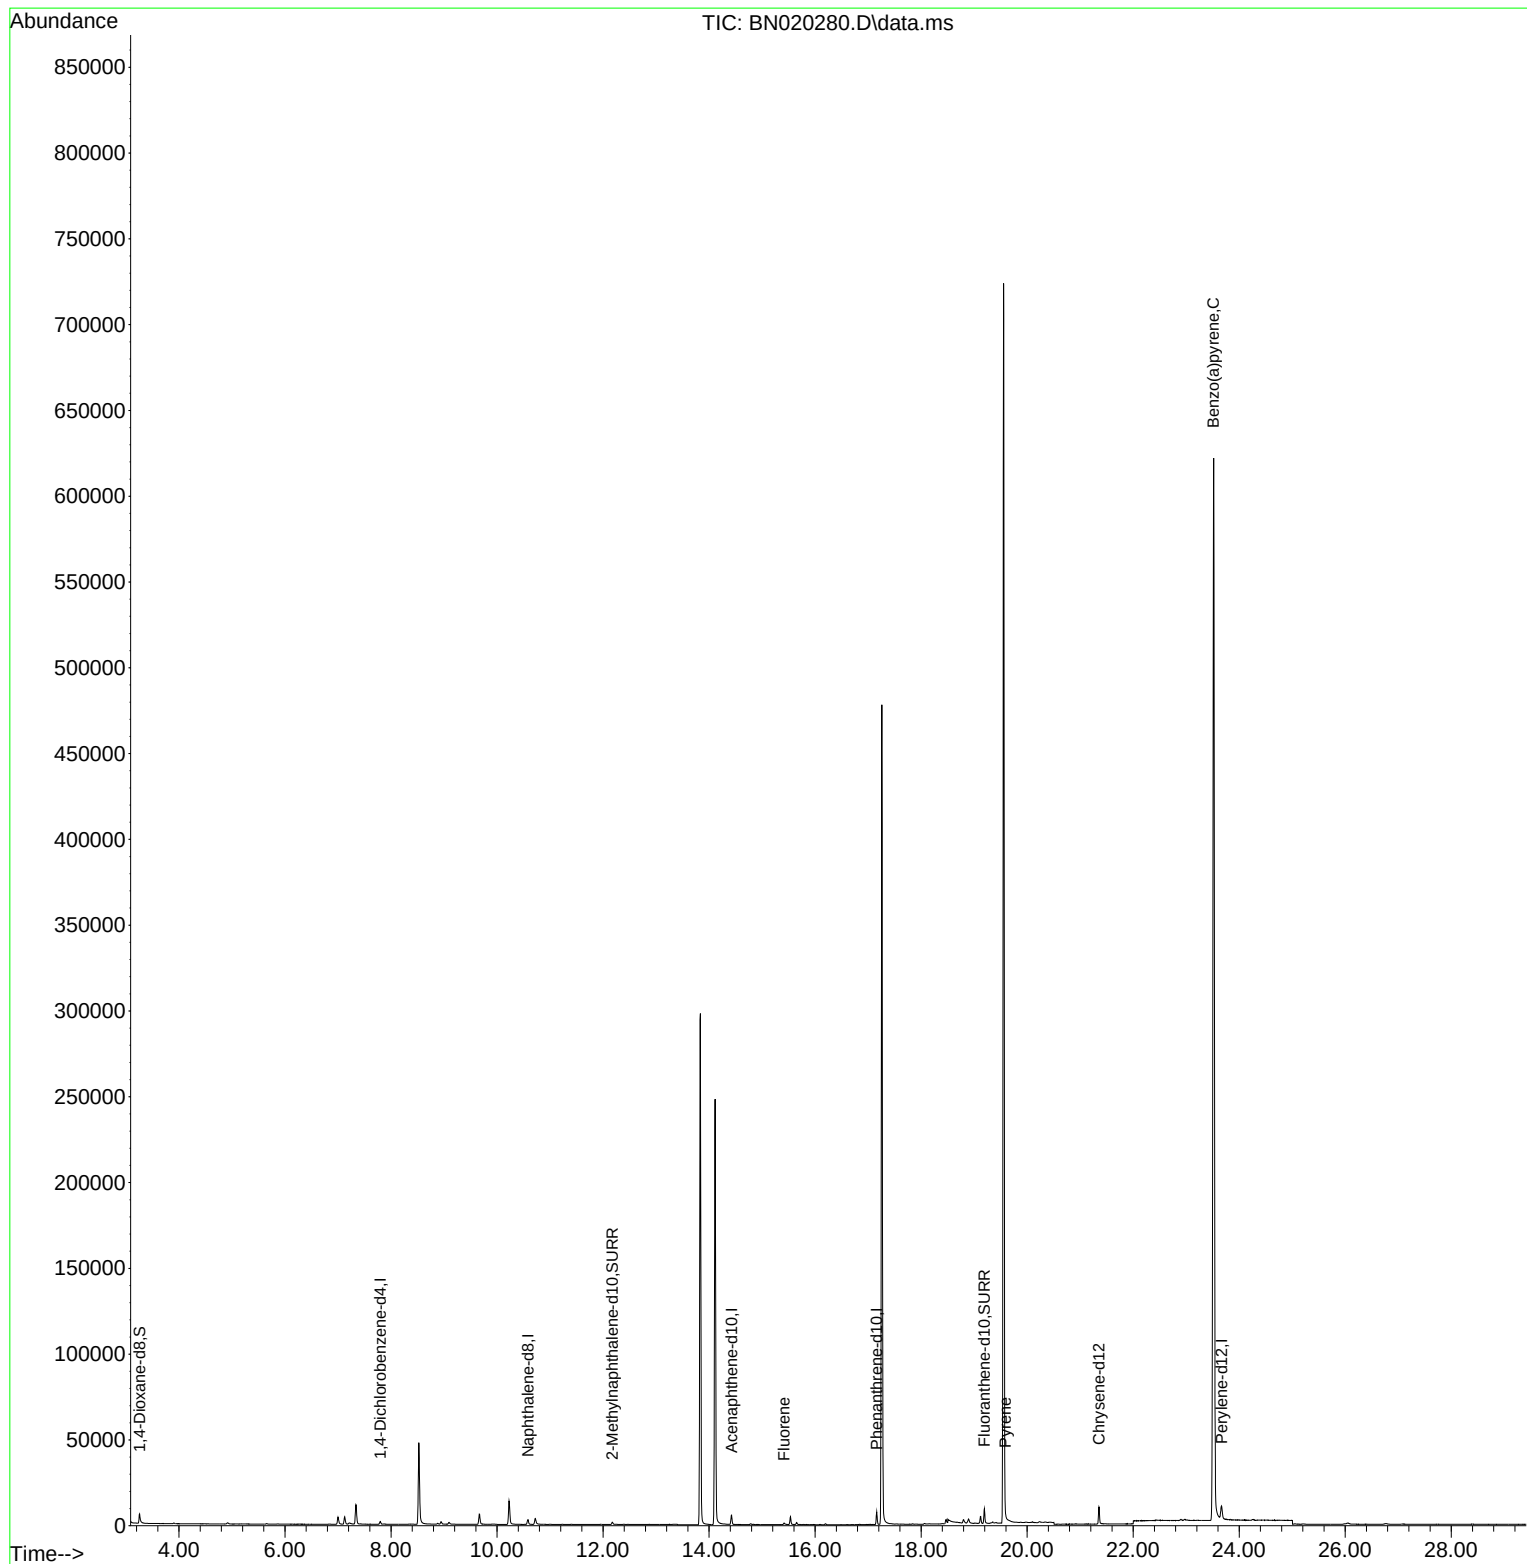


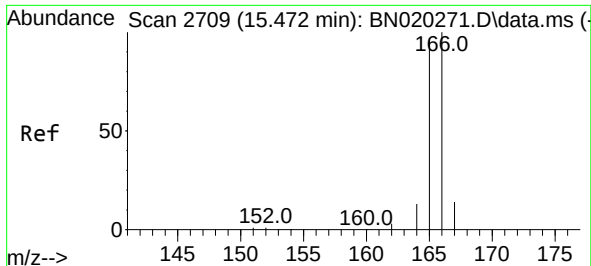

#12
Fluorene
Concen: 0.054 ng/ul
RT: 15.413 min Scan# 2696
Delta R.T. -0.060 min
Lab File: BN020280.D
Acq: 20 Jun 2022 16:04




Instrument :
BNA_N
ClientSampleId :
EW4Q2


Tgt Ion:166 Resp: 815
Ion Ratio Lower Upper
166 100
165 16.8 78.2 117.4#
167 38.5 12.1 18.1#

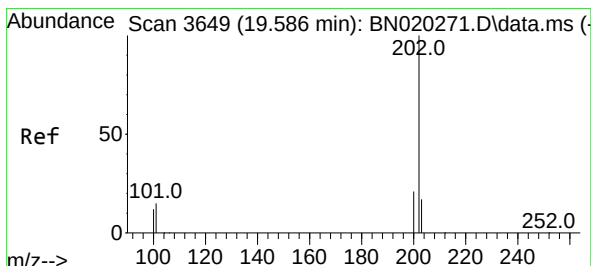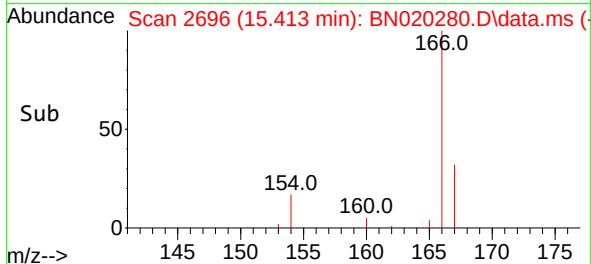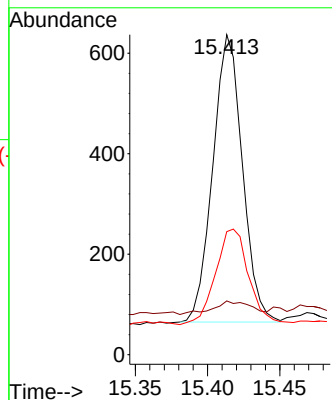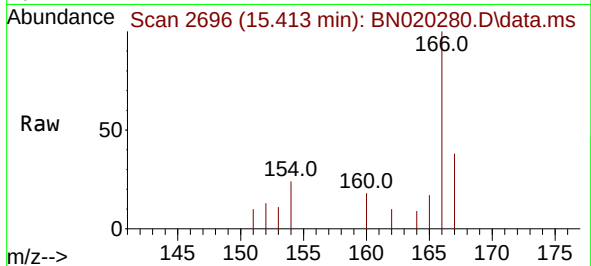

#20
Pyrene
Concen: 0.027 ng/ul
RT: 19.587 min Scan# 3649
Delta R.T. 0.005 min
Lab File: BN020280.D
Acq: 20 Jun 2022 16:04


Tgt Ion:202 Resp: 1172
Ion Ratio Lower Upper
202 100
101 318.5 12.6 19.0#
100 48.7 10.3 15.5#

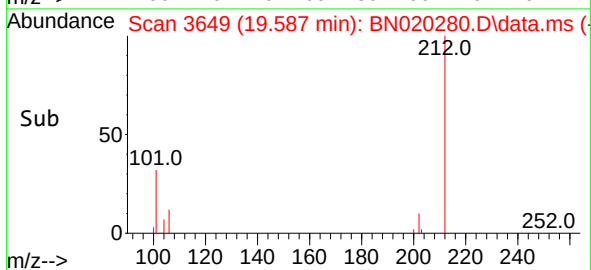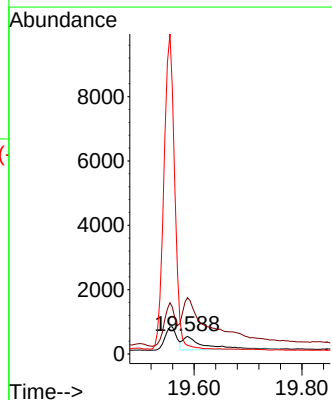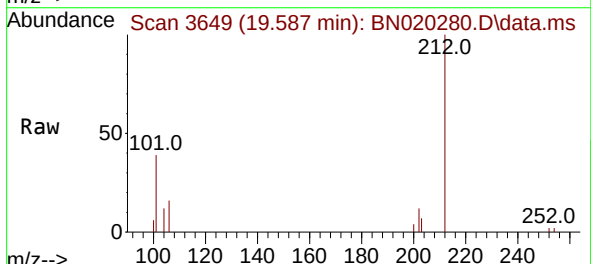

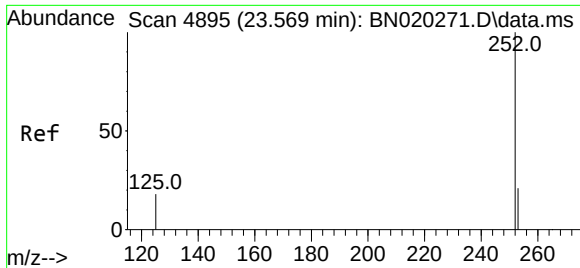

#26
 Benzo(a)pyrene
 Concen: 0.059 ng/ul
 RT: 23.515 min Scan# 41
 Delta R.T. -0.048 min
 Lab File: BN020280.D
 Acq: 20 Jun 2022 16:04

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q2

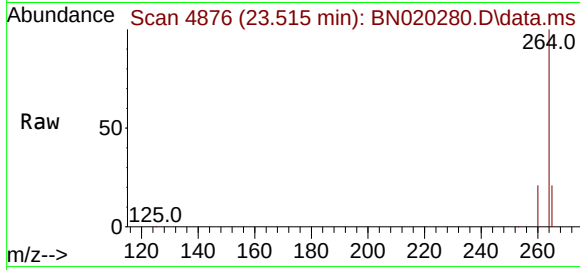

Tgt Ion:252 Resp: 3138
 Ion Ratio Lower Upper
 252 100
 253 55.0 21.7 32.5#
 125 46.5 18.6 28.0#

