

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020281.D
 Acq On : 20 Jun 2022 16:40
 Operator : CG/JU
 Sample : N3294-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P8

Quant Time: Jun 21 02:38:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	802	0.400	ng/ul	0.00
4) Naphthalene-d8	10.584	136	3341	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.424	164	2757	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.163	188	7234	0.400	ng/ul	0.00
17) Chrysene-d12	21.354	240	8542	0.400	ng/ul	0.00
23) Perylene-d12	23.660	264	11115	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	3764	4.110	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.173	152	1907	0.345	ng/ul	0.00
18) Fluoranthene-d10	19.193	212	8375	0.475	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.556	202	1260	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.511	252	3372	0.067	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020281.D
Acq On : 20 Jun 2022 16:40
Operator : CG/JU
Sample : N3294-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P8

Quant Time: Jun 21 02:38:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




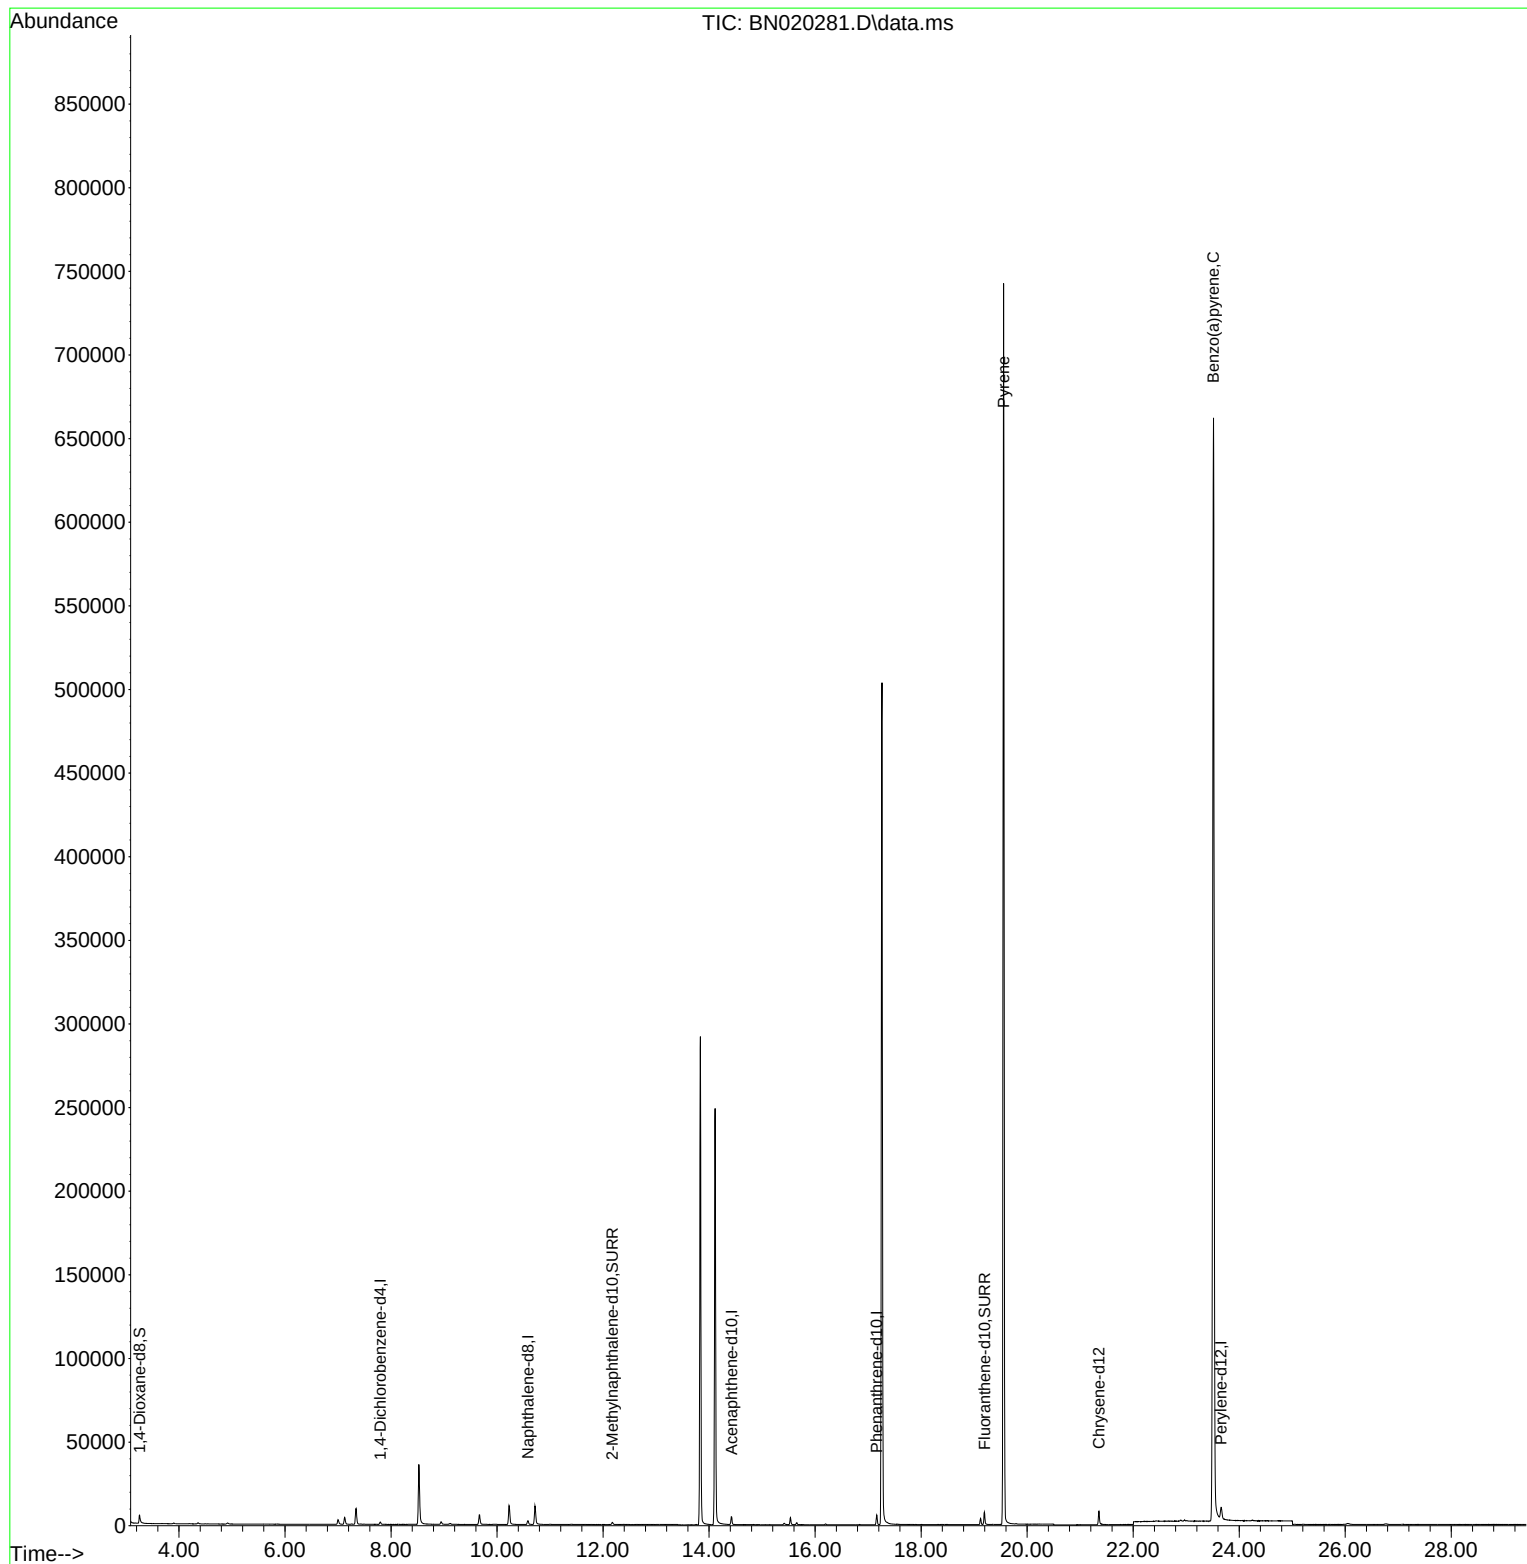


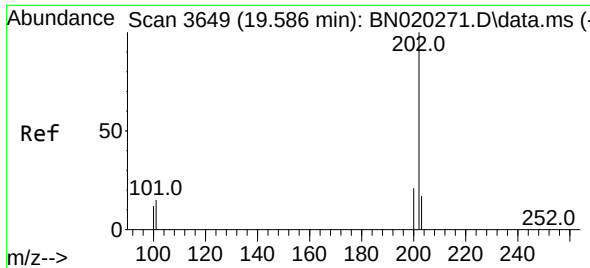

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.556 min Scan# 30
Delta R.T. -0.027 min
Lab File: BN020281.D
Acq: 20 Jun 2022 16:40

Instrument :
BNA_N
ClientSampleId :
EW4P8

Tgt Ion:202 Resp: 1260
Ion Ratio Lower Upper
202 100
101 166.5 12.6 19.0#
100 1164.2 10.3 15.5#

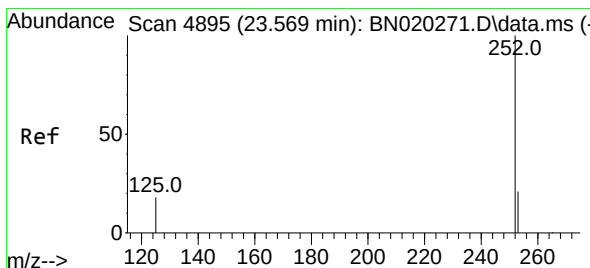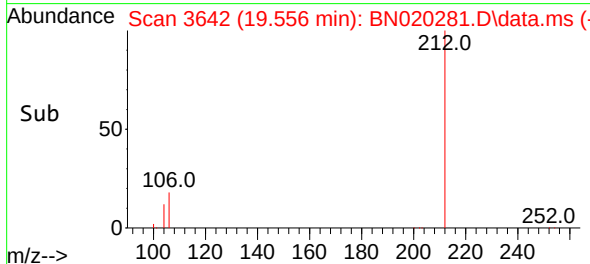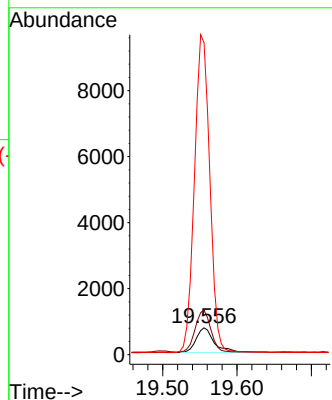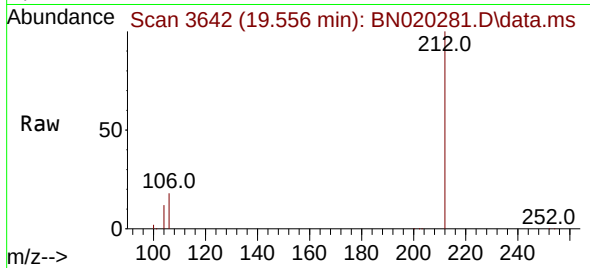

#26
Benzo(a)pyrene
Concen: 0.067 ng/ul
RT: 23.511 min Scan# 4875
Delta R.T. -0.052 min
Lab File: BN020281.D
Acq: 20 Jun 2022 16:40

Tgt Ion:252 Resp: 3372
Ion Ratio Lower Upper
252 100
253 49.9 21.7 32.5#
125 42.2 18.6 28.0#

