

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020282.D
 Acq On : 20 Jun 2022 17:16
 Operator : CG/JU
 Sample : N3294-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q7

Quant Time: Jun 21 02:38:17 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	864	0.400	ng/ul	0.00
4) Naphthalene-d8	10.584	136	3408	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.424	164	2759	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.163	188	7355	0.400	ng/ul	0.00
17) Chrysene-d12	21.354	240	8815	0.400	ng/ul	0.00
23) Perylene-d12	23.660	264	11719	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	3730	3.781	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.179	152	1940	0.344	ng/ul	0.00
18) Fluoranthene-d10	19.193	212	8997	0.494	ng/ul	0.00
Target Compounds						
					Qvalue	
14) Pentachlorophenol	16.834	266	37	0.026	ng/ul#	86
20) Pyrene	19.556	202	1310	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.514	252	3545	0.067	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020282.D
Acq On : 20 Jun 2022 17:16
Operator : CG/JU
Sample : N3294-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q7

Quant Time: Jun 21 02:38:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




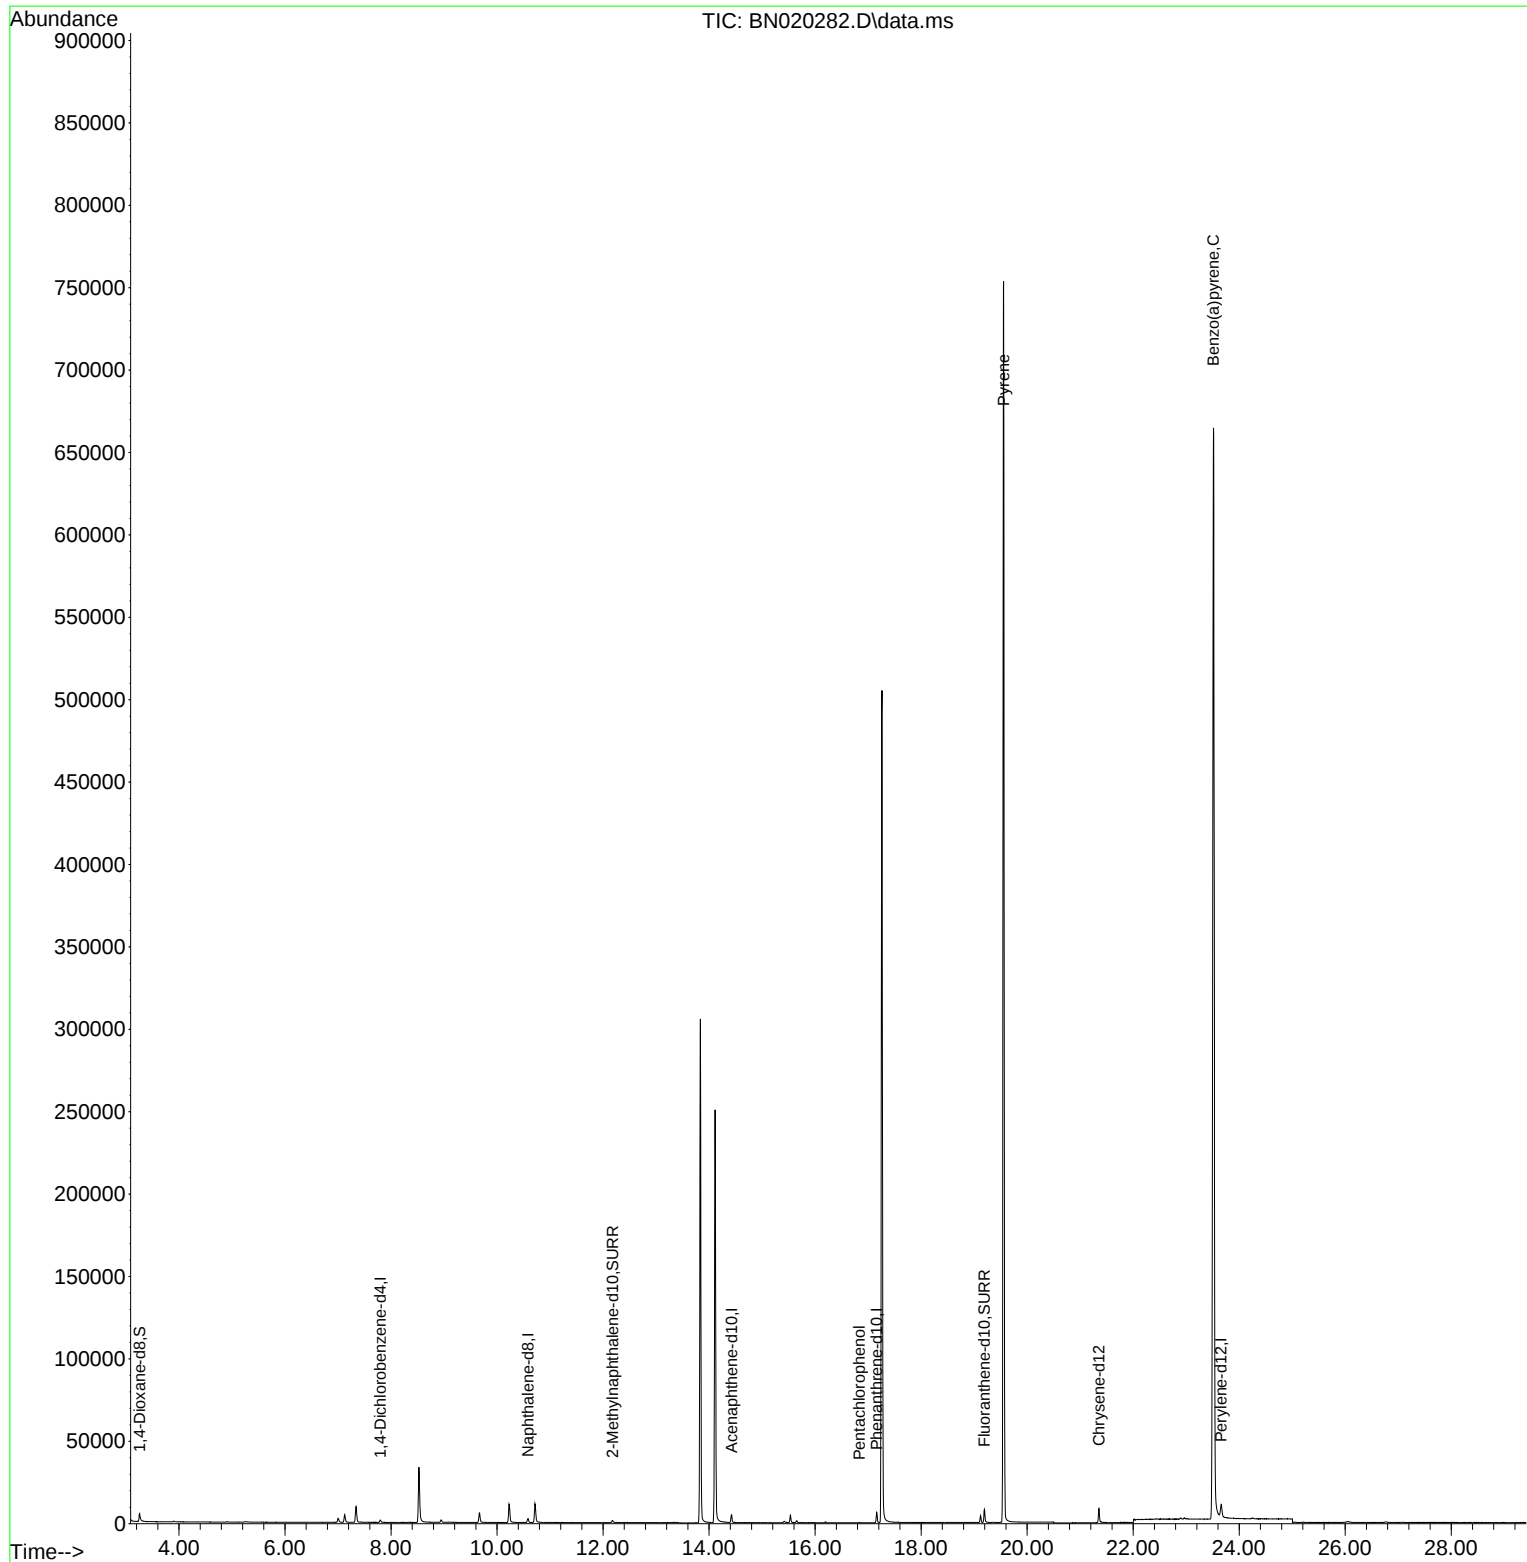


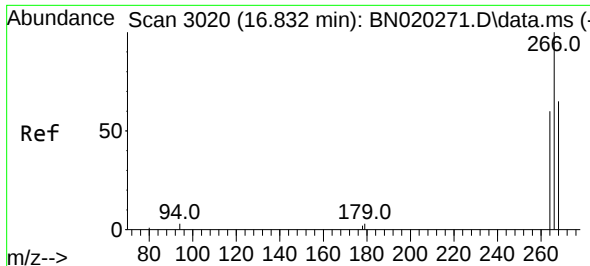

#14
Pentachlorophenol
Concen: 0.026 ng/ul
RT: 16.834 min Scan# 3020
Delta R.T. -0.003 min
Lab File: BN020282.D
Acq: 20 Jun 2022 17:16




Instrument :
BNA_N
ClientSampleId :
EW4Q7


Tgt Ion:266 Resp: 37
Ion Ratio Lower Upper
266 100
264 40.5 49.8 74.8#
268 64.9 51.8 77.6

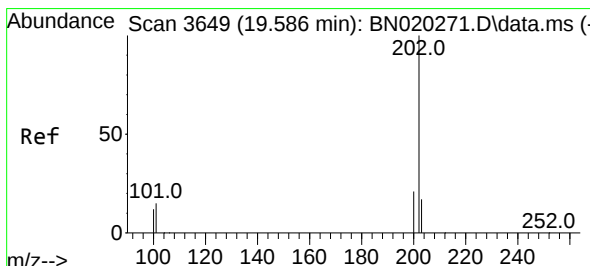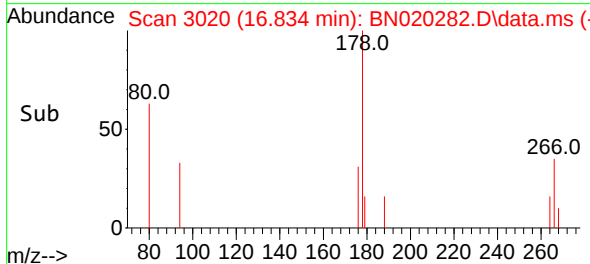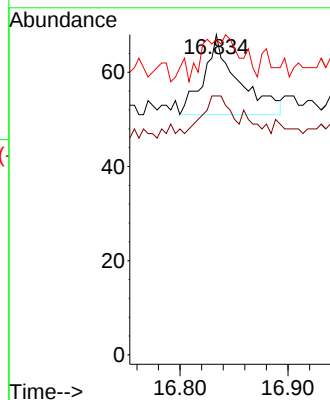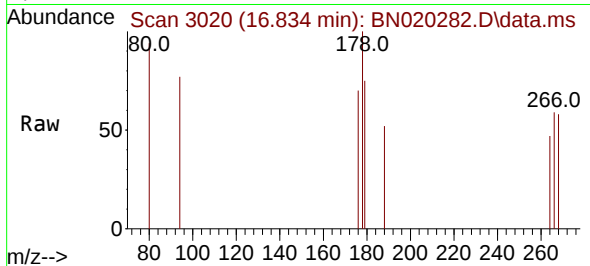

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.556 min Scan# 3642
Delta R.T. -0.027 min
Lab File: BN020282.D
Acq: 20 Jun 2022 17:16

Tgt Ion:202 Resp: 1310
Ion Ratio Lower Upper
202 100
101 163.4 12.6 19.0#
100 1141.1 10.3 15.5#

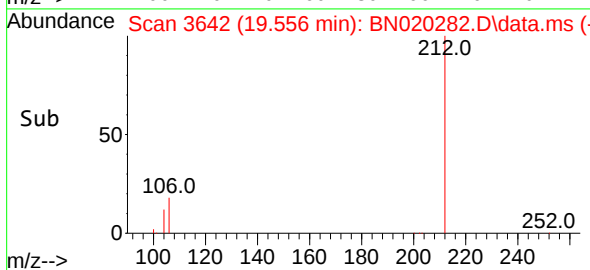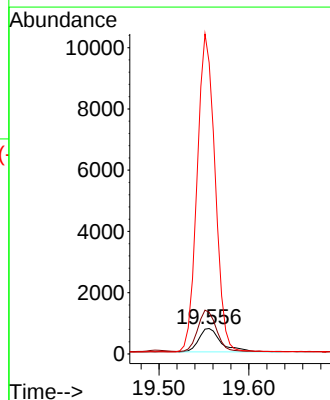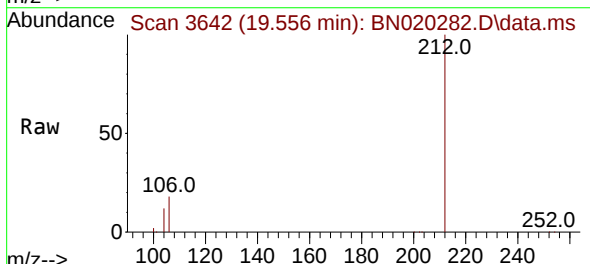

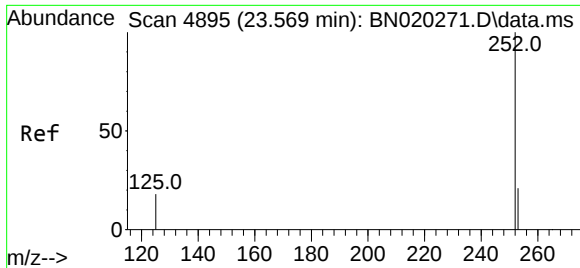

#26

Benzo(a)pyrene

Concen: 0.067 ng/ul

RT: 23.514 min Scan# 4876

Delta R.T. -0.049 min

Lab File: BN020282.D


Acq: 20 Jun 2022 17:16

Instrument :

BNA_N

ClientSampleId :

EW4Q7

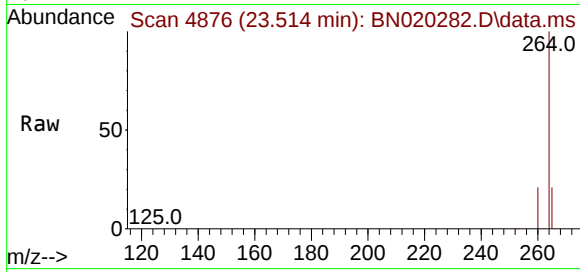

Tgt Ion:252 Resp: 3545

Ion Ratio Lower Upper

252 100

253 51.5 21.7 32.5#

125 40.9 18.6 28.0#

