

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020288.D
 Acq On : 20 Jun 2022 21:30
 Operator : CG/JU
 Sample : PB145550BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK550

Quant Time: Jun 21 02:38:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	869	0.400	ng/ul	0.00
4) Naphthalene-d8	10.584	136	3325	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.423	164	2540	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.162	188	6602	0.400	ng/ul	0.00
17) Chrysene-d12	21.354	240	8384	0.400	ng/ul	0.00
23) Perylene-d12	23.658	264	11648	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	4780	4.817	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.179	152	1563	0.284	ng/ul	0.00
18) Fluoranthene-d10	19.192	212	6169	0.356	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.413	166	614	0.051	ng/ul#	20
14) Pentachlorophenol	16.837	266	26	0.021	ng/ul#	58
20) Pyrene	19.555	202	986	0.027	ng/ul#	1
26) Benzo(a)pyrene	23.509	252	2949	0.056	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020288.D
Acq On : 20 Jun 2022 21:30
Operator : CG/JU
Sample : PB145550BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK550

Quant Time: Jun 21 02:38:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




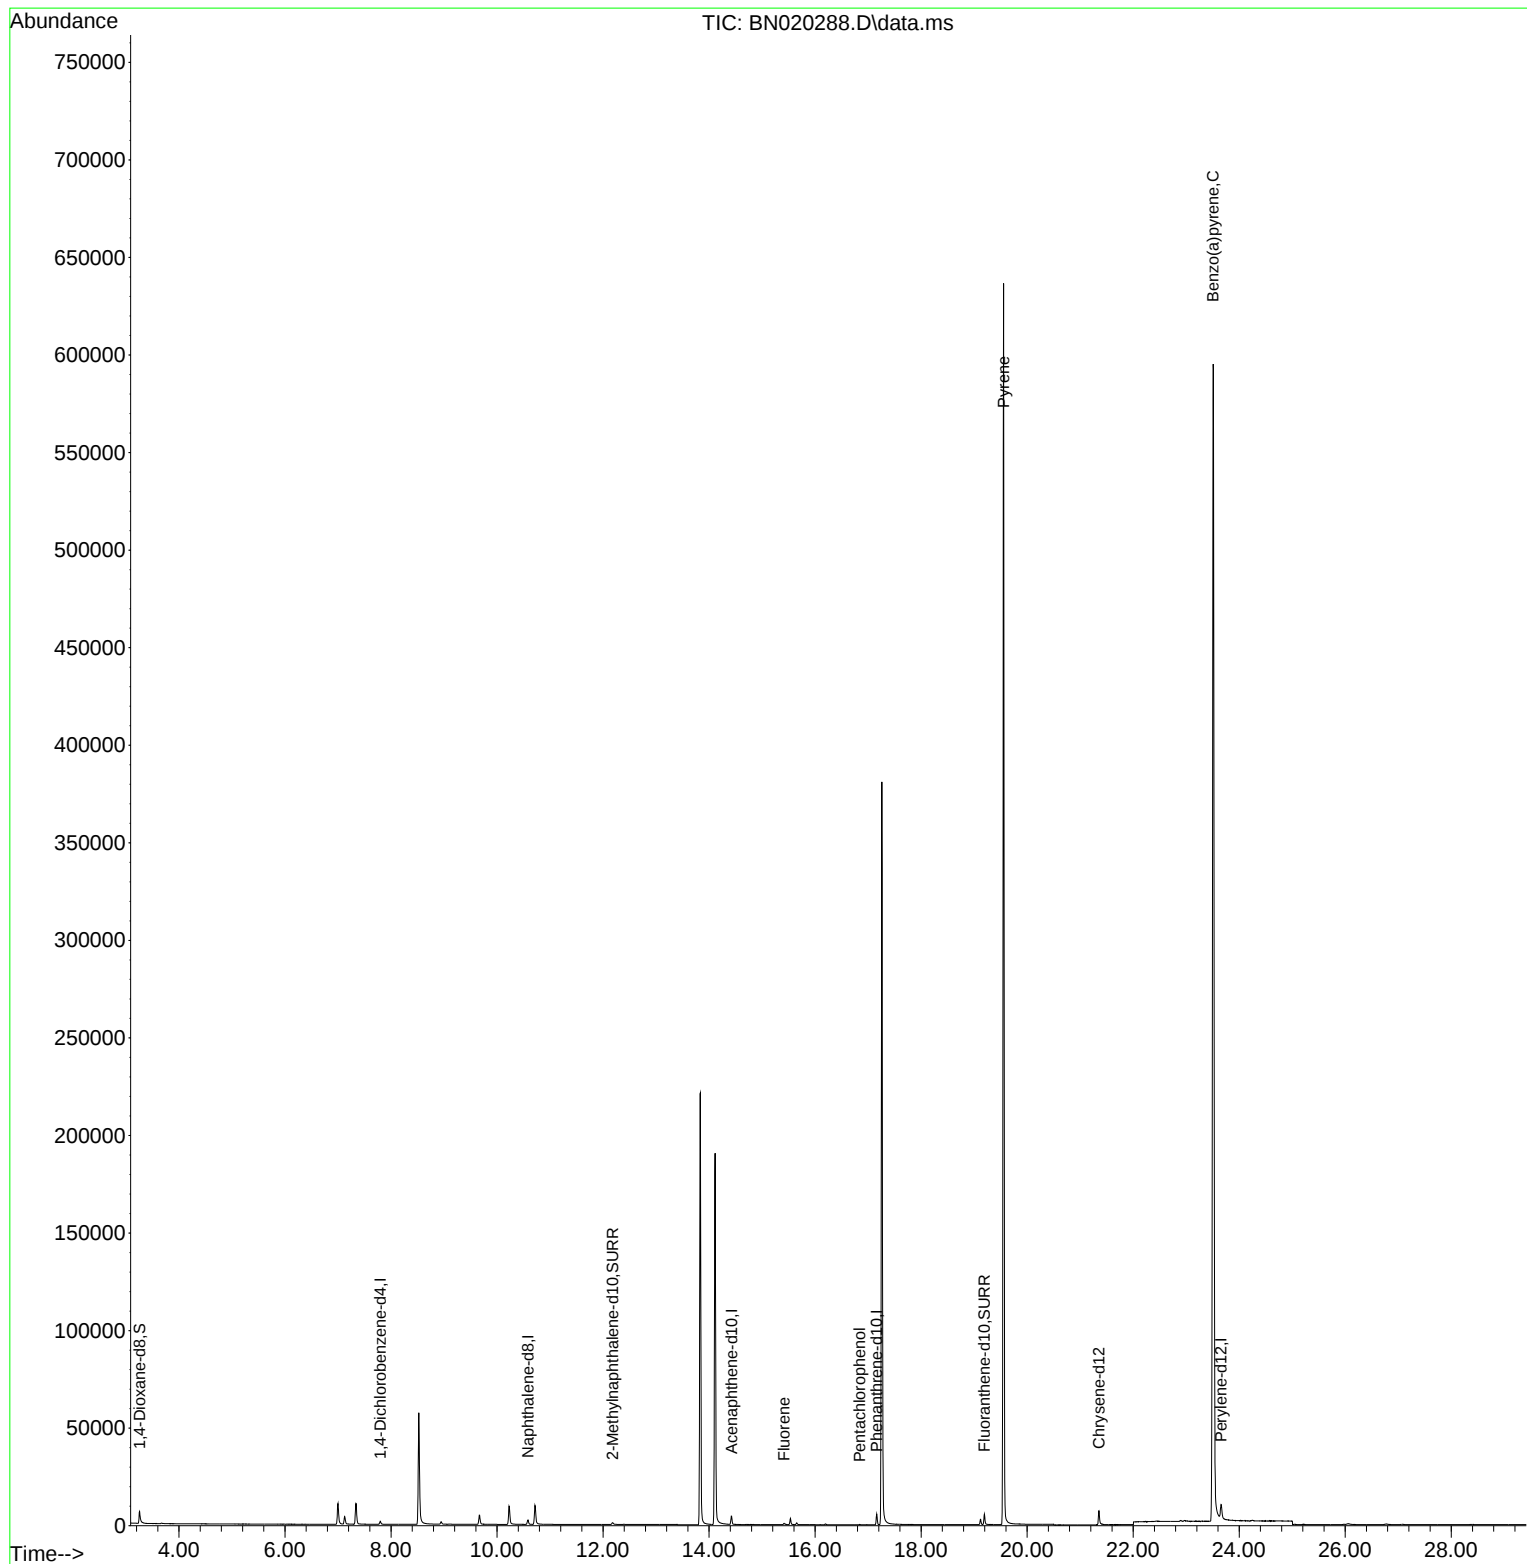


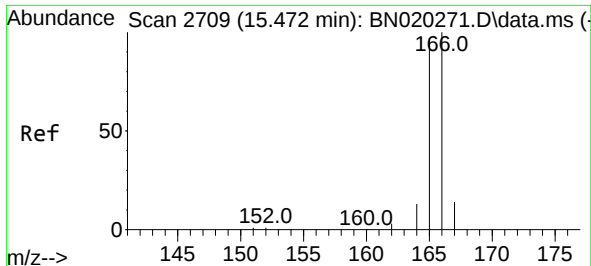

#12
Fluorene
Concen: 0.051 ng/ul
RT: 15.413 min Scan# 2696
Delta R.T. -0.060 min
Lab File: BN020288.D
Acq: 20 Jun 2022 21:30




Instrument :
BNA_N
ClientSampleId :
SBLK550


Tgt Ion:166 Resp: 614
Ion Ratio Lower Upper
166 100
165 16.5 78.2 117.4#
167 41.5 12.1 18.1#

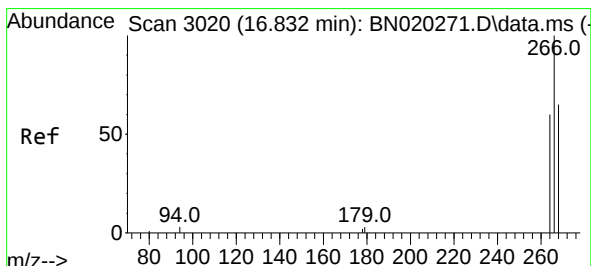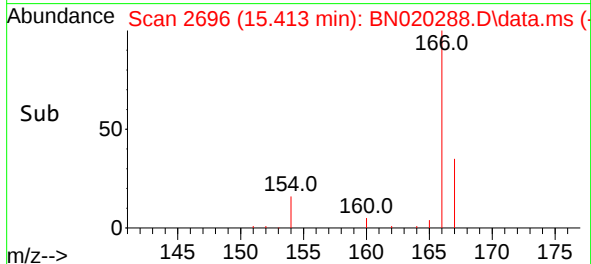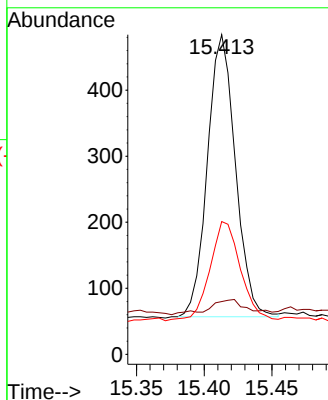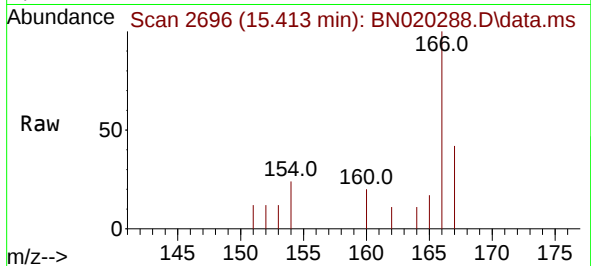

#14
Pentachlorophenol
Concen: 0.021 ng/ul
RT: 16.837 min Scan# 3021
Delta R.T. -0.000 min
Lab File: BN020288.D
Acq: 20 Jun 2022 21:30

Tgt Ion:266 Resp: 26
Ion Ratio Lower Upper
266 100
264 23.1 49.8 74.8#
268 38.5 51.8 77.6#

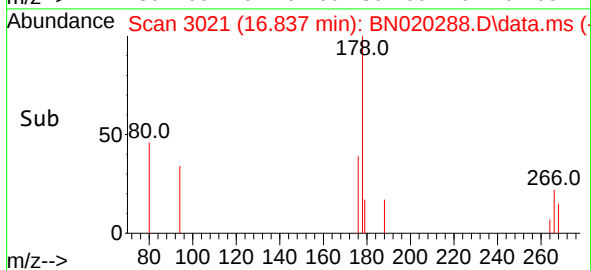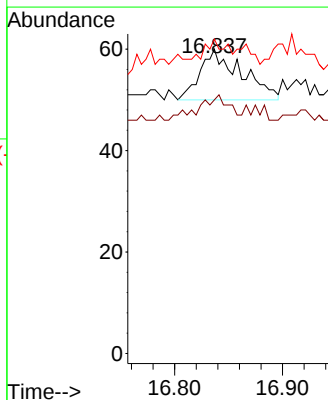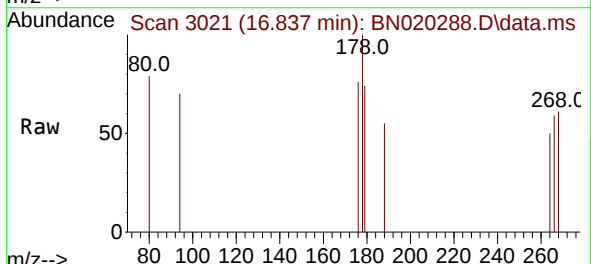

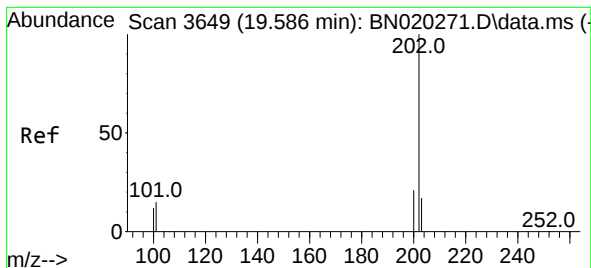

#20

Pyrene

Concen: 0.027 ng/ul

RT: 19.555 min Scan# 3

Delta R.T. -0.028 min

Lab File: BN020288.D

Acq: 20 Jun 2022 21:30

Instrument :





BNA_N

ClientSampleId :

SBLK550

Tgt Ion:202 Resp: 986

Ion	Ratio	Lower	Upper
202	100		
101	169.2	12.6	19.0#
100	1181.1	10.3	15.5#

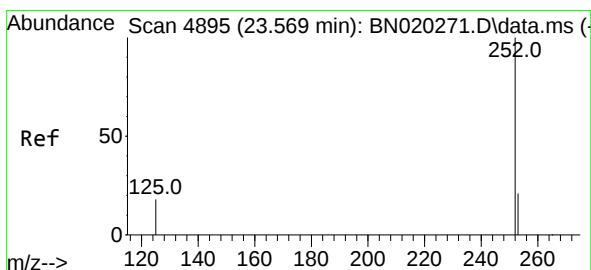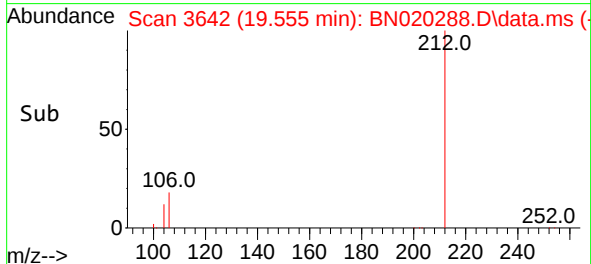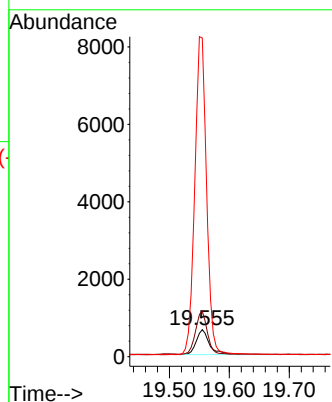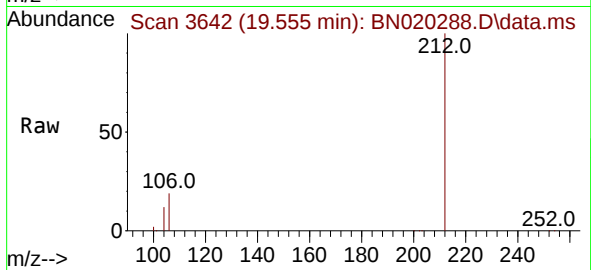

#26

Benzo(a)pyrene

Concen: 0.056 ng/ul

RT: 23.509 min Scan# 4874

Delta R.T. -0.054 min

Lab File: BN020288.D

Acq: 20 Jun 2022 21:30

Tgt Ion:252 Resp: 2949

Ion	Ratio	Lower	Upper
252	100		
253	48.6	21.7	32.5#
125	39.6	18.6	28.0#

