

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020290.D
 Acq On : 20 Jun 2022 22:42
 Operator : CG/JU
 Sample : N3294-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4R0

Quant Time: Jun 21 02:38:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	996	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	4114	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.418	164	3156	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.162	188	8147	0.400	ng/ul	0.00
17) Chrysene-d12	21.352	240	9588	0.400	ng/ul	0.00
23) Perylene-d12	23.661	264	12127	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	2169	1.907	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.173	152	2231	0.328	ng/ul	0.00
18) Fluoranthene-d10	19.192	212	9452	0.478	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.413	166	929	0.062	ng/ul#	20
14) Pentachlorophenol	16.824	266	34	0.022	ng/ul#	38
20) Pyrene	19.555	202	1320	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.515	252	3618	0.066	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020290.D
Acq On : 20 Jun 2022 22:42
Operator : CG/JU
Sample : N3294-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4R0

Quant Time: Jun 21 02:38:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




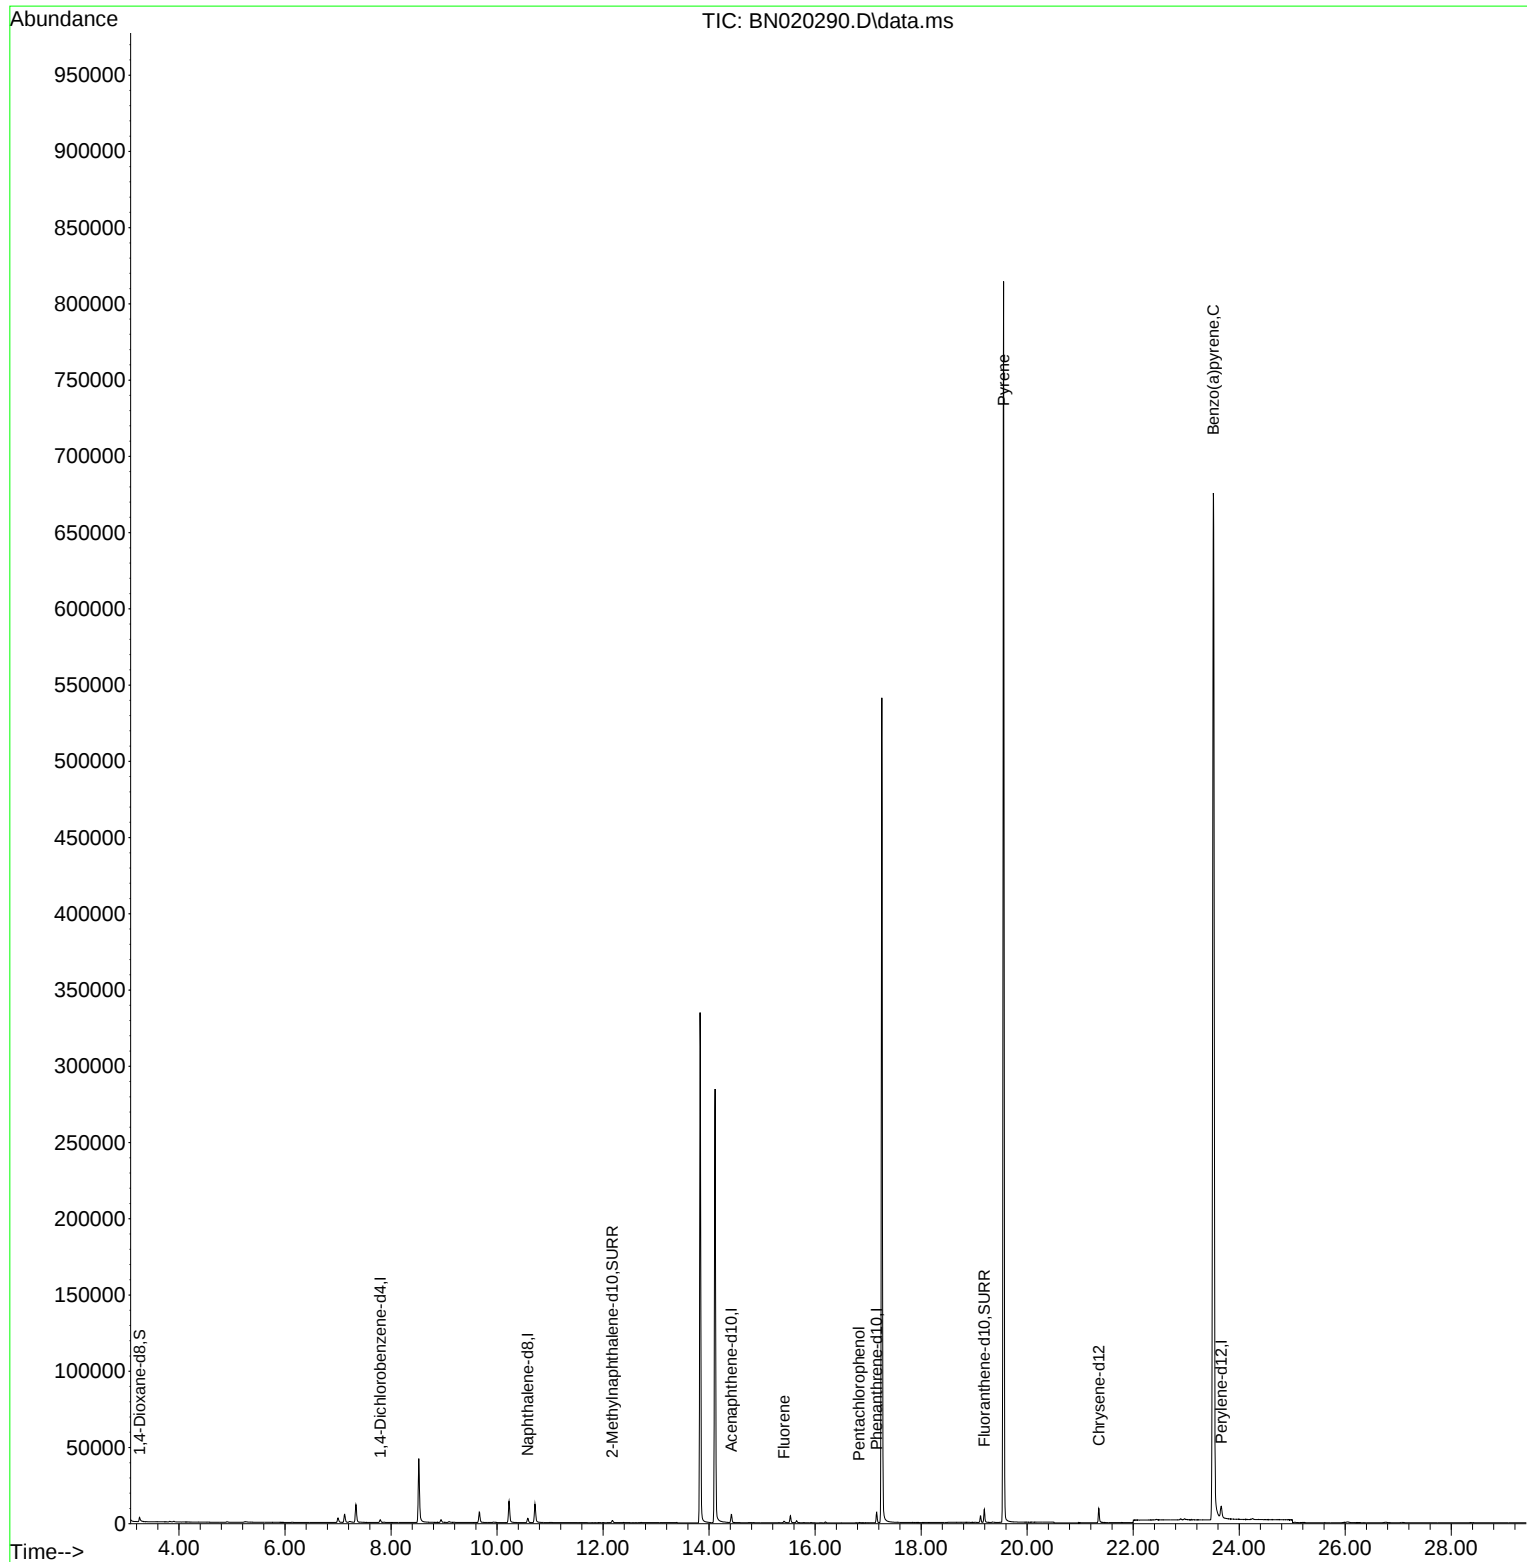


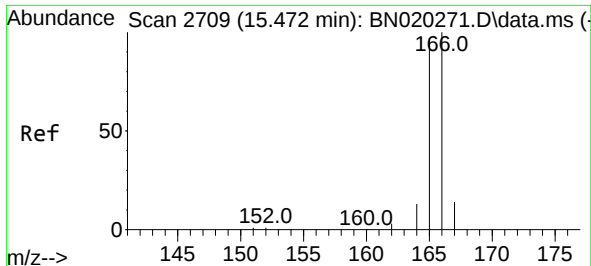

#12
Fluorene
Concen: 0.062 ng/ul
RT: 15.413 min Scan# 2696
Delta R.T. -0.060 min
Lab File: BN020290.D
Acq: 20 Jun 2022 22:42




Instrument :
BNA_N
ClientSampleId :
EW4R0


Tgt Ion:166 Resp: 929
Ion Ratio Lower Upper
166 100
165 15.7 78.2 117.4#
167 38.7 12.1 18.1#

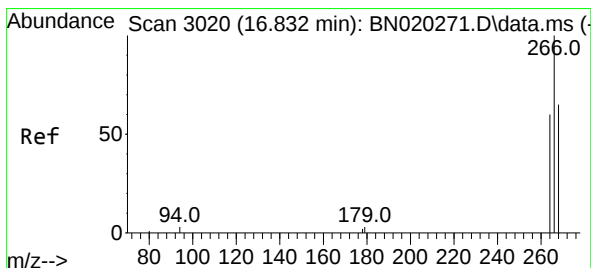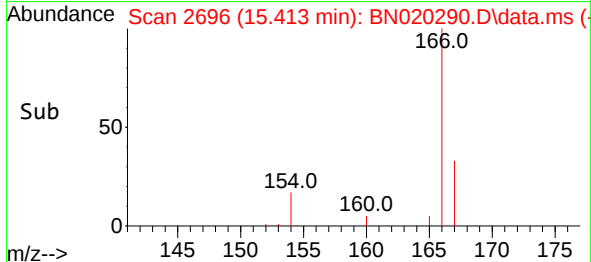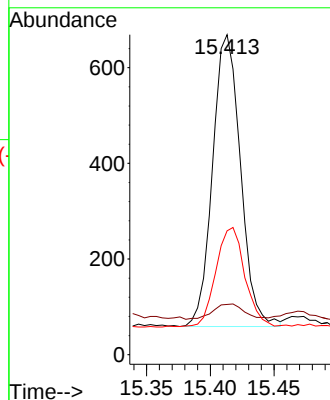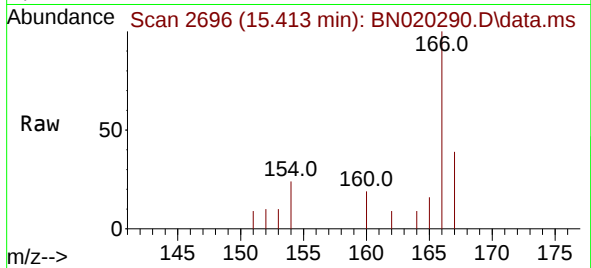

#14
Pentachlorophenol
Concen: 0.022 ng/ul
RT: 16.824 min Scan# 3018
Delta R.T. -0.013 min
Lab File: BN020290.D
Acq: 20 Jun 2022 22:42

Tgt Ion:266 Resp: 34
Ion Ratio Lower Upper
266 100
264 0.0 49.8 74.8#
268 29.4 51.8 77.6#


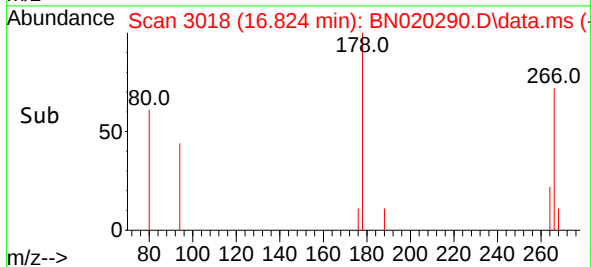
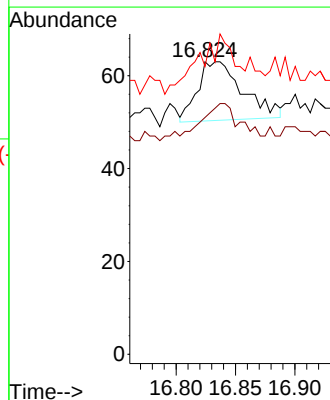
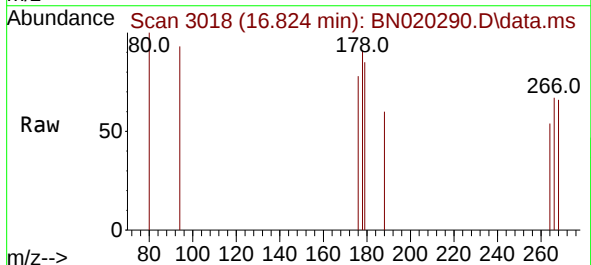


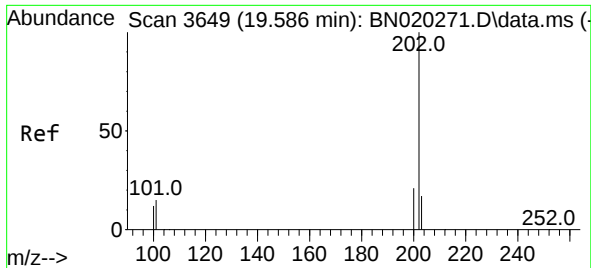

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.555 min Scan# 3642
Delta R.T. -0.028 min
Lab File: BN020290.D
Acq: 20 Jun 2022 22:42

Instrument :
BNA_N
ClientSampleId :
EW4R0

Tgt Ion:202 Resp: 1320
Ion Ratio Lower Upper
202 100
101 163.9 12.6 19.0#
100 1169.7 10.3 15.5#

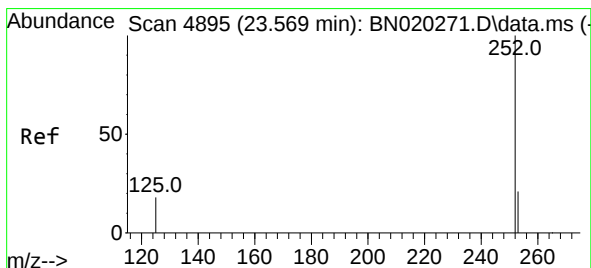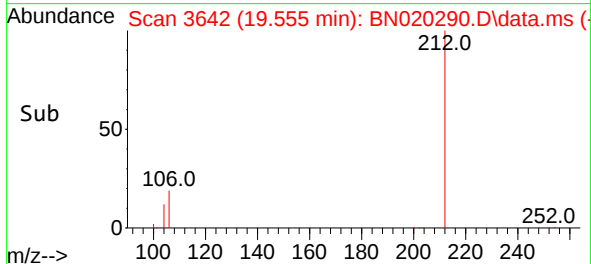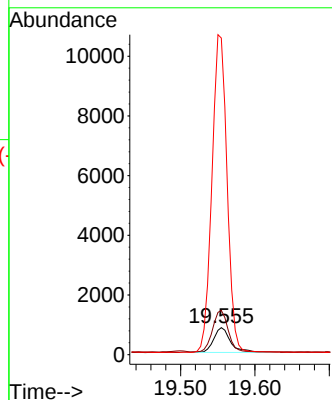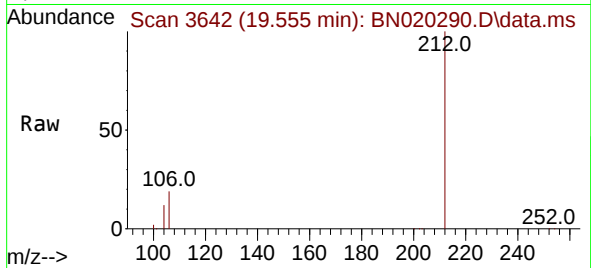

#26
Benzo(a)pyrene
Concen: 0.066 ng/ul
RT: 23.515 min Scan# 4876
Delta R.T. -0.048 min
Lab File: BN020290.D
Acq: 20 Jun 2022 22:42

Tgt Ion:252 Resp: 3618
Ion Ratio Lower Upper
252 100
253 51.9 21.7 32.5#
125 40.2 18.6 28.0#

