

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020292.D
 Acq On : 20 Jun 2022 23:54
 Operator : CG/JU
 Sample : N3294-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q9

Quant Time: Jun 21 02:39:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	953	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	4077	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.419	164	3111	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.162	188	7953	0.400	ng/ul	0.00
17) Chrysene-d12	21.352	240	9441	0.400	ng/ul	0.00
23) Perylene-d12	23.658	264	11716	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	2011	1.848	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.173	152	2263	0.336	ng/ul	0.00
18) Fluoranthene-d10	19.192	212	9789	0.502	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.555	202	1421	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.512	252	3612	0.068	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020292.D
Acq On : 20 Jun 2022 23:54
Operator : CG/JU
Sample : N3294-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q9

Quant Time: Jun 21 02:39:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




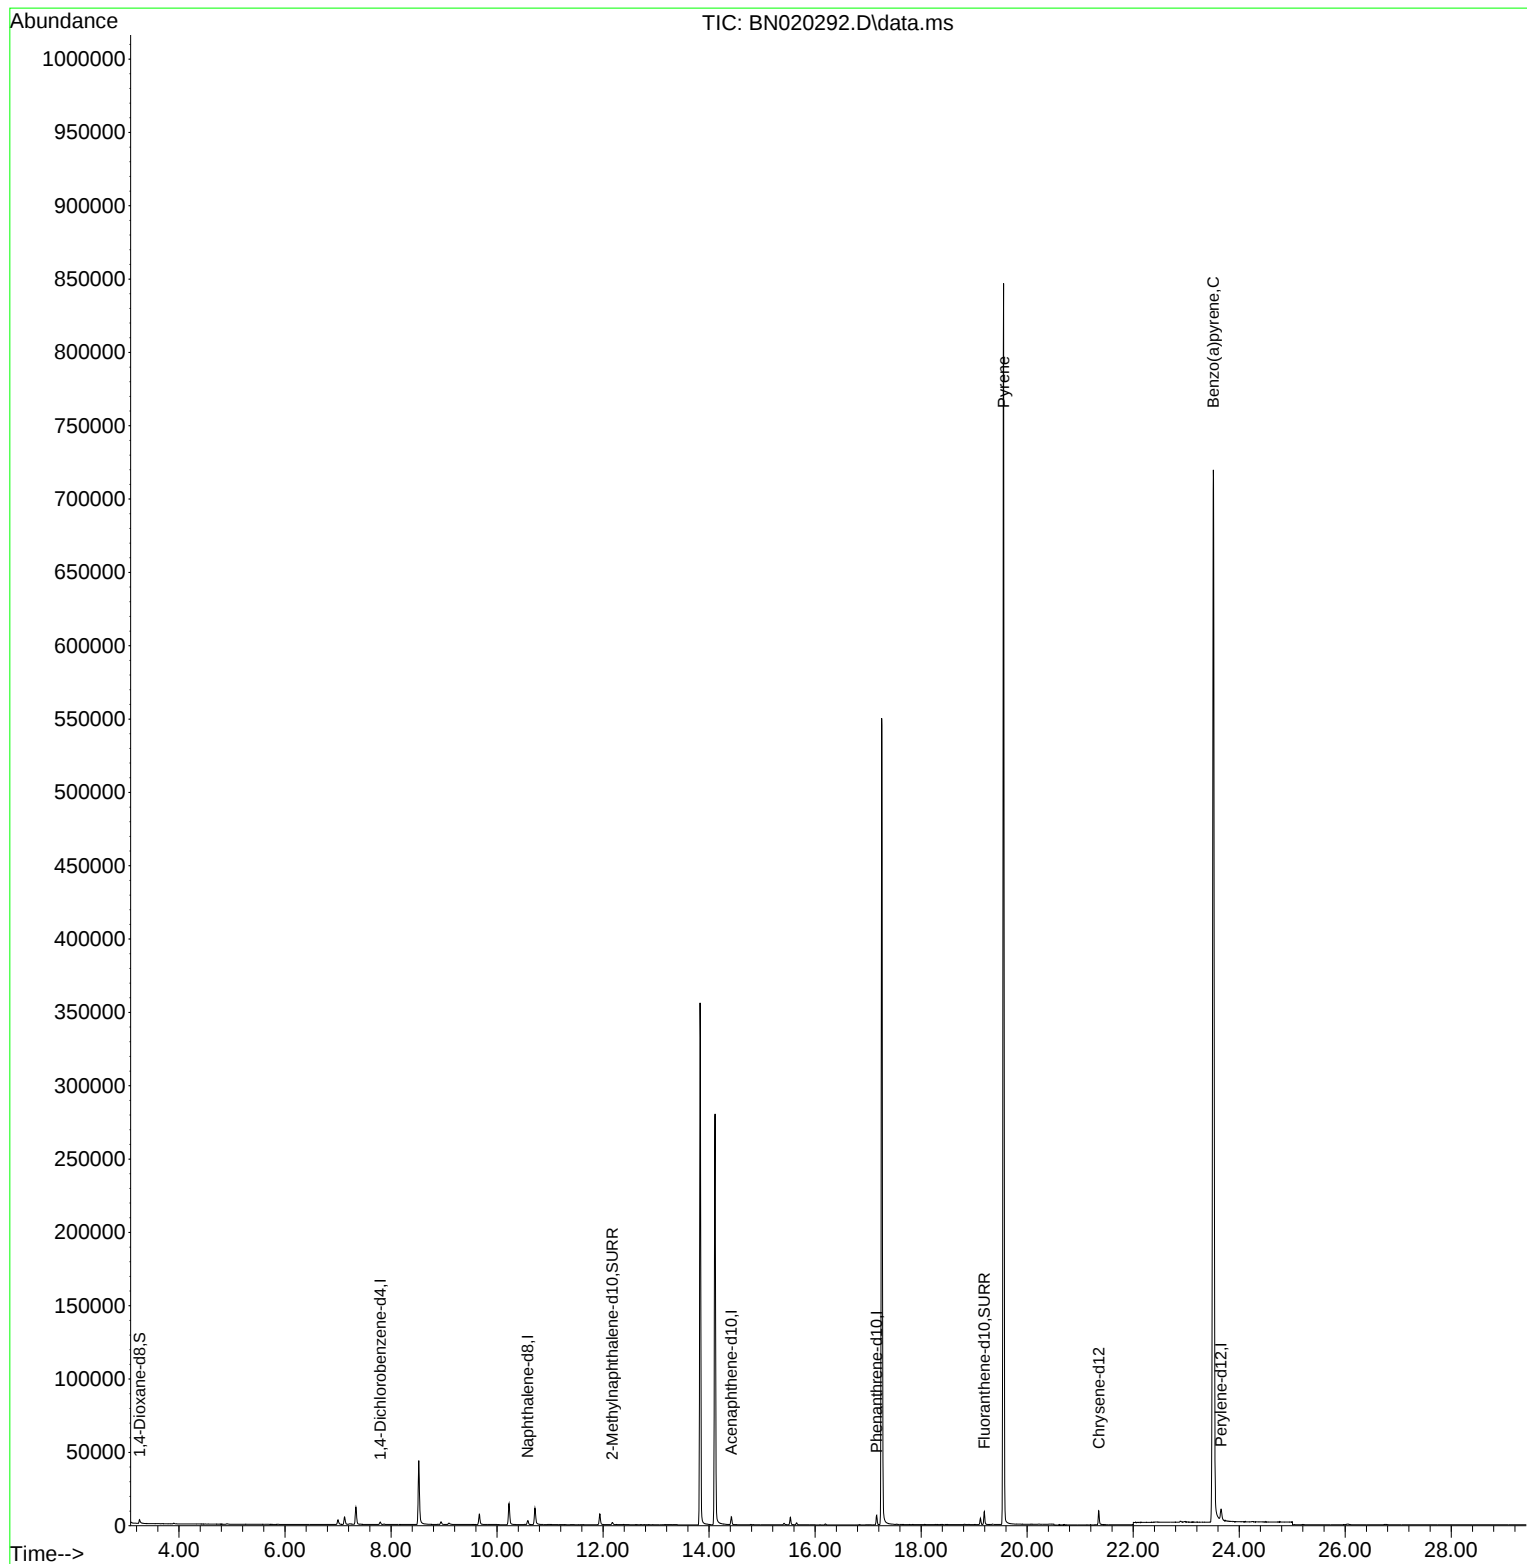


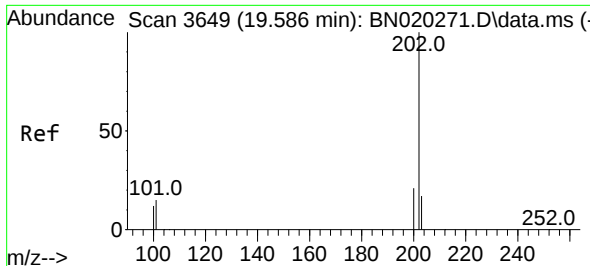

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.555 min Scan# 3642
Delta R.T. -0.028 min
Lab File: BN020292.D
Acq: 20 Jun 2022 23:54

Instrument :
BNA_N
ClientSampleId :
EW4Q9

Tgt Ion:202 Resp: 1421
Ion Ratio Lower Upper
202 100
101 169.7 12.6 19.0#
100 1163.9 10.3 15.5#

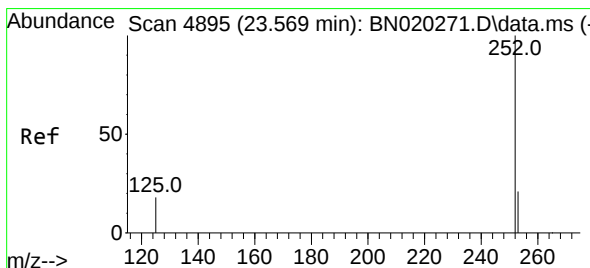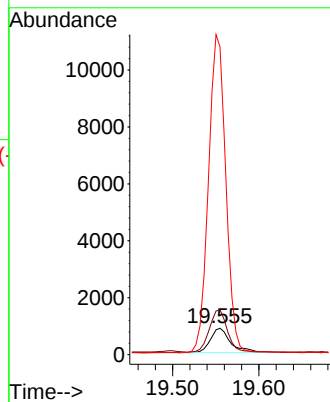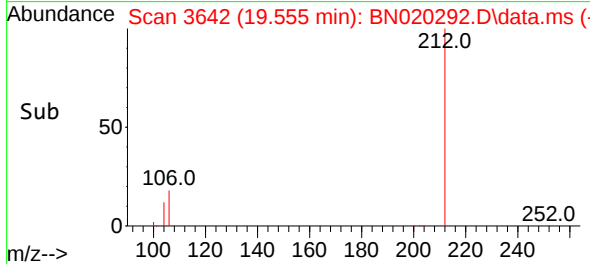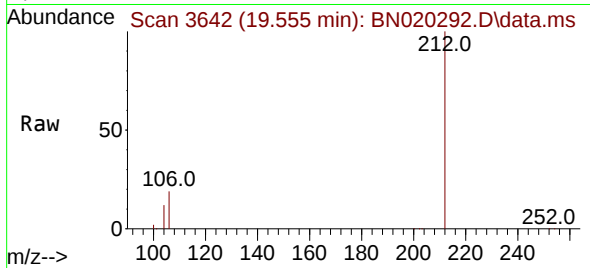

#26
Benzo(a)pyrene
Concen: 0.068 ng/ul
RT: 23.512 min Scan# 4875
Delta R.T. -0.051 min
Lab File: BN020292.D
Acq: 20 Jun 2022 23:54

Tgt Ion:252 Resp: 3612
Ion Ratio Lower Upper
252 100
253 48.5 21.7 32.5#
125 39.2 18.6 28.0#

