

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020293.D
 Acq On : 21 Jun 2022 00:30
 Operator : CG/JU
 Sample : N3294-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4Q8

Quant Time: Jun 21 02:39:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	836	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	4024	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.419	164	2869	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.159	188	7449	0.400	ng/ul	0.00
17) Chrysene-d12	21.351	240	9186	0.400	ng/ul	0.00
23) Perylene-d12	23.660	264	11909	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	2120	2.221	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.173	152	2159	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.189	212	8892	0.469	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.281	88	67	0.073	ng/ul#	80
14) Pentachlorophenol	16.834	266	32	0.022	ng/ul#	67
20) Pyrene	19.551	202	1358	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.511	252	3585	0.067	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020293.D
Acq On : 21 Jun 2022 00:30
Operator : CG/JU
Sample : N3294-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4Q8

Quant Time: Jun 21 02:39:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




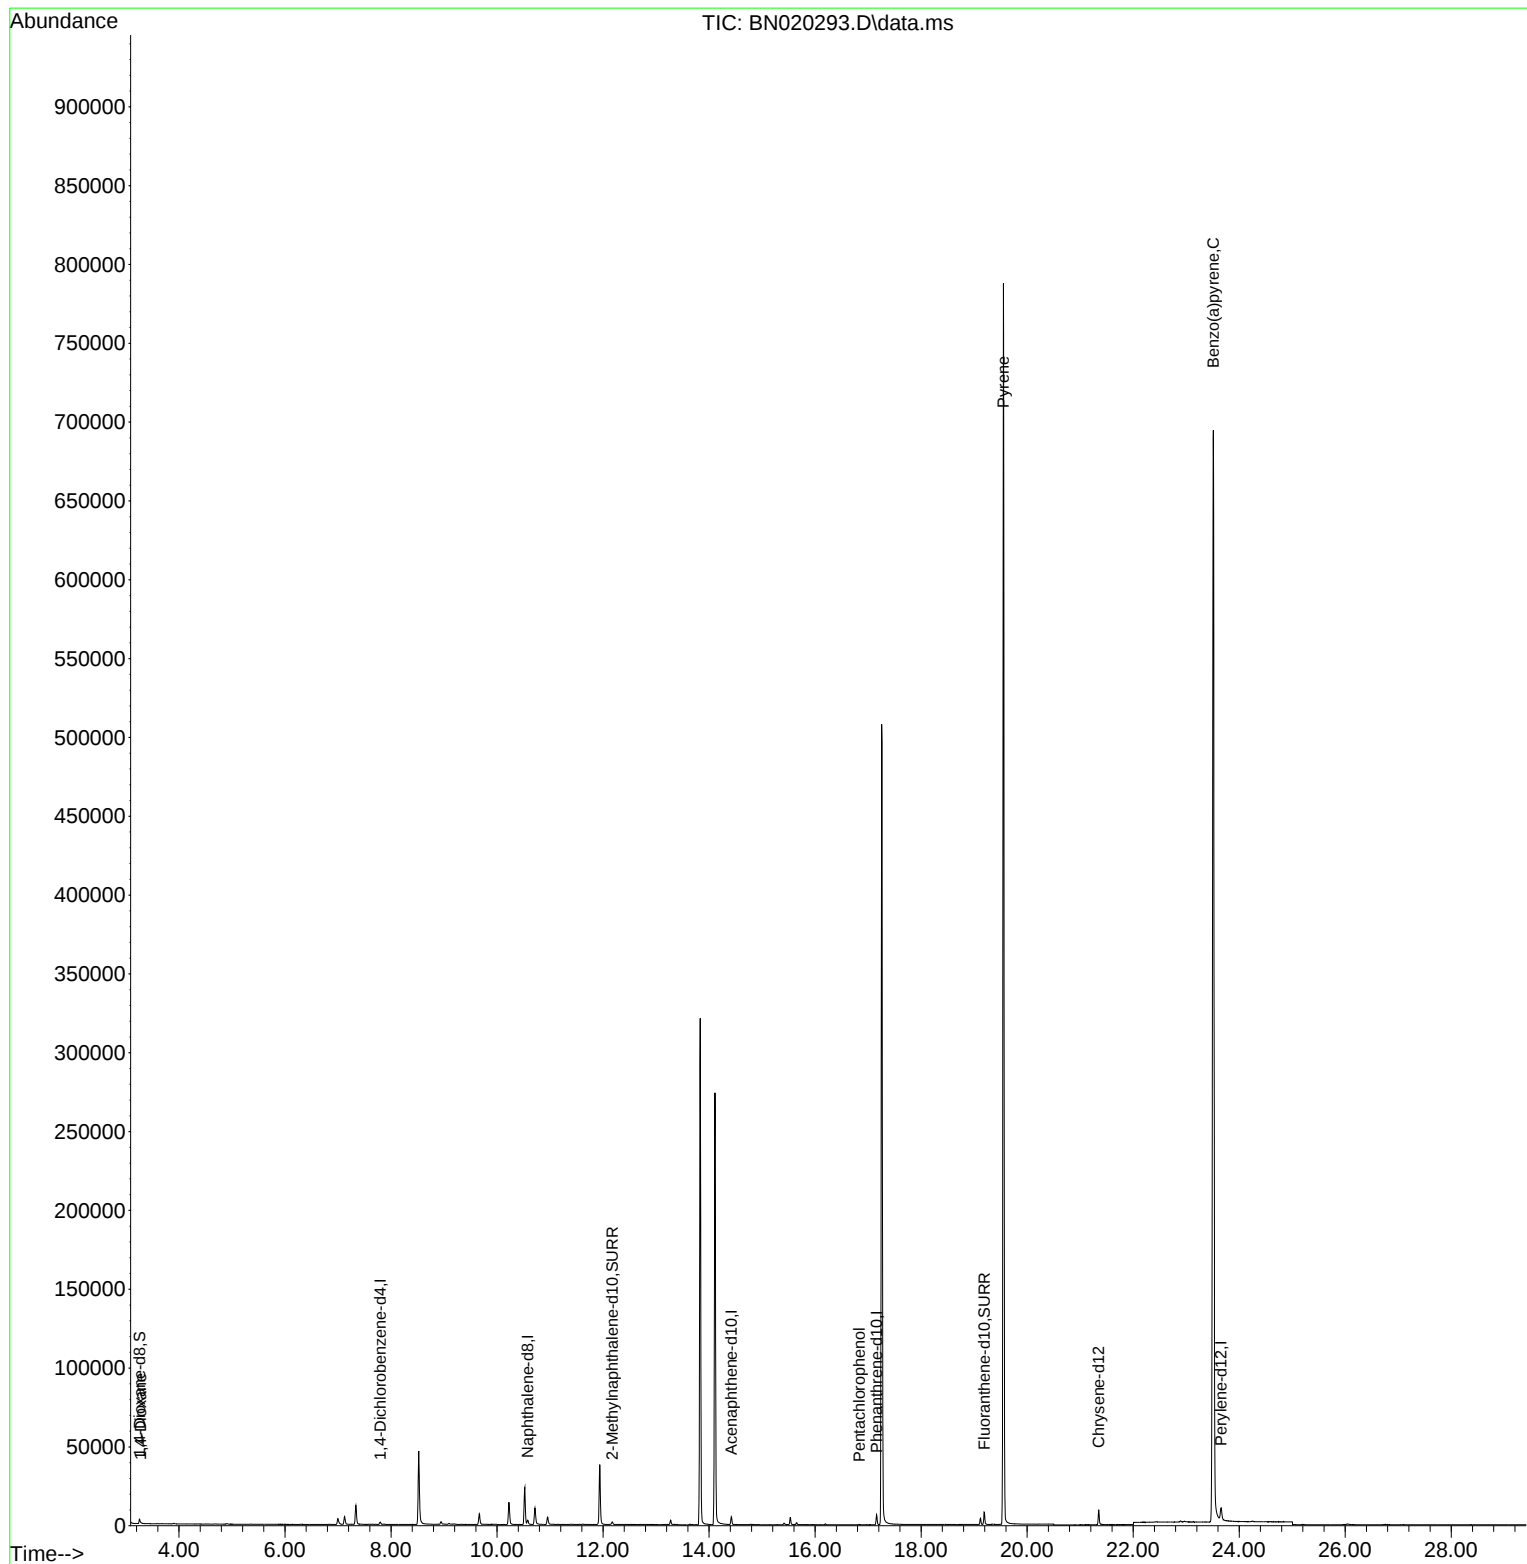


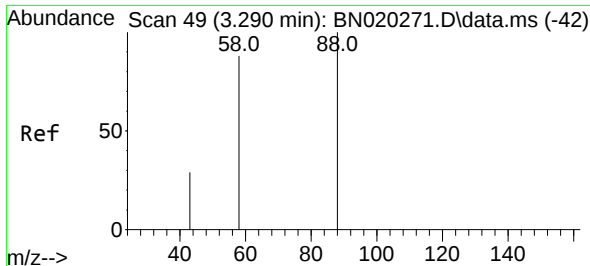

#2
 1,4-Dioxane
 Concen: 0.073 ng/ul
 RT: 3.281 min Scan# 41
 Delta R.T. -0.013 min
 Lab File: BN020293.D
 Acq: 21 Jun 2022 00:30




Instrument :
 BNA_N
 ClientSampleId :
 EW4Q8


Tgt Ion: 88 Resp: 67
 Ion Ratio Lower Upper
 88 100
 43 50.7 31.6 47.4#
 58 17.7 23.8 35.6#

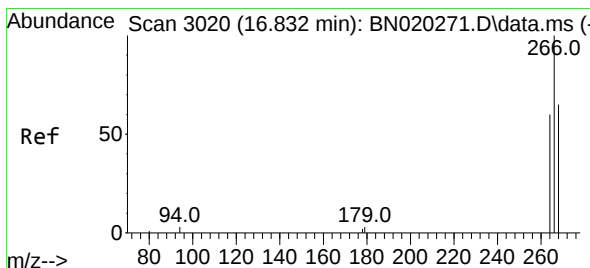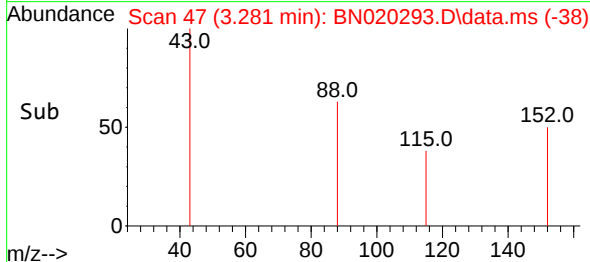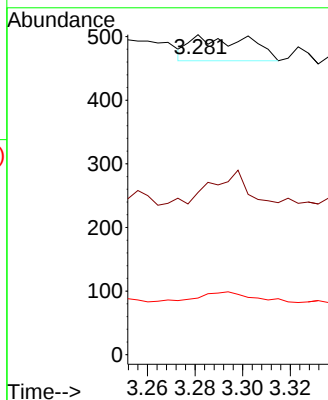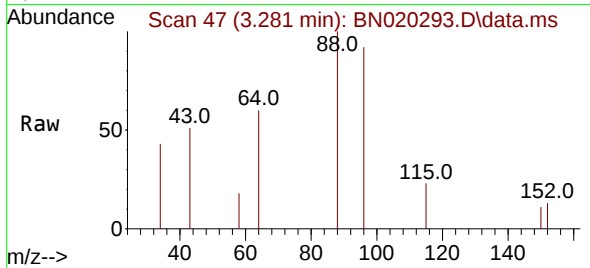

#14
 Pentachlorophenol
 Concen: 0.022 ng/ul
 RT: 16.834 min Scan# 3020
 Delta R.T. -0.003 min
 Lab File: BN020293.D
 Acq: 21 Jun 2022 00:30

Tgt Ion: 266 Resp: 32
 Ion Ratio Lower Upper
 266 100
 264 40.6 49.8 74.8#
 268 34.4 51.8 77.6#


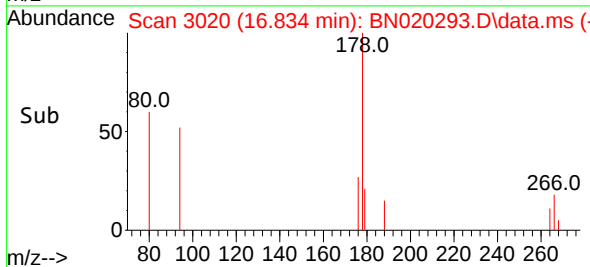
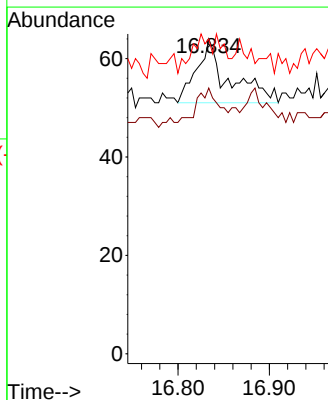
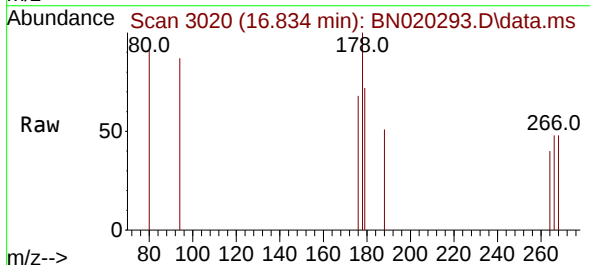


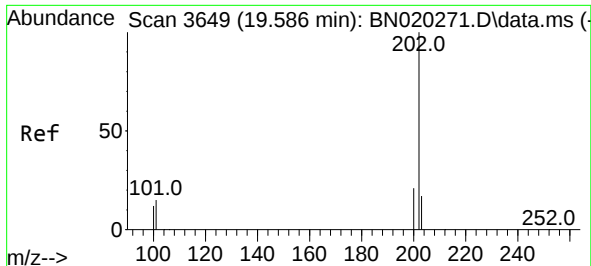

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.551 min Scan# 3641
Delta R.T. -0.032 min
Lab File: BN020293.D
Acq: 21 Jun 2022 00:30

Instrument :
BNA_N
ClientSampleId :
EW4Q8

Tgt Ion:202 Resp: 1358
Ion Ratio Lower Upper
202 100
101 166.7 12.6 19.0#
100 1219.1 10.3 15.5#

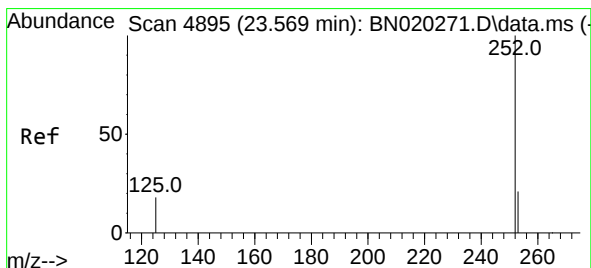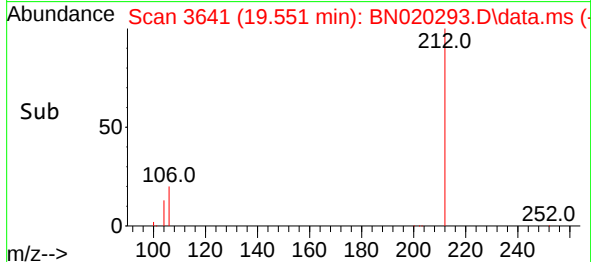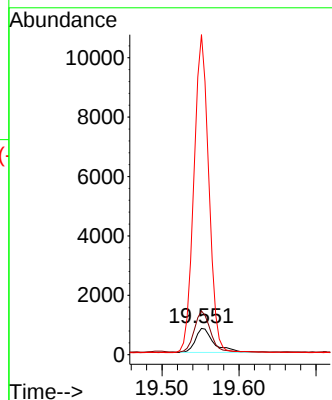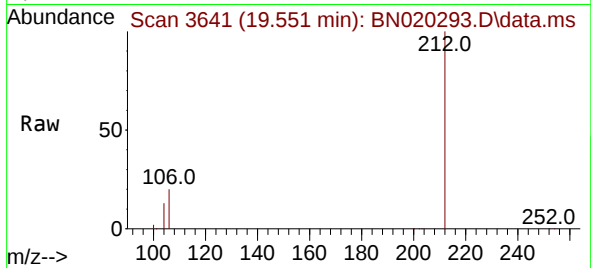

#26
Benzo(a)pyrene
Concen: 0.067 ng/ul
RT: 23.511 min Scan# 4875
Delta R.T. -0.052 min
Lab File: BN020293.D
Acq: 21 Jun 2022 00:30

Tgt Ion:252 Resp: 3585
Ion Ratio Lower Upper
252 100
253 46.7 21.7 32.5#
125 38.6 18.6 28.0#

