

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
 Data File : BN020275.D
 Acq On : 20 Jun 2022 13:04
 Operator : CG/JU
 Sample : N3294-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P9

Quant Time: Jun 21 02:37:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	716	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	2975	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.423	164	2467	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.162	188	6656	0.400	ng/ul	0.00
17) Chrysene-d12	21.355	240	8128	0.400	ng/ul	# 0.00
23) Perylene-d12	23.667	264	10542	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	3783	4.627	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.173	152	1984	0.403	ng/ul	0.00
18) Fluoranthene-d10	19.192	212	9751	0.581	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.628	128	459	0.048	ng/ul#	Qvalue 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062022\
Data File : BN020275.D
Acq On : 20 Jun 2022 13:04
Operator : CG/JU
Sample : N3294-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P9


Quant Time: Jun 21 02:37:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration

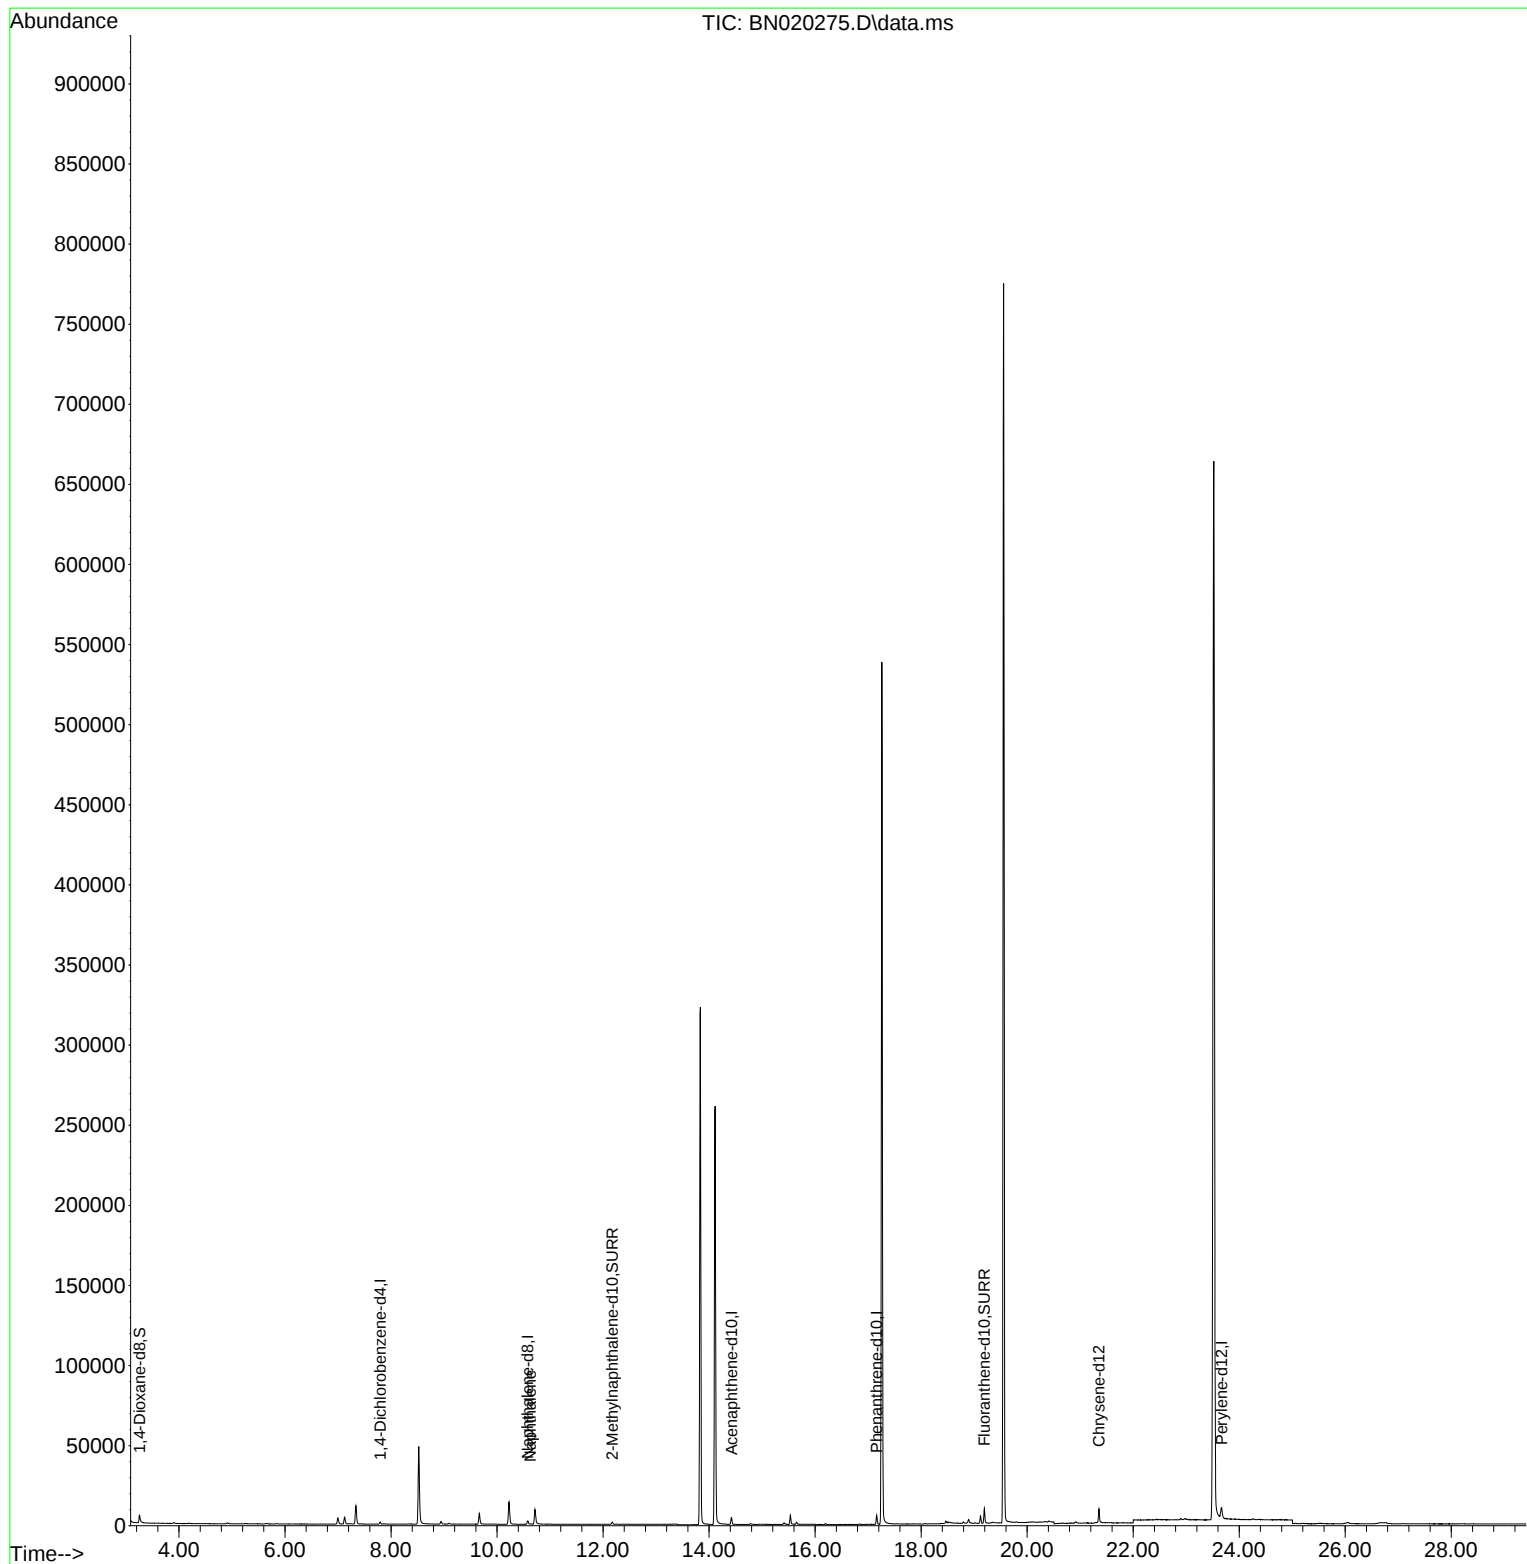

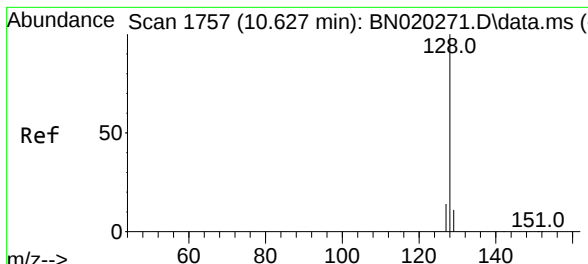

#5
 Naphthalene
 Concen: 0.048 ng/ul
 RT: 10.628 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BN020275.D
 Acq: 20 Jun 2022 13:04

Instrument :
 BNA_N
 ClientSampleId :
 EW4P9

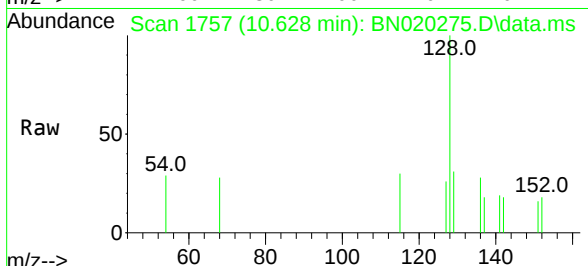

Tgt Ion:128 Resp: 459
 Ion Ratio Lower Upper
 128 100
 129 31.0 11.0 16.4#
 127 25.6 12.8 19.2#

