

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
 Data File : BN037347.D
 Acq On : 19 Jun 2025 15:36
 Operator : RC/JU
 Sample : PB166502BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK502

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN037347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	26	30	37	rVB	25097	37490	1.67%	0.163%
2	3.469	95	99	115	rBV	302696	474314	21.18%	2.059%
3	3.787	150	153	161	rVB6	6629	9547	0.43%	0.041%
4	6.134	548	552	555	rBV5	1780	2821	0.13%	0.012%
5	6.740	649	655	666	rVV	409229	630693	28.16%	2.738%
6	6.905	677	683	692	rBV	328043	494689	22.09%	2.148%
7	7.099	709	716	726	rBV	448430	704622	31.46%	3.059%
8	7.563	789	795	803	rBV	367079	567373	25.33%	2.463%
9	8.052	873	878	880	rBV4	1516	2709	0.12%	0.012%
10	8.275	909	916	929	rBV	509715	778771	34.77%	3.381%
11	8.716	984	991	1001	rBV	382851	614731	27.45%	2.669%
12	8.840	1008	1012	1016	rBV6	3964	4995	0.22%	0.022%
13	9.434	1106	1113	1123	rBV	341436	537689	24.01%	2.334%
14	9.969	1197	1204	1217	rBV	570787	912053	40.72%	3.959%
15	10.340	1260	1267	1274	rVV	422036	671573	29.99%	2.915%
16	10.481	1284	1291	1305	rBV	422367	734016	32.78%	3.187%
17	11.945	1537	1540	1545	rBV4	4185	7233	0.32%	0.031%
18	13.634	1821	1827	1839	rBV	932117	1218563	54.41%	5.290%
19	13.910	1867	1874	1889	rBV	1030586	1511137	67.48%	6.560%
20	14.216	1920	1926	1936	rVB	682536	947101	42.29%	4.112%
21	14.428	1954	1962	1976	rBV	271321	415959	18.57%	1.806%
22	15.216	2090	2096	2108	rBV	1395611	1881454	84.01%	8.168%
23	15.339	2112	2117	2128	rVV	329126	436219	19.48%	1.894%
24	15.410	2128	2129	2134	rVV2	1916	2380	0.11%	0.010%
25	15.457	2134	2137	2141	rVB3	5331	6719	0.30%	0.029%
26	16.757	2354	2358	2362	rBV2	2685	4035	0.18%	0.018%
27	16.969	2388	2394	2403	rBV2	803101	1073701	47.94%	4.661%
28	17.069	2404	2411	2423	rVV	1364567	1961383	87.58%	8.515%
29	17.539	2486	2491	2496	rBV5	1706	3403	0.15%	0.015%
30	18.669	2681	2683	2686	rBV4	1843	2403	0.11%	0.010%
31	18.892	2717	2721	2723	rBV5	1744	3090	0.14%	0.013%
32	18.933	2725	2728	2733	rVV3	15991	20319	0.91%	0.088%
33	19.004	2736	2740	2745	rVB	12477	17200	0.77%	0.075%
34	19.369	2796	2802	2813	rBV	1776561	2239542	100.00%	9.722%
35	21.198	3108	3113	3119	rBV	790663	1063029	47.47%	4.615%
36	23.851	3556	3564	3576	rBV	864927	1954121	87.26%	8.483%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
Data File : BN037347.D
Acq On : 19 Jun 2025 15:36
Operator : RC/JU
Sample : PB166502BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK502

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
Title : SVOA CALIBRATION

37	24.045	3590	3597	3610	rVB	458236	1087602	48.56%	4.722%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 23034679

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
Data File : BN037347.D
Acq On : 19 Jun 2025 15:36
Operator : RC/JU
Sample : PB166502BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

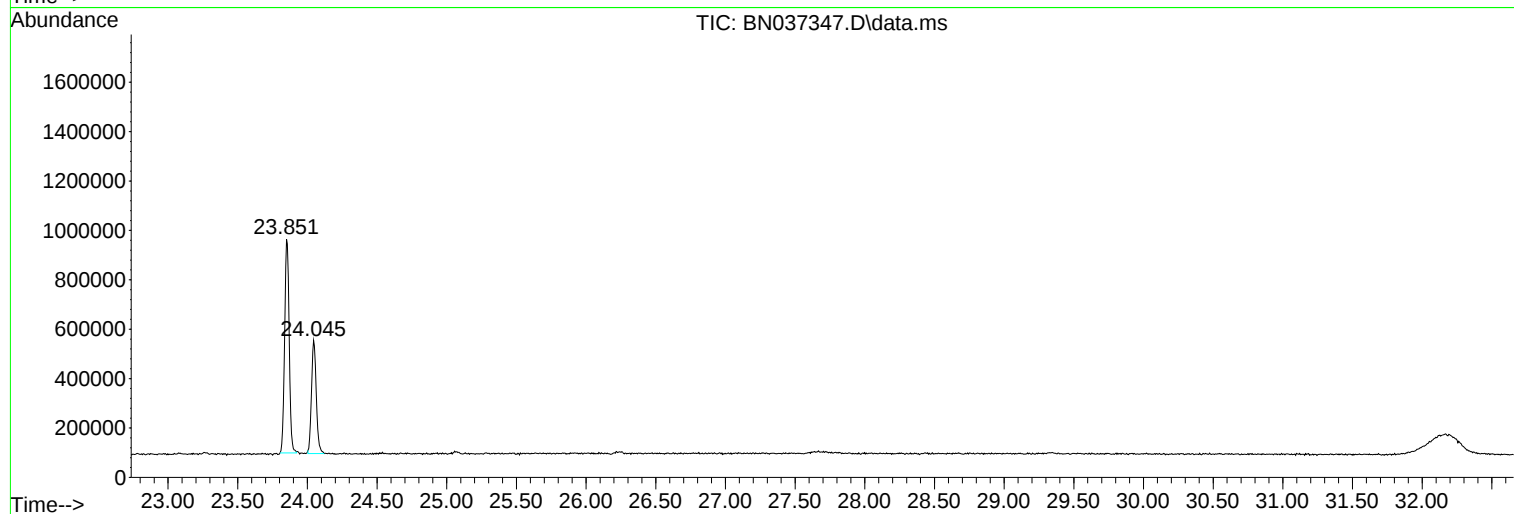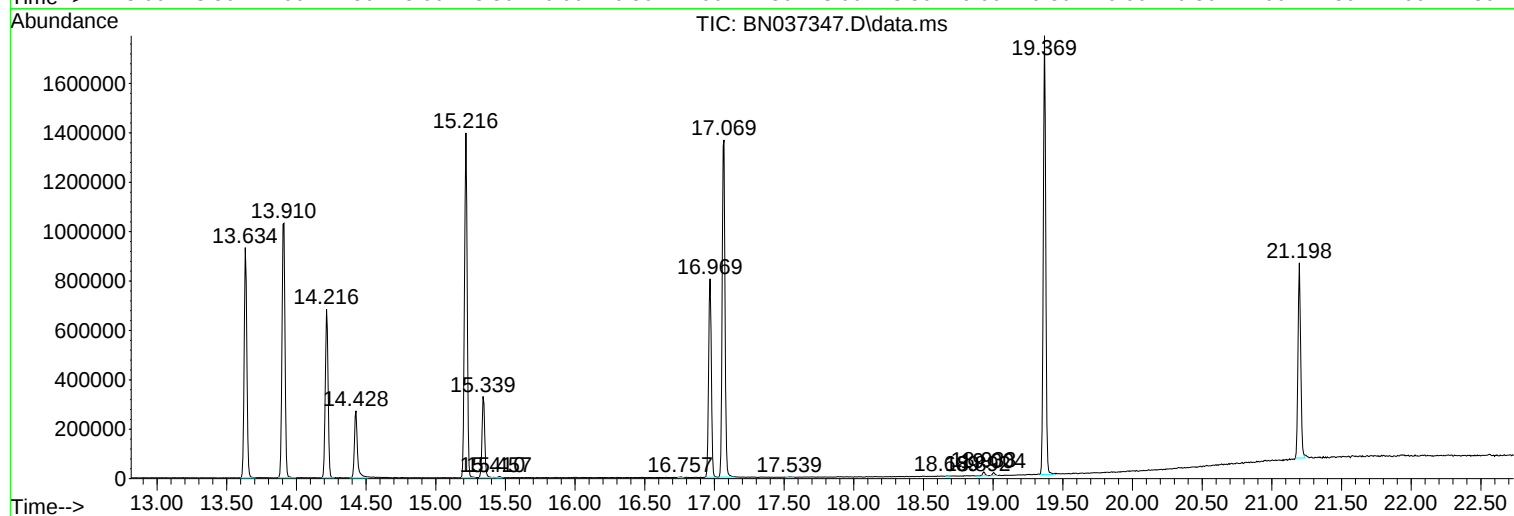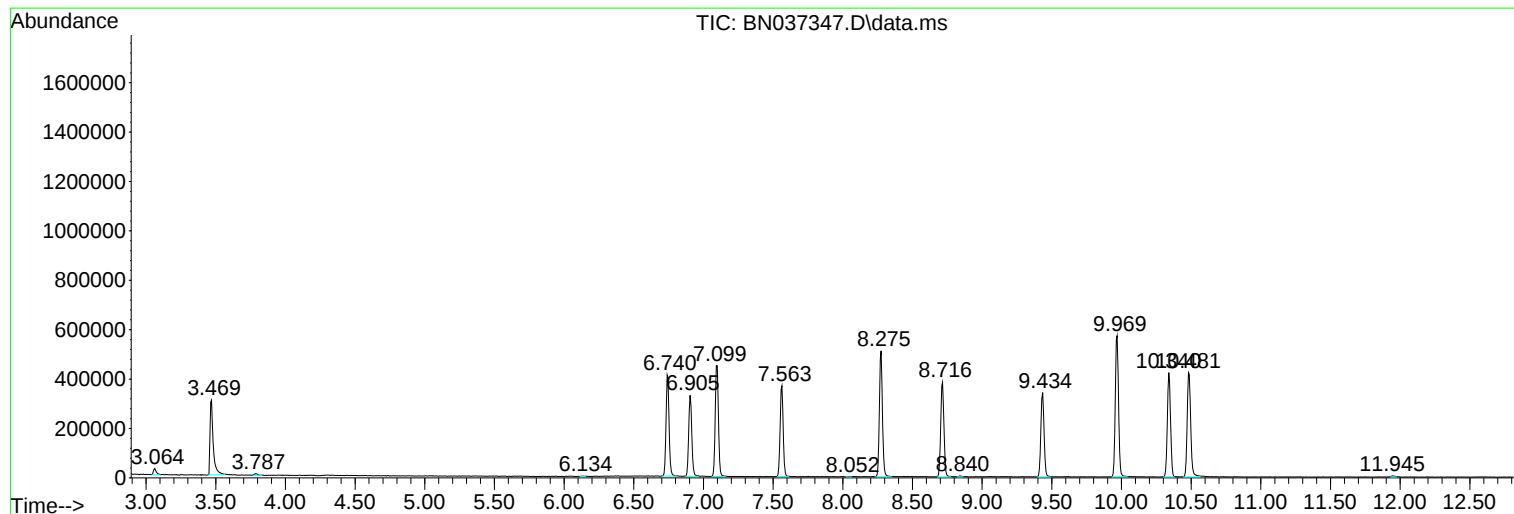

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
Data File : BN037347.D
Acq On : 19 Jun 2025 15:36
Operator : RC/JU
Sample : PB166502BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
Data File : BN037347.D
Acq On : 19 Jun 2025 15:36
Operator : RC/JU
Sample : PB166502BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc