

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
 Data File : BN037349.D
 Acq On : 19 Jun 2025 16:55
 Operator : RC/JU
 Sample : Q2318-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN037349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.011	19	21	24	rVB3	1869	1438	0.17%	0.035%
2	3.181	49	50	53	rBV3	2046	2025	0.24%	0.050%
3	3.440	92	94	96	rVB2	1395	1044	0.13%	0.026%
4	3.787	151	153	157	rVB3	3228	3629	0.44%	0.089%
5	3.864	164	166	169	rBV3	1523	1625	0.19%	0.040%
6	4.105	205	207	208	rBV	1440	882	0.11%	0.022%
7	4.558	282	284	289	rVB4	1212	1628	0.20%	0.040%
8	4.752	316	317	320	rVB2	1726	1445	0.17%	0.036%
9	4.869	334	337	339	rVB2	1004	1167	0.14%	0.029%
10	4.958	350	352	355	rVB4	1234	1230	0.15%	0.030%
11	5.058	367	369	372	rBV3	931	989	0.12%	0.024%
12	5.269	403	405	408	rVB4	798	877	0.11%	0.022%
13	5.434	432	433	434	rBV	1514	971	0.12%	0.024%
14	5.505	443	445	446	rBV2	1220	880	0.11%	0.022%
15	5.769	489	490	493	rVB3	1317	847	0.10%	0.021%
16	5.881	507	509	511	rBV2	1392	1345	0.16%	0.033%
17	5.911	511	514	515	rBV3	1388	1012	0.12%	0.025%
18	6.022	529	533	534	rBV3	1357	1828	0.22%	0.045%
19	6.199	560	563	565	rBV4	1043	1152	0.14%	0.028%
20	6.287	575	578	579	rBV3	938	994	0.12%	0.024%
21	6.552	621	623	627	rBV5	1070	1434	0.17%	0.035%
22	6.646	638	639	642	rBV3	1112	1196	0.14%	0.029%
23	6.687	642	646	647	rVB2	914	855	0.10%	0.021%
24	6.752	655	657	660	rVB4	1121	1242	0.15%	0.031%
25	6.799	662	665	669	rBV5	1283	1511	0.18%	0.037%
26	6.852	669	674	676	rVB5	1013	1333	0.16%	0.033%
27	7.058	708	709	716	rVB4	1003	1446	0.17%	0.036%
28	7.158	724	726	731	rVB4	1002	1043	0.13%	0.026%
29	7.428	770	772	773	rBV2	1255	914	0.11%	0.023%
30	7.563	789	795	803	rBV	255397	393857	47.23%	9.706%
31	8.005	866	870	874	rBV3	728	1310	0.16%	0.032%
32	8.152	890	895	897	rBV4	1137	1502	0.18%	0.037%
33	8.263	912	914	917	rVB3	853	973	0.12%	0.024%
34	8.322	920	924	928	rVB2	797	1094	0.13%	0.027%
35	9.069	1045	1051	1052	rBV2	704	1059	0.13%	0.026%
36	9.087	1052	1054	1056	rVV2	1079	1071	0.13%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
 Data File : BN037349.D
 Acq On : 19 Jun 2025 16:55
 Operator : RC/JU
 Sample : Q2318-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
 Title : SVOA CALIBRATION

37	9.134	1060	1062	1064	rVV3	1146	878	0.11%	0.022%
38	9.163	1064	1067	1069	rVB3	1248	1354	0.16%	0.033%
39	9.193	1069	1072	1075	rBV4	802	1104	0.13%	0.027%
40	9.299	1088	1090	1094	rBV2	763	892	0.11%	0.022%
41	9.522	1124	1128	1129	rBV2	996	1149	0.14%	0.028%
42	9.704	1155	1159	1160	rVB2	837	922	0.11%	0.023%
43	9.787	1170	1173	1175	rBV2	1214	1039	0.12%	0.026%
44	9.963	1201	1203	1206	rBV3	736	893	0.11%	0.022%
45	10.016	1209	1212	1214	rBV3	1097	1178	0.14%	0.029%
46	10.157	1234	1236	1240	rVB3	930	992	0.12%	0.024%
47	10.228	1247	1248	1252	rVB2	983	845	0.10%	0.021%
48	10.340	1260	1267	1276	rBV	279927	462144	55.41%	11.389%
49	10.440	1282	1284	1289	rVB5	873	1274	0.15%	0.031%
50	10.610	1311	1313	1315	rBV2	1097	1015	0.12%	0.025%
51	10.657	1319	1321	1324	rVB2	922	854	0.10%	0.021%
52	10.769	1337	1340	1341	rBV2	948	961	0.12%	0.024%
53	10.822	1345	1349	1351	rVV4	844	898	0.11%	0.022%
54	11.863	1522	1526	1530	rVB4	642	1166	0.14%	0.029%
55	11.910	1530	1534	1535	rVB2	1083	1022	0.12%	0.025%
56	12.157	1573	1576	1578	rBV3	787	903	0.11%	0.022%
57	12.287	1597	1598	1603	rBV	727	901	0.11%	0.022%
58	12.593	1647	1650	1653	rBV2	819	850	0.10%	0.021%
59	12.851	1691	1694	1696	rBV	915	1059	0.13%	0.026%
60	13.657	1827	1831	1833	rBV3	673	982	0.12%	0.024%
61	13.992	1886	1888	1892	rBV2	781	952	0.11%	0.023%
62	14.145	1911	1914	1917	rBV2	630	836	0.10%	0.021%
63	14.216	1920	1926	1938	rVV	466495	674090	80.83%	16.612%
64	14.310	1940	1942	1944	rVB2	1563	1307	0.16%	0.032%
65	14.604	1991	1992	1996	rBV3	806	867	0.10%	0.021%
66	15.222	2095	2097	2102	rVV3	919	1518	0.18%	0.037%
67	15.645	2164	2169	2170	rBV3	600	930	0.11%	0.023%
68	15.763	2186	2189	2192	rVB4	891	1001	0.12%	0.025%
69	15.928	2214	2217	2218	rBV2	1132	1051	0.13%	0.026%
70	15.986	2222	2227	2230	rBV4	910	1423	0.17%	0.035%
71	16.251	2269	2272	2275	rVB2	837	1009	0.12%	0.025%
72	16.286	2275	2278	2281	rBV3	839	1011	0.12%	0.025%
73	16.345	2285	2288	2290	rBV3	919	1081	0.13%	0.027%
74	16.604	2329	2332	2336	rVB2	852	942	0.11%	0.023%
75	16.745	2353	2356	2357	rBV2	1519	1401	0.17%	0.035%
76	16.763	2357	2359	2361	rVB2	1121	1127	0.14%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
 Data File : BN037349.D
 Acq On : 19 Jun 2025 16:55
 Operator : RC/JU
 Sample : Q2318-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
 Title : SVOA CALIBRATION

77	16.851	2370	2374	2376	rVB2	1088	1533	0.18%	0.038%
78	16.969	2388	2394	2407	rBV	562259	759380	91.05%	18.713%
79	17.069	2407	2411	2415	rVV5	2917	4631	0.56%	0.114%
80	17.175	2426	2429	2434	rBV4	907	1805	0.22%	0.044%
81	17.333	2455	2456	2458	rBV2	1196	948	0.11%	0.023%
82	17.363	2458	2461	2464	rVV4	964	1481	0.18%	0.036%
83	17.451	2474	2476	2479	rBV3	947	1102	0.13%	0.027%
84	17.498	2482	2484	2487	rVB3	1061	990	0.12%	0.024%
85	17.563	2491	2495	2497	rBV5	1182	1767	0.21%	0.044%
86	17.880	2547	2549	2551	rBV2	819	873	0.10%	0.022%
87	17.963	2562	2563	2566	rVB2	1307	1085	0.13%	0.027%
88	18.022	2570	2573	2576	rBV4	796	1182	0.14%	0.029%
89	18.416	2638	2640	2642	rVB2	1493	1061	0.13%	0.026%
90	18.433	2642	2643	2646	rBV3	1765	1603	0.19%	0.040%
91	18.598	2668	2671	2672	rBV3	971	1108	0.13%	0.027%
92	18.628	2674	2676	2678	rBV3	1064	1171	0.14%	0.029%
93	18.733	2692	2694	2696	rVB2	1443	1361	0.16%	0.034%
94	18.769	2696	2700	2701	rBV4	1348	1772	0.21%	0.044%
95	19.298	2789	2790	2792	rBV2	1699	1346	0.16%	0.033%
96	19.380	2801	2804	2805	rBV3	1686	1716	0.21%	0.042%
97	21.198	3108	3113	3127	rBV	610979	821365	98.49%	20.241%
98	24.051	3589	3598	3612	rBV2	352154	833986	100.00%	20.552%




Sum of corrected areas: 4057935

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
Data File : BN037349.D
Acq On : 19 Jun 2025 16:55
Operator : RC/JU
Sample : Q2318-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

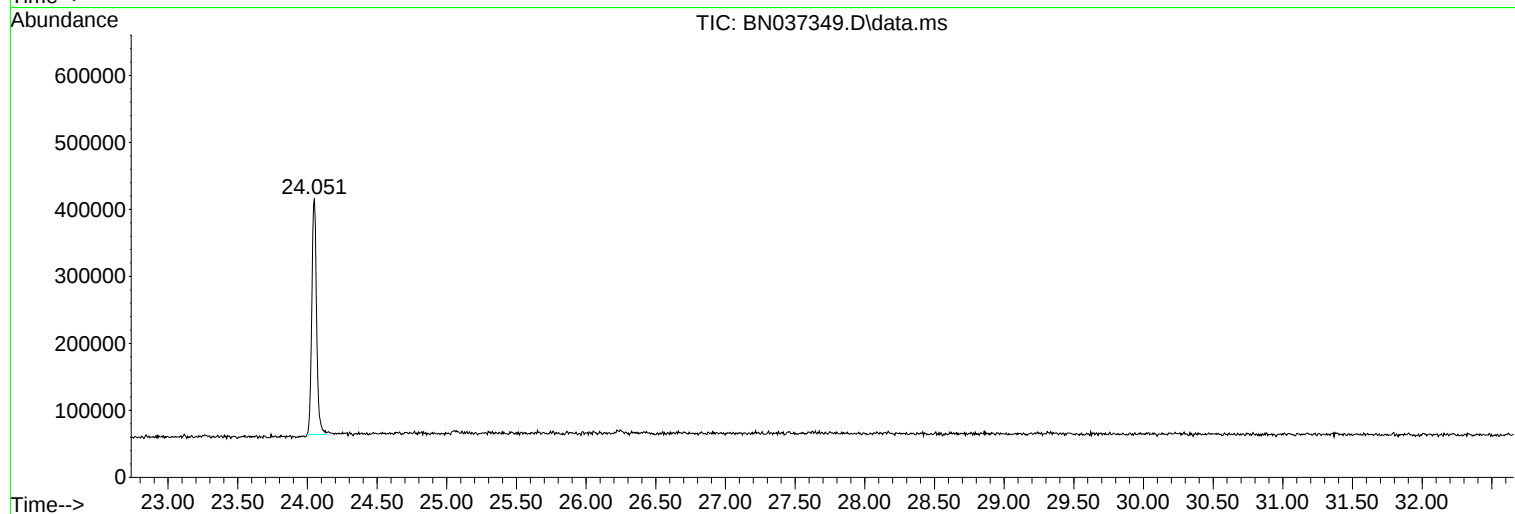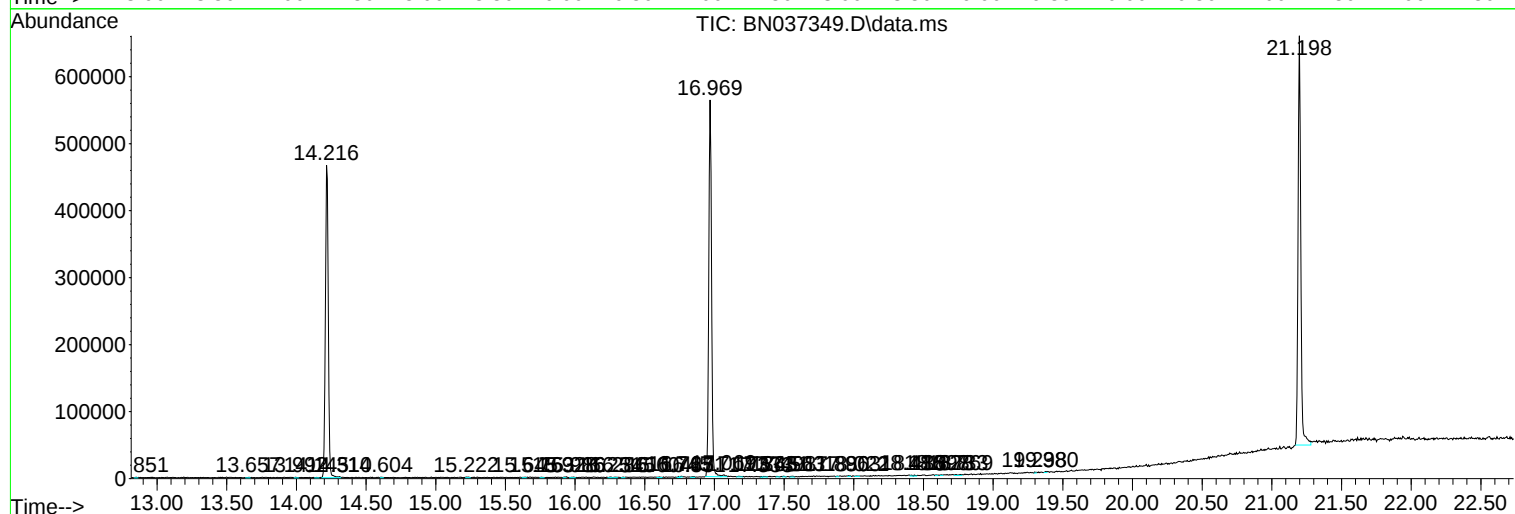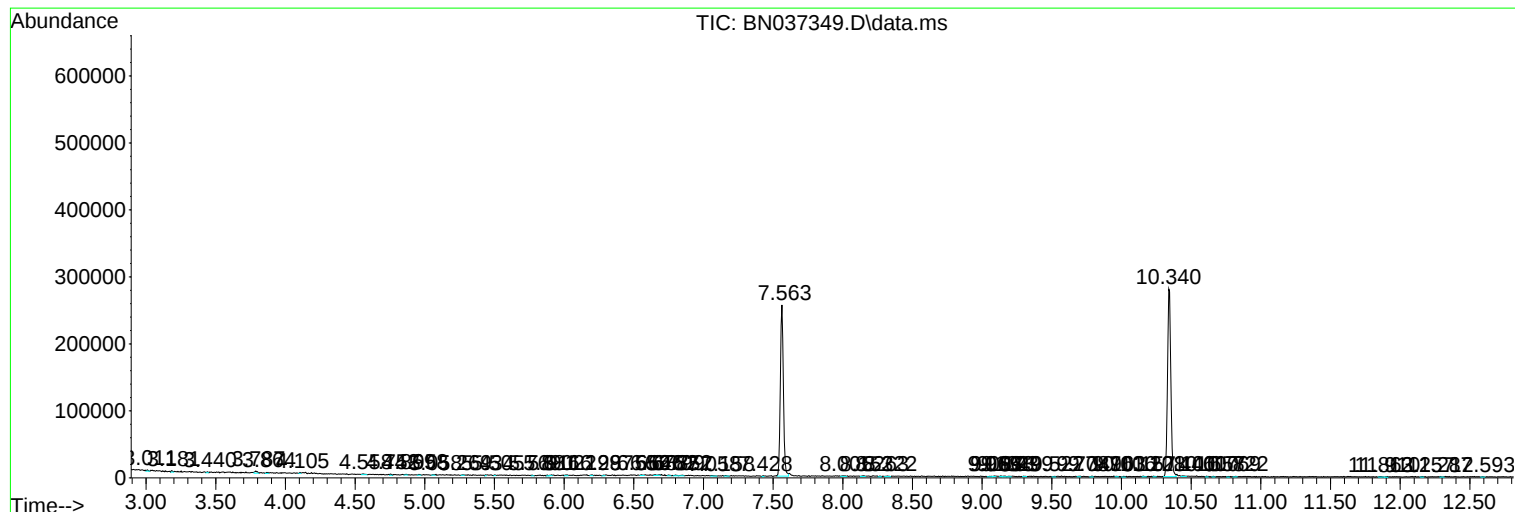

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
Data File : BN037349.D
Acq On : 19 Jun 2025 16:55
Operator : RC/JU
Sample : Q2318-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
Data File : BN037349.D
Acq On : 19 Jun 2025 16:55
Operator : RC/JU
Sample : Q2318-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc