


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062025\
Data File : BN037339.D
Acq On : 19 Jun 2025 10:06
Operator : RC/JU
Sample : DFTPP377
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP377

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
Title : SVOA CALIBRATION
Last Update : Thu Jun 19 14:59:41 2025

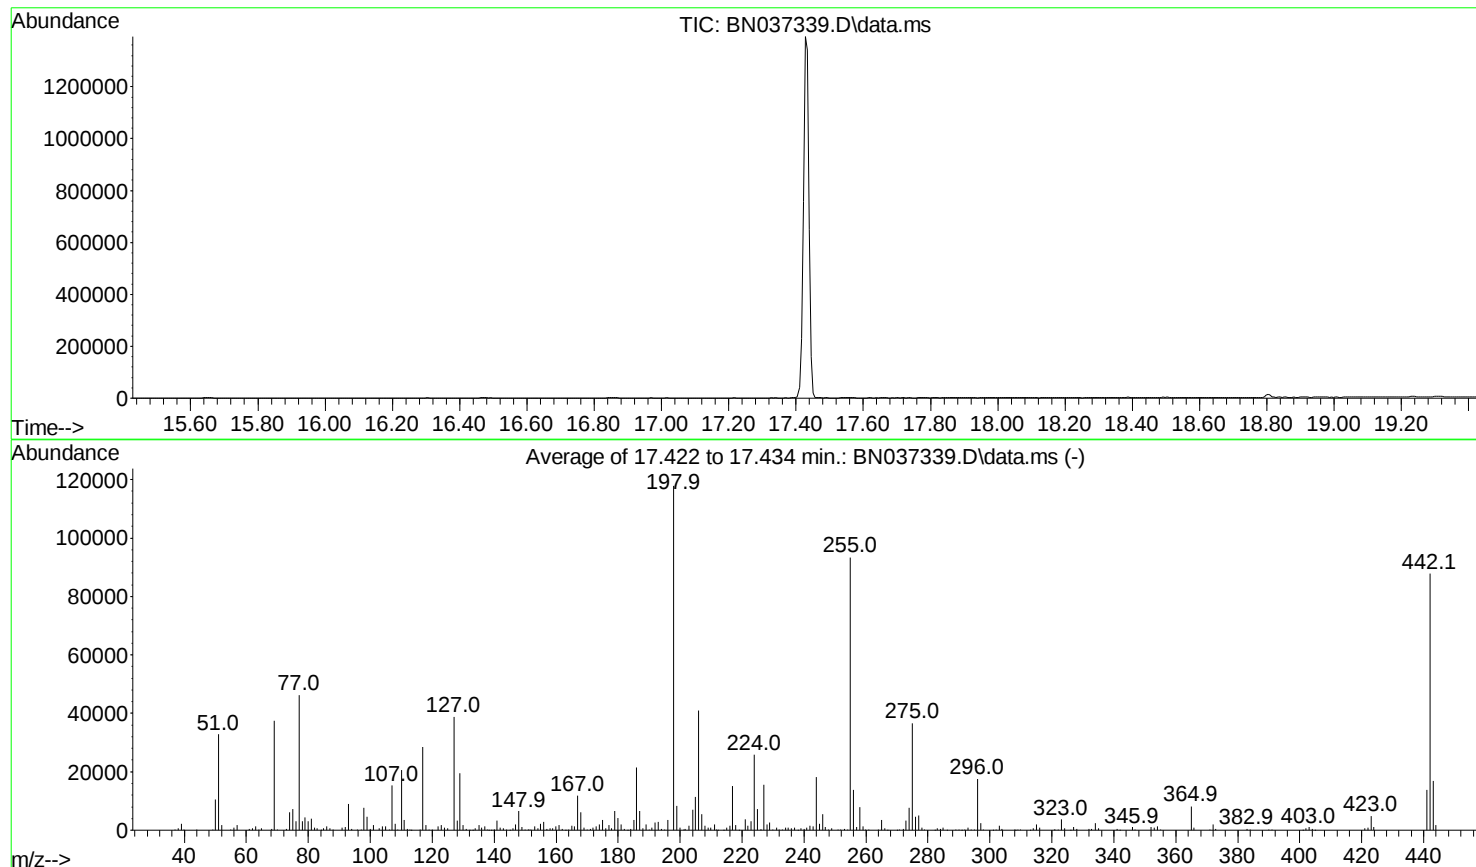

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2466

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	27.8	32803	PASS
68	69	0.00	2	1.3	487	PASS
69	198	0.00	100	31.7	37368	PASS
70	69	0.00	2	0.7	258	PASS
127	198	10	80	32.9	38832	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	117877	PASS
199	198	5	9	7.0	8251	PASS
275	198	10	60	31.1	36635	PASS
365	198	1	100	6.9	8159	PASS
441	198	0.01	100	11.7	13803	PASS
442	198	50	100	74.5	87765	PASS
443	442	15	24	19.2	16841	PASS