
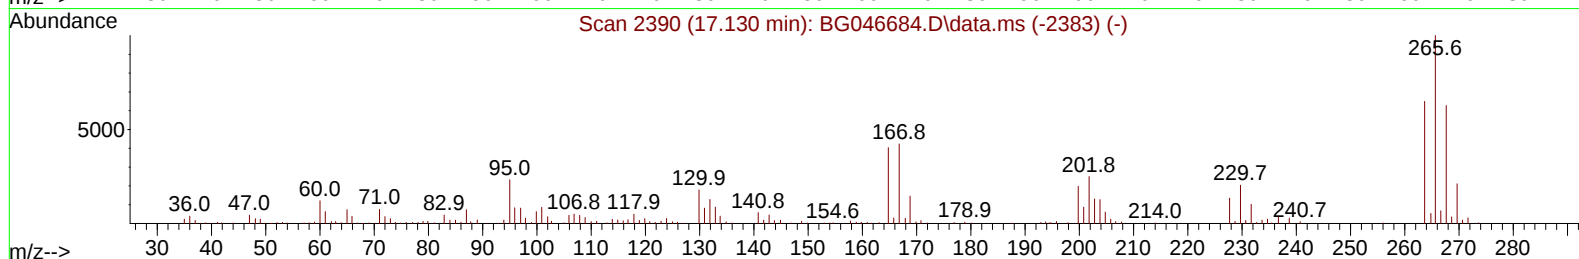
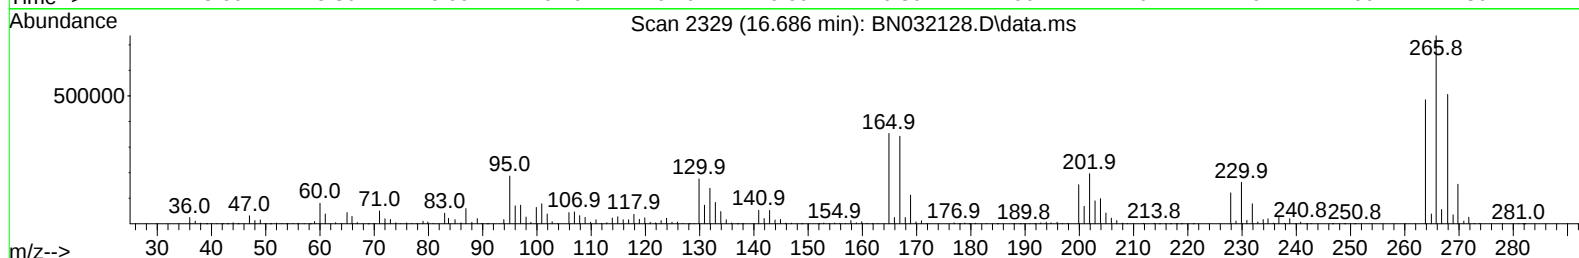


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032128.D
Acq On : 21 Jun 2024 12:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 13:37:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

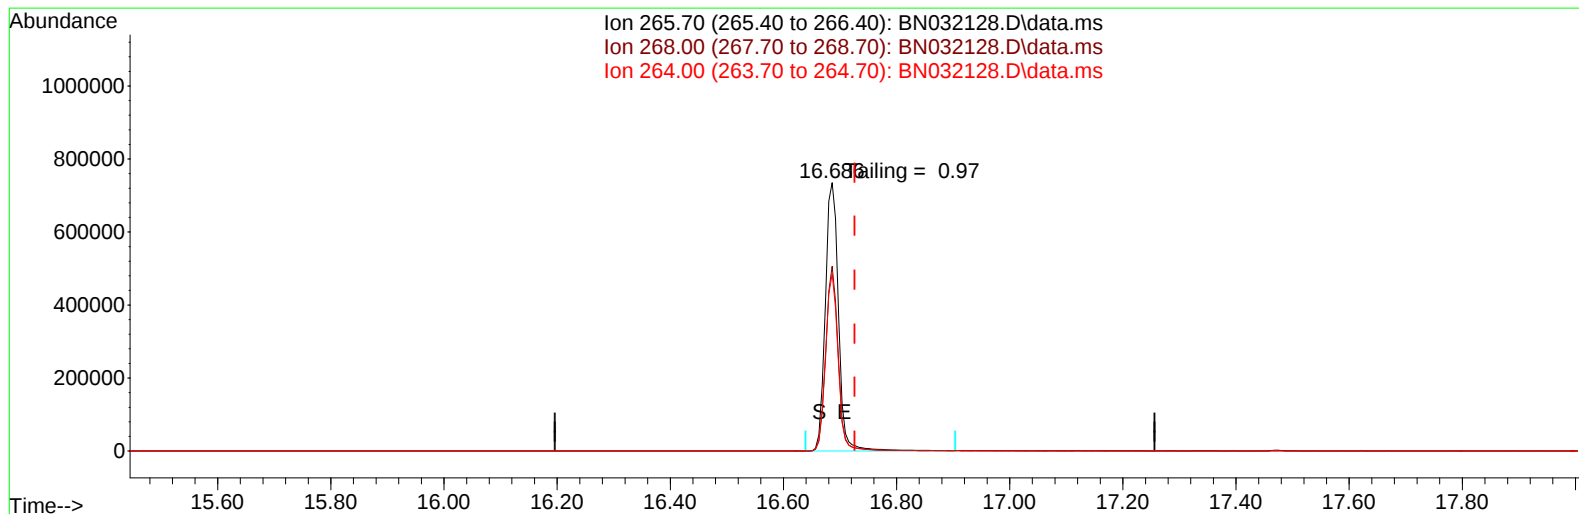

TIC: BN032128.D\data.ms

(70) Pentachlorophenol (C)




16.686min (-0.040) 25982.85 ng

response 1195506

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.82
264.00	61.60	66.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032128.D
Acq On : 21 Jun 2024 12:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 13:37:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

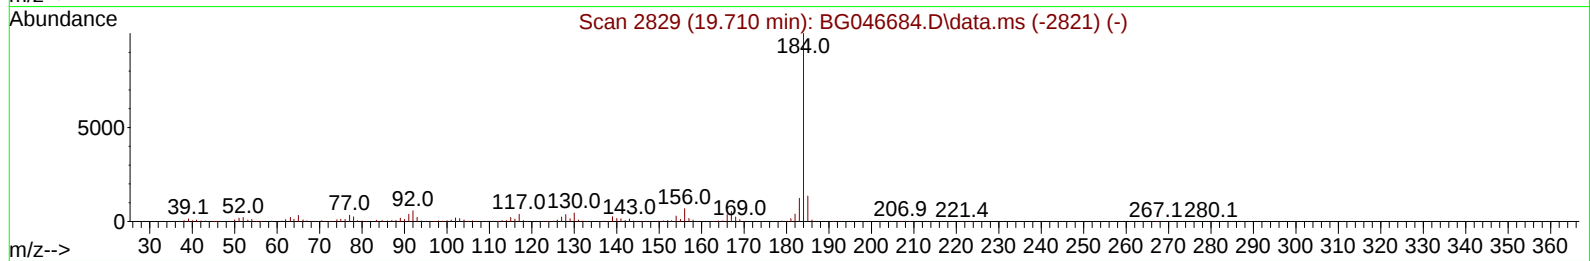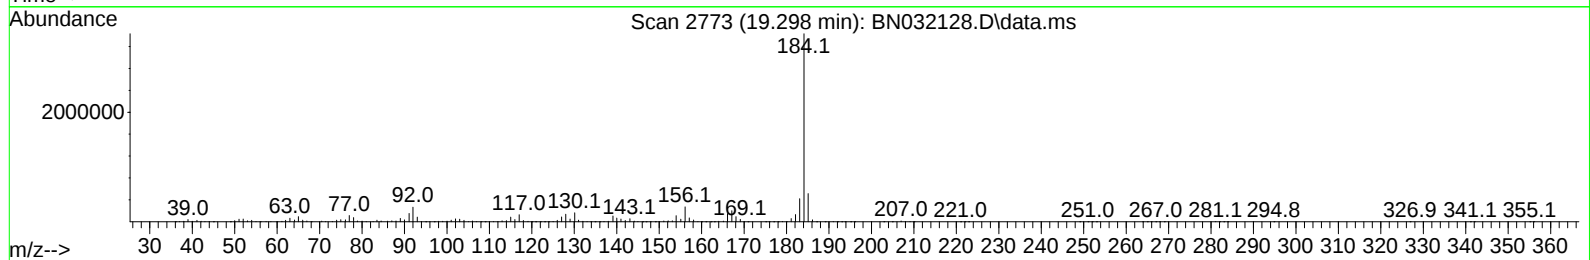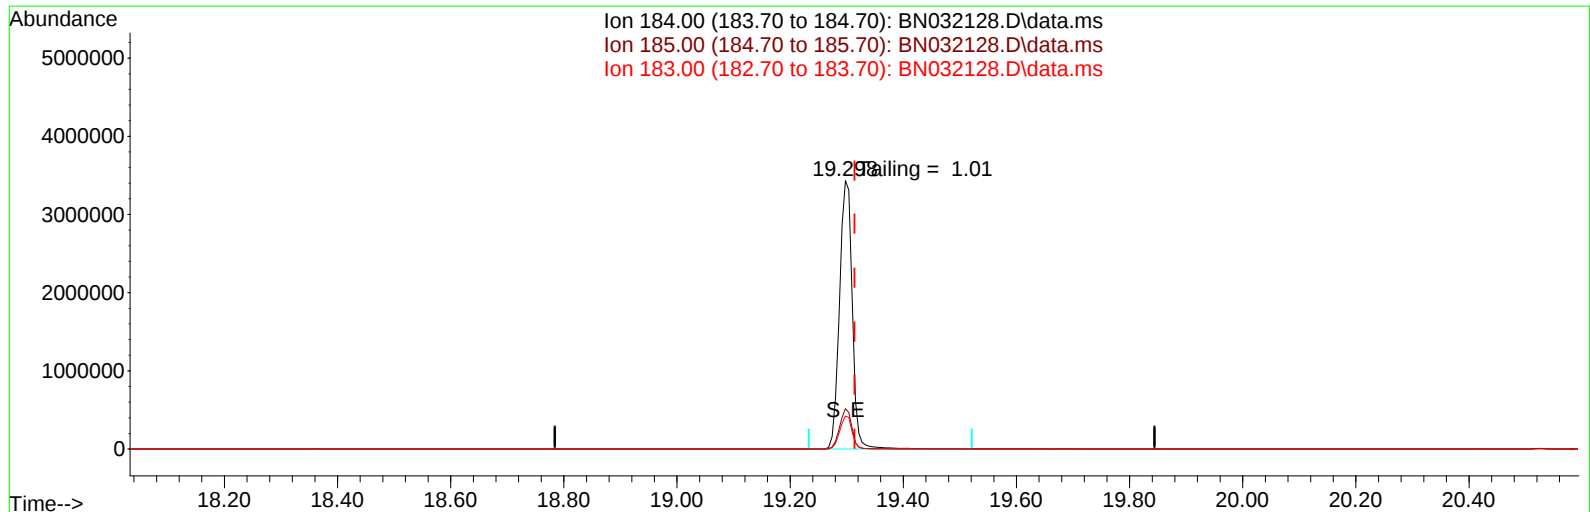

TIC: BN032128.D\data.ms

(77) Benzidine**19.298min (-0.016) 1367725.80 ng****response 5396564**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.01
183.00	13.20	12.28
0.00	0.00	0.00