
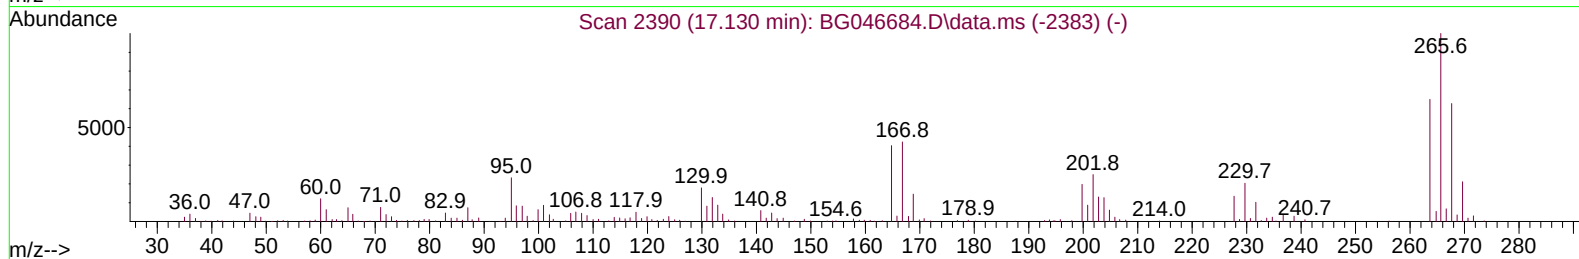
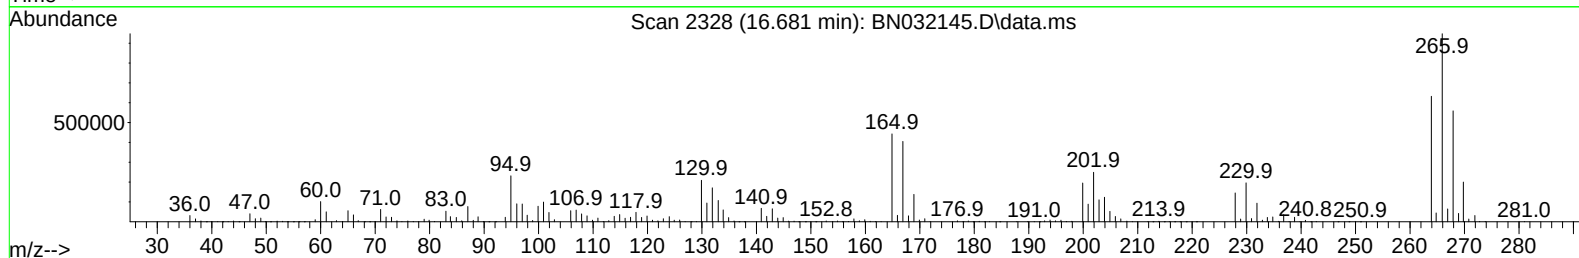


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032145.D
Acq On : 22 Jun 2024 00:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Jun 22 01:23:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

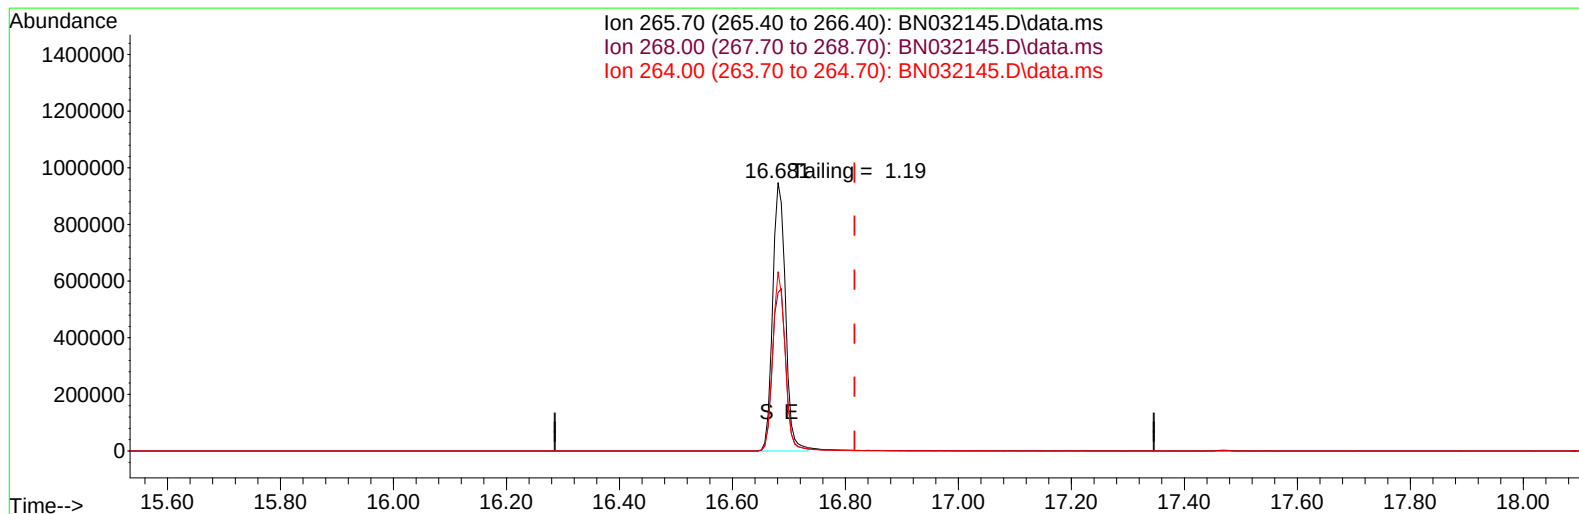

TIC: BN032145.D\data.ms

(70) Pentachlorophenol (C)




16.681min (-0.135) 27633.01 ng

response 1521902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.98
264.00	61.60	66.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032145.D
Acq On : 22 Jun 2024 00:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Jun 22 01:23:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

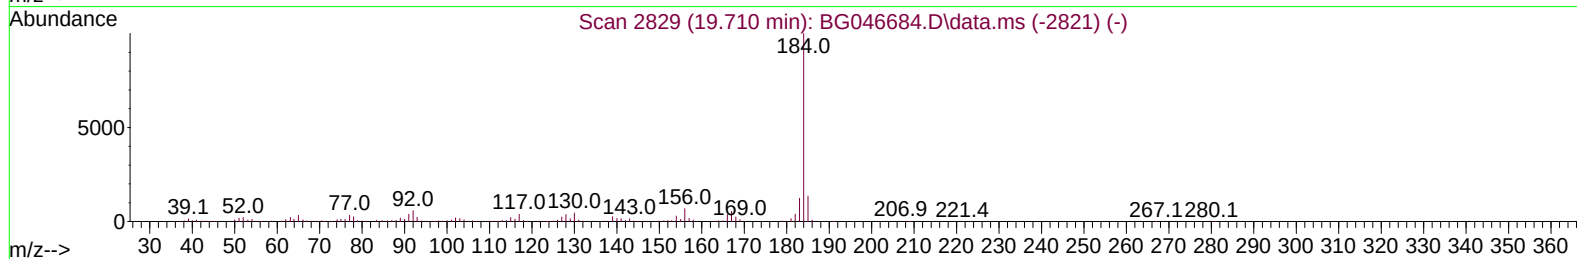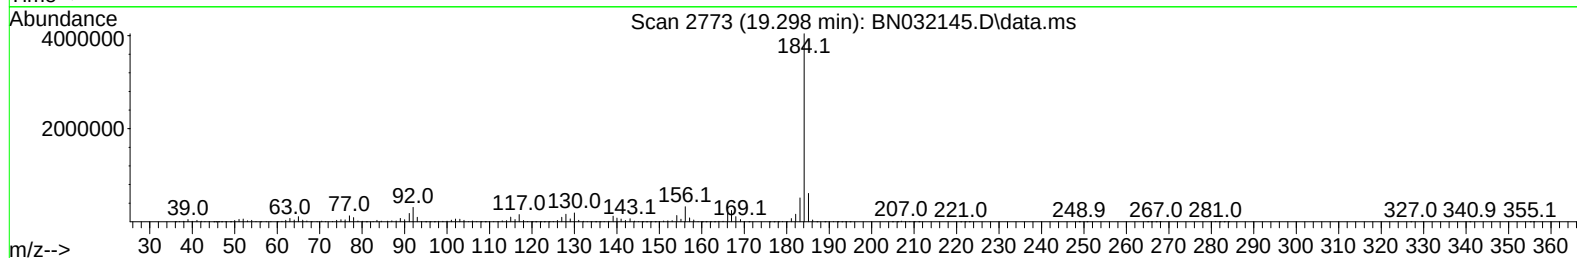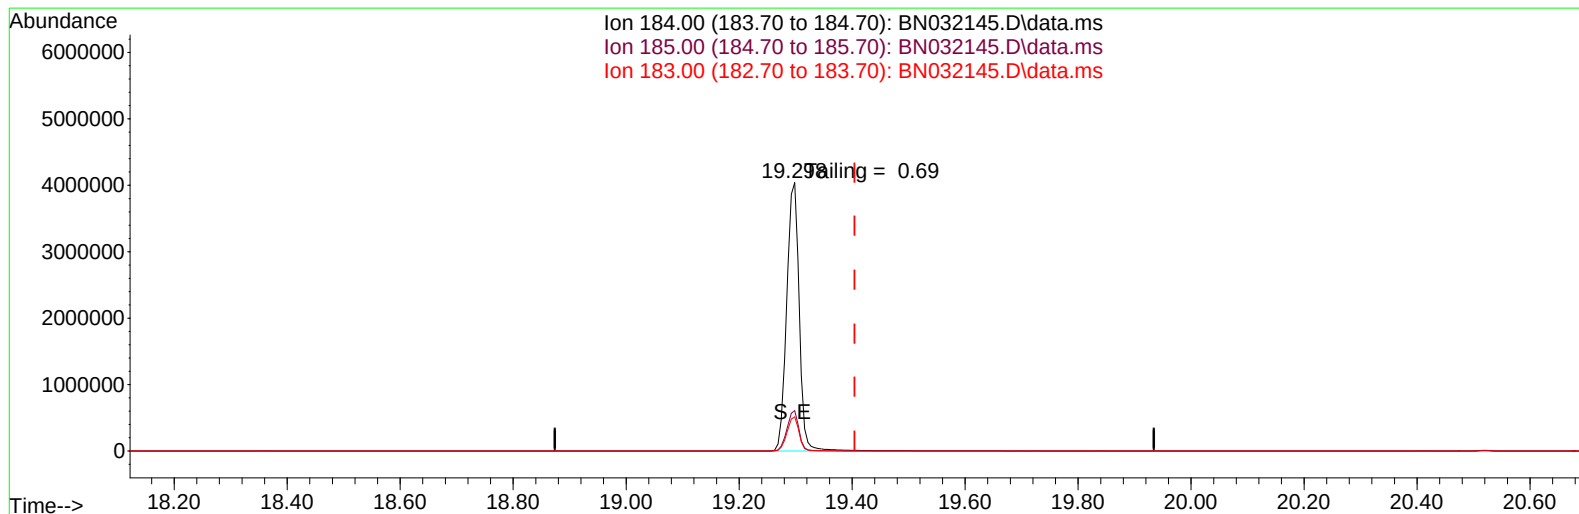

TIC: BN032145.D\data.ms

(77) Benzidine

19.298min (-0.106) 0.00 ng

response 6231428

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.04
183.00	13.20	12.72
0.00	0.00	0.00